

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023615.D
 Acq On : 18 Nov 2021 19:40
 Operator : SY/MD
 Sample : M4694-09DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4672DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	41	50	63	rBV	88840	79980	22.33%	2.335%
2	1.307	75	83	92	rBV2	69907	72598	20.27%	2.120%
3	1.568	156	164	175	rVB	47223	53989	15.08%	1.576%
4	2.108	321	332	347	rVB	97948	140428	39.21%	4.100%
5	2.506	448	456	467	rVB2	4734	7860	2.19%	0.230%
6	2.767	525	537	553	rBV3	22304	44762	12.50%	1.307%
7	3.912	878	893	923	rBV2	119584	336636	94.00%	9.830%
8	4.349	1014	1029	1053	rBV2	67656	166907	46.61%	4.874%
9	5.050	1229	1247	1273	rBV3	142068	358111	100.00%	10.457%
10	5.619	1413	1424	1446	rBV	123690	252436	70.49%	7.371%
11	5.918	1506	1517	1536	rBV	57370	117661	32.86%	3.436%
12	6.072	1548	1565	1590	rBV	82029	170000	47.47%	4.964%
13	6.989	1841	1850	1869	rBV	39264	73332	20.48%	2.141%
14	7.317	1941	1952	1971	rBV	160375	283160	79.07%	8.268%
15	7.625	2039	2048	2069	rBV	22501	42164	11.77%	1.231%
16	8.091	2183	2193	2228	rBV	127976	288157	80.47%	8.414%
17	8.853	2417	2430	2455	rBV	191519	316053	88.26%	9.229%
18	10.217	2843	2854	2875	rVB2	58445	93229	26.03%	2.722%
19	11.249	3165	3175	3196	rBV	179154	279133	77.95%	8.151%
20	11.625	3280	3292	3308	rBV	156693	248060	69.27%	7.243%

Sum of corrected areas: 3424656

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023615.D
Acq On : 18 Nov 2021 19:40
Operator : SY/MD
Sample : M4694-09DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4672DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.201	1.58 ug/L	79980	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methyl nitrite	61	CH3NO2	000624-91-9	5
2			o-Ethylhydroxylamine	61	C2H7NO	000624-86-2	4
3			Methyl formate	60	C2H4O2	000107-31-3	4
4			Methanamine, N-methoxy-	61	C2H7NO	001117-97-1	4
5			Cyanogen chloride	61	CClN	000506-77-4	4

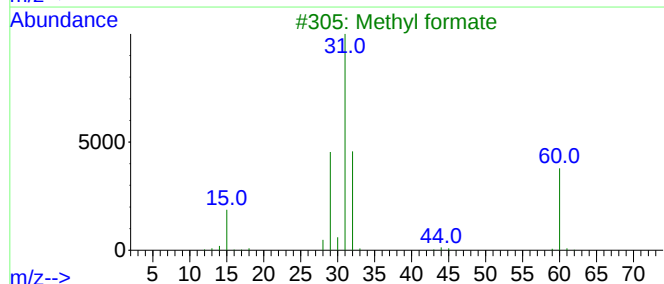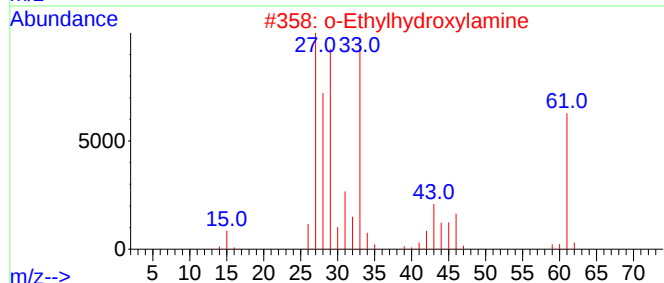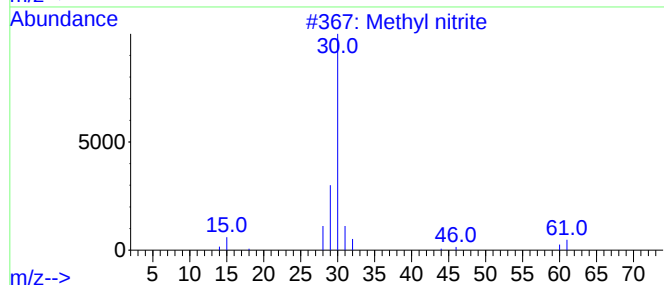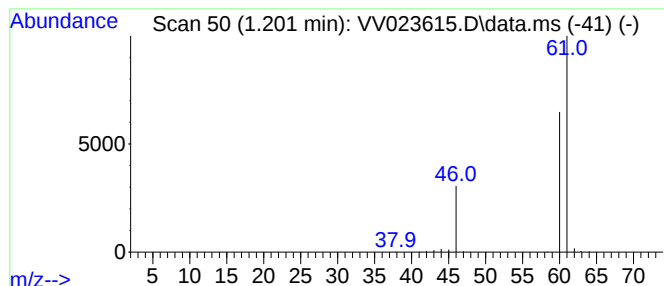

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023615.D
Acq On : 18 Nov 2021 19:40
Operator : SY/MD
Sample : M4694-09DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4672DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.201	1.6	ug/L	79980	1	5.619	252436	5.0