

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023616.D
 Acq On : 18 Nov 2021 20:04
 Operator : SY/MD
 Sample : M4694-10DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4683DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023616.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.195	42	48	57	rBV	77603	64802	17.97%	1.957%
2	1.297	73	80	92	rBV2	62588	66195	18.36%	1.999%
3	1.564	155	163	174	rVB	45226	50740	14.07%	1.533%
4	2.108	322	332	347	rBV	91400	129688	35.96%	3.917%
5	2.506	445	456	463	rBV8	3446	6293	1.74%	0.190%
6	2.757	524	534	540	rBV2	17327	33781	9.37%	1.020%
7	3.902	874	890	904	rBV	113634	287049	79.60%	8.671%
8	4.346	1010	1028	1052	rVB2	67309	170989	47.41%	5.165%
9	5.043	1231	1245	1275	rBV3	160154	360635	100.00%	10.893%
10	5.622	1412	1425	1445	rBV	130537	262039	72.66%	7.915%
11	5.921	1505	1518	1541	rBV	60894	129965	36.04%	3.926%
12	6.091	1557	1571	1589	rBV2	83201	169198	46.92%	5.111%
13	7.001	1841	1854	1873	rBV	38175	70625	19.58%	2.133%
14	7.326	1940	1955	1975	rBV	156744	273749	75.91%	8.269%
15	7.635	2041	2051	2067	rBV2	22720	40515	11.23%	1.224%
16	8.107	2186	2198	2232	rBV	146044	281995	78.19%	8.518%
17	8.857	2419	2431	2450	rBV	192583	312074	86.53%	9.426%
18	10.220	2841	2855	2866	rBV	57243	91566	25.39%	2.766%
19	11.249	3165	3175	3200	rBV	176984	274750	76.19%	8.299%
20	11.625	3280	3292	3316	rBV	149089	233973	64.88%	7.067%

Sum of corrected areas: 3310621

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023616.D
Acq On : 18 Nov 2021 20:04
Operator : SY/MD
Sample : M4694-10DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4683DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.195	1.24 ug/L	64802	1,4-Difluorobenzene	5.622

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethyne, chloro-	60	C2HCl	000593-63-5	5
2			Methyl nitrite	61	CH3NO2	000624-91-9	5
3			o-Ethylhydroxylamine	61	C2H7NO	000624-86-2	4
4			Thiirane	60	C2H4S	000420-12-2	4
5			Methanamine, N-methoxy-	61	C2H7NO	001117-97-1	4

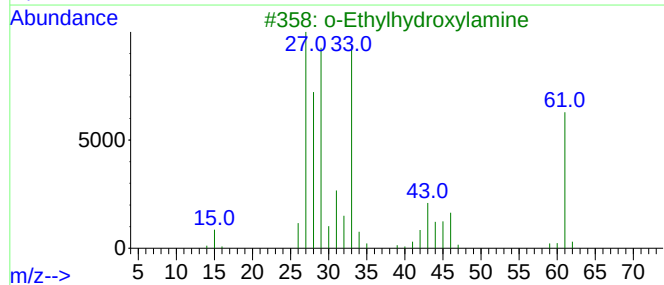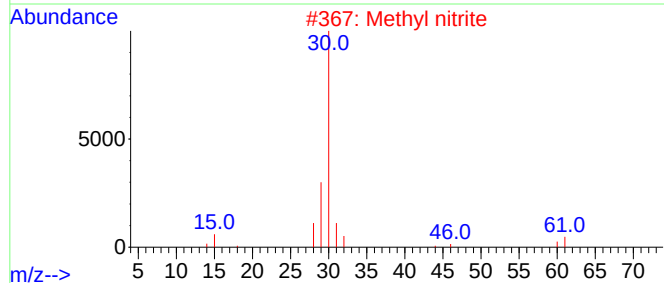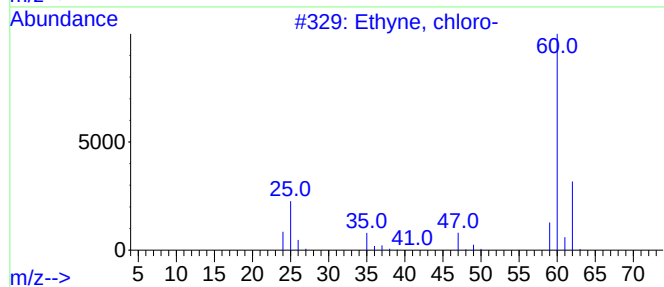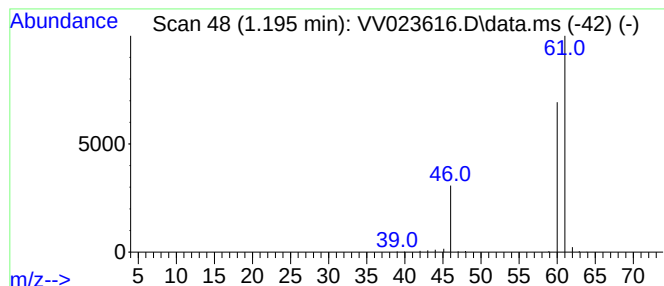

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023616.D
Acq On : 18 Nov 2021 20:04
Operator : SY/MD
Sample : M4694-10DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4683DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.195	1.2	ug/L	64802	1	5.622	262039	5.0