

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023622.D
 Acq On : 18 Nov 2021 22:27
 Operator : SY/MD
 Sample : M4706-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AA9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023622.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	57	62	71	rVB	6110	7116	2.16%	0.259%
2	1.304	76	82	92	rVB	51445	51420	15.64%	1.871%
3	1.568	157	164	173	rBV	46726	50234	15.28%	1.828%
4	2.108	319	332	347	rBV	88082	123769	37.65%	4.504%
5	3.912	879	893	913	rBV3	18714	66840	20.33%	2.433%
6	4.352	1015	1030	1064	rVB3	53971	157879	48.02%	5.746%
7	5.050	1231	1247	1274	rBV4	131614	328747	100.00%	11.965%
8	5.619	1412	1424	1445	rBV	123001	250150	76.09%	9.104%
9	6.072	1552	1565	1589	rBV2	74053	155457	47.29%	5.658%
10	6.989	1840	1850	1865	rBV2	33856	63966	19.46%	2.328%
11	7.317	1942	1952	1971	rBV	149559	260918	79.37%	9.496%
12	7.628	2040	2049	2070	rBV	20807	38547	11.73%	1.403%
13	7.976	2152	2157	2167	rVB5	2211	3591	1.09%	0.131%
14	8.091	2184	2193	2235	rBV	105905	267297	81.31%	9.728%
15	8.854	2419	2430	2456	rBV	195864	321478	97.79%	11.700%
16	10.217	2843	2854	2873	rVB2	53276	86524	26.32%	3.149%
17	10.381	2898	2905	2915	rVB4	2280	3452	1.05%	0.126%
18	11.249	3164	3175	3196	rBV	178431	277351	84.37%	10.094%
19	11.625	3280	3292	3310	rBV	146577	232947	70.86%	8.478%




Sum of corrected areas: 2747683

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023622.D
Acq On : 18 Nov 2021 22:27
Operator : SY/MD
Sample : M4706-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

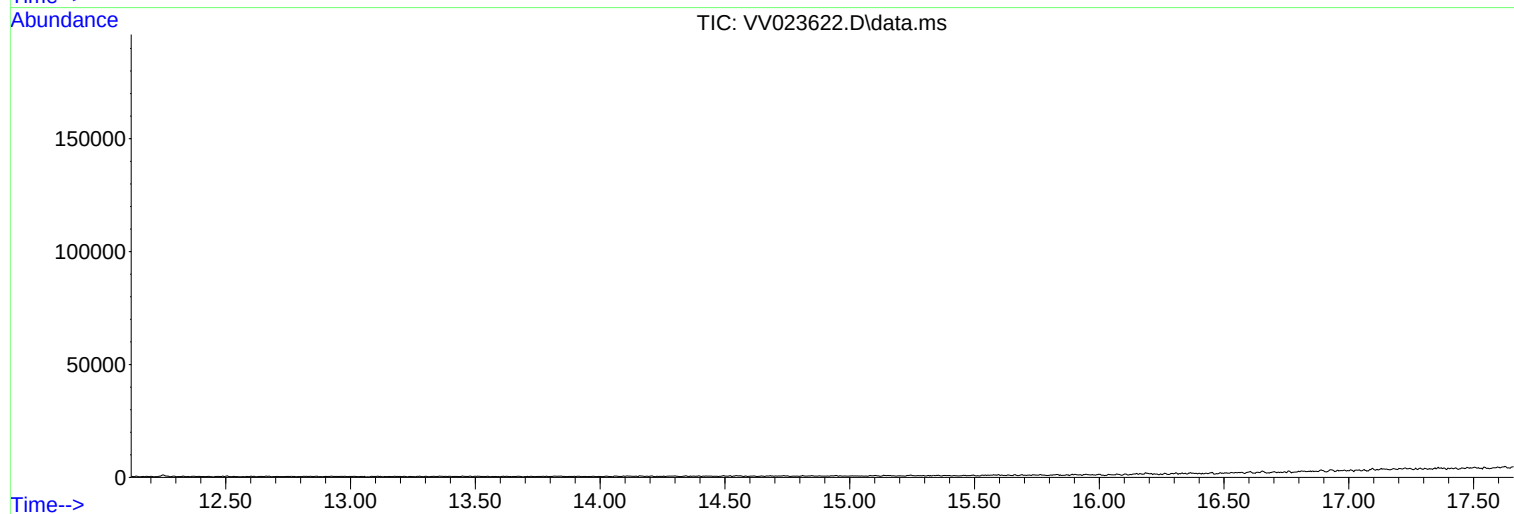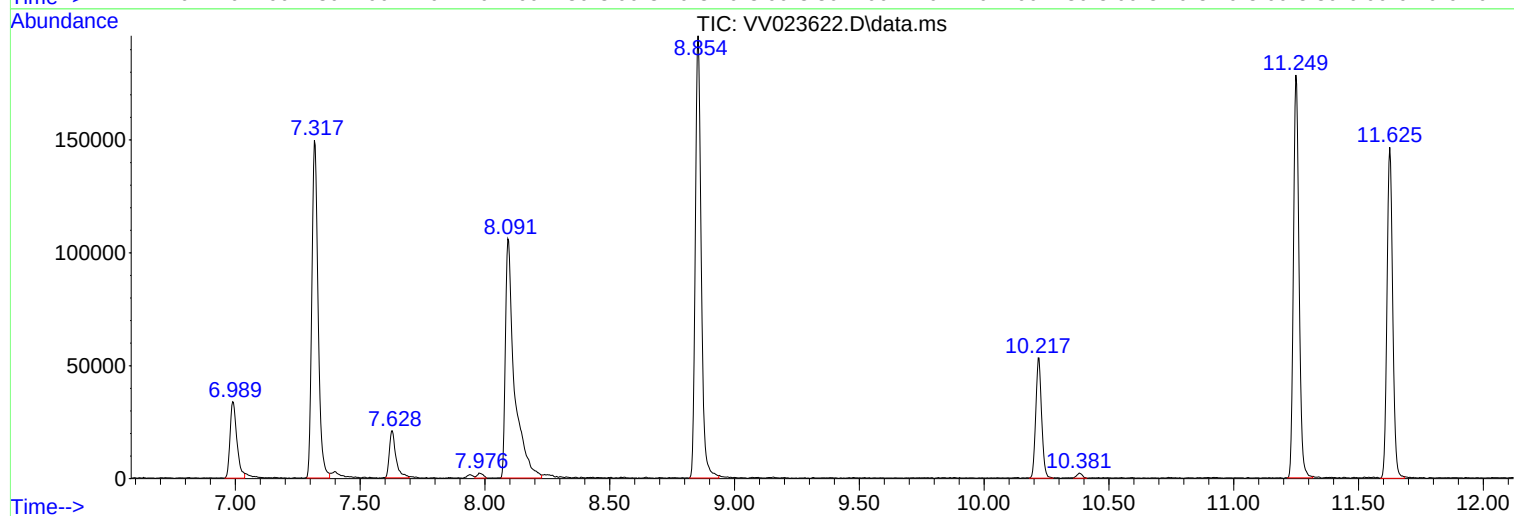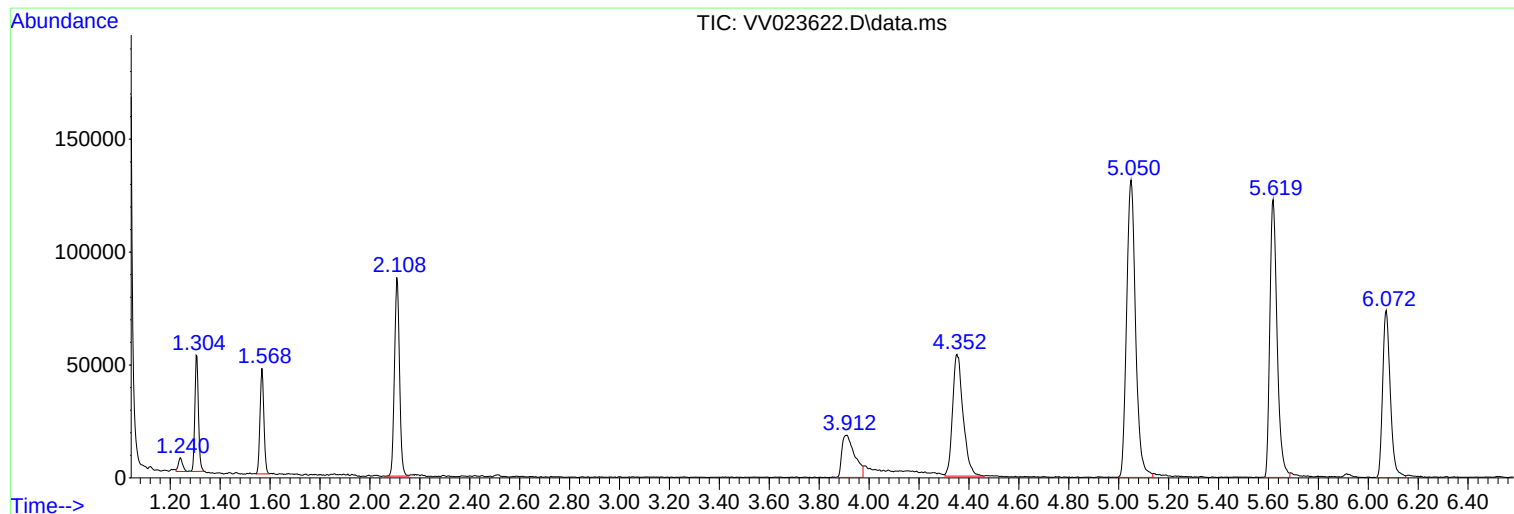

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023622.D
Acq On : 18 Nov 2021 22:27
Operator : SY/MD
Sample : M4706-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023622.D
Acq On : 18 Nov 2021 22:27
Operator : SY/MD
Sample : M4706-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc