

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023626.D
 Acq On : 19 Nov 2021 00:03
 Operator : SY/MD
 Sample : M4706-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AB5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	56	62	68	rVB2	4379	4886	1.43%	0.167%
2	1.304	75	82	94	rBV	53459	54867	16.09%	1.875%
3	1.568	156	164	180	rBV	46539	53113	15.58%	1.815%
4	2.108	321	332	345	rBV	87170	125356	36.77%	4.284%
5	2.506	443	456	479	rBB	50092	87270	25.60%	2.982%
6	3.912	882	893	923	rBV3	19171	78869	23.13%	2.695%
7	4.355	1011	1031	1058	rBV4	64815	200065	58.68%	6.837%
8	5.050	1231	1247	1279	rBV2	136746	340933	100.00%	11.650%
9	5.619	1413	1424	1443	rBV	121841	248532	72.90%	8.493%
10	5.911	1507	1515	1529	rBV7	2222	4865	1.43%	0.166%
11	6.072	1552	1565	1589	rBV2	78034	162328	47.61%	5.547%
12	6.522	1695	1705	1712	rBV4	2096	3627	1.06%	0.124%
13	6.989	1840	1850	1866	rBV	34433	64548	18.93%	2.206%
14	7.317	1941	1952	1972	rBV	152262	271041	79.50%	9.262%
15	7.625	2040	2048	2066	rBV2	20685	37575	11.02%	1.284%
16	8.095	2182	2194	2234	rBV2	107802	269724	79.11%	9.217%
17	8.853	2418	2430	2456	rBV	197155	325077	95.35%	11.108%
18	10.217	2841	2854	2876	rBV	53632	84816	24.88%	2.898%
19	11.249	3164	3175	3195	rBV	178512	275442	80.79%	9.412%
20	11.625	3279	3292	3319	rVB	146757	233449	68.47%	7.977%




Sum of corrected areas: 2926383

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023626.D
Acq On : 19 Nov 2021 00:03
Operator : SY/MD
Sample : M4706-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AB5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

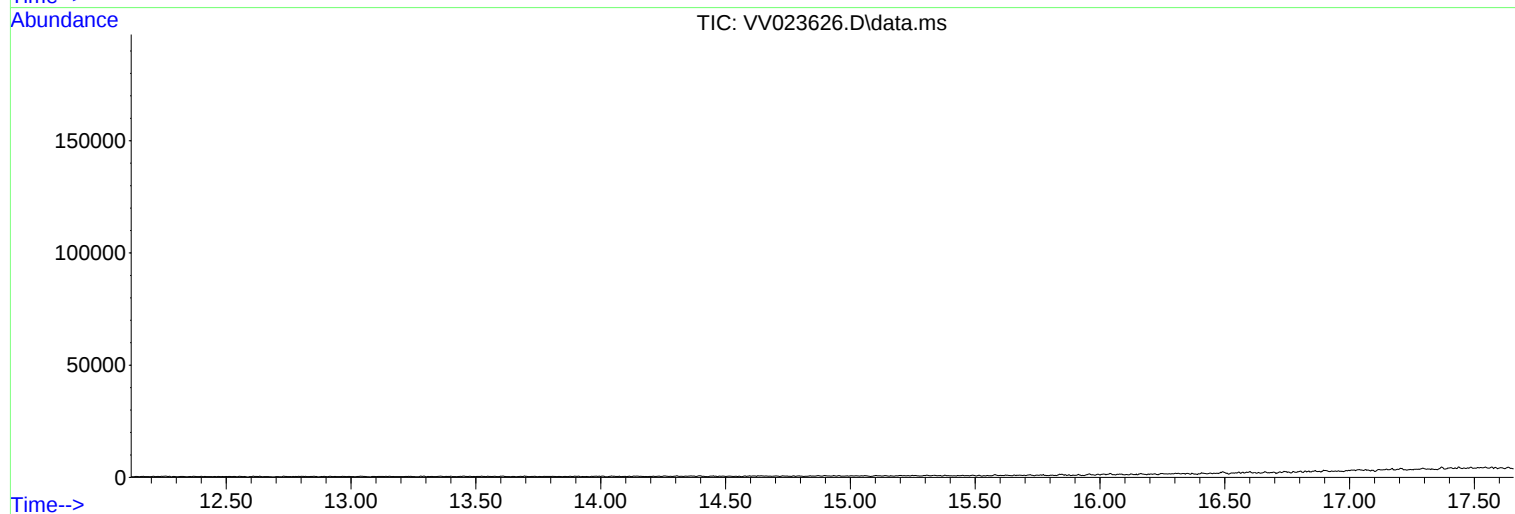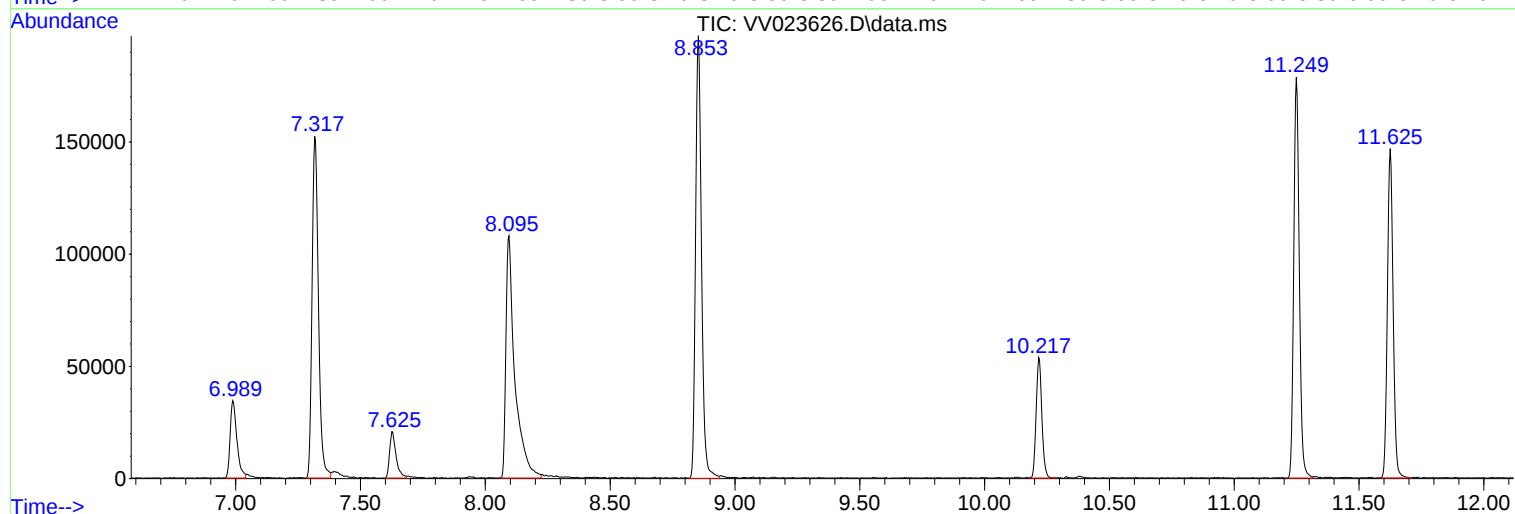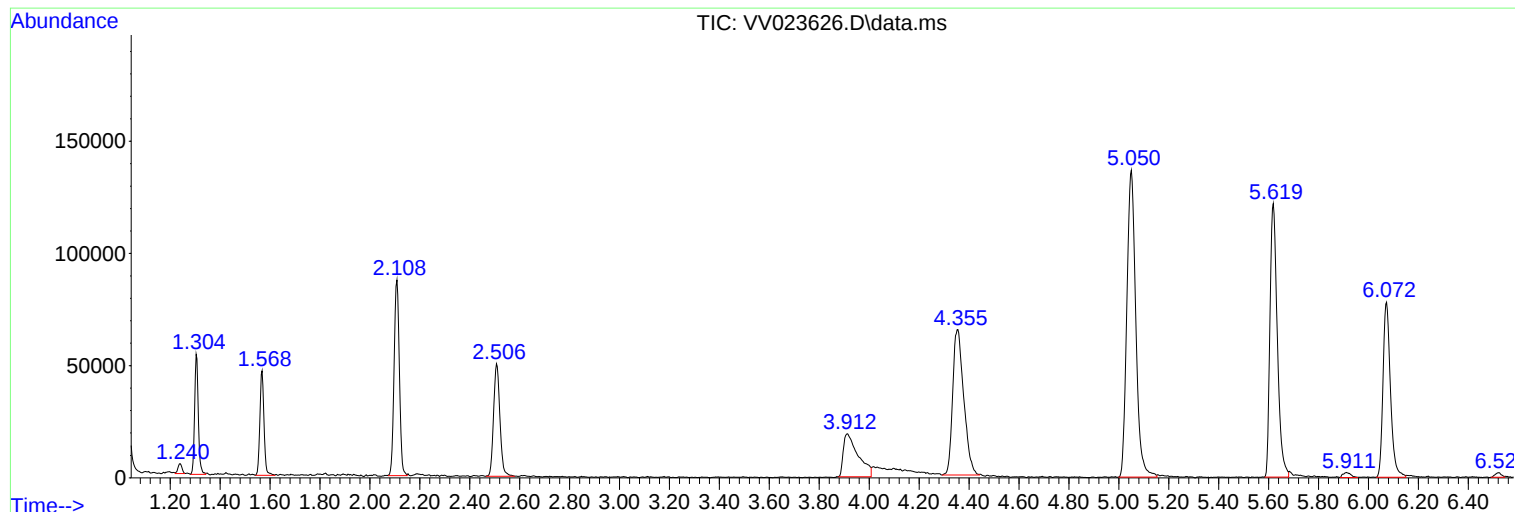

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023626.D
Acq On : 19 Nov 2021 00:03
Operator : SY/MD
Sample : M4706-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AB5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023626.D
Acq On : 19 Nov 2021 00:03
Operator : SY/MD
Sample : M4706-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AB5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc