

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023627.D
 Acq On : 19 Nov 2021 00:26
 Operator : SY/MD
 Sample : M4706-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AB6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	57	62	72	rVB	4659	5254	1.59%	0.182%
2	1.304	74	82	97	rVB	54780	55544	16.84%	1.925%
3	1.568	155	164	176	rBV	46003	52201	15.83%	1.809%
4	2.108	320	332	344	rBV	87690	125776	38.14%	4.358%
5	2.506	444	456	477	rBV	51086	86872	26.34%	3.010%
6	3.905	876	891	914	rBV3	17527	65141	19.75%	2.257%
7	4.352	1013	1030	1053	rBV3	64398	192393	58.34%	6.667%
8	5.046	1231	1246	1279	rBV2	130994	327879	99.43%	11.361%
9	5.619	1409	1424	1444	rBV	128629	258796	78.48%	8.967%
10	6.072	1552	1565	1595	rBV	73805	155789	47.24%	5.398%
11	6.519	1695	1704	1712	rBV4	2262	3534	1.07%	0.122%
12	6.989	1841	1850	1868	rBV	33131	64866	19.67%	2.248%
13	7.316	1941	1952	1969	rBV	150485	263163	79.80%	9.119%
14	7.628	2039	2049	2069	rBV	19763	38290	11.61%	1.327%
15	8.095	2184	2194	2232	rBV	102439	264201	80.12%	9.155%
16	8.853	2419	2430	2449	rBV	199697	329759	100.00%	11.426%
17	10.217	2843	2854	2868	rBV	53326	83971	25.46%	2.910%
18	11.249	3164	3175	3199	rBV	179609	284623	86.31%	9.862%
19	11.625	3280	3292	3306	rBV	143665	227894	69.11%	7.897%




Sum of corrected areas: 2885946

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023627.D
Acq On : 19 Nov 2021 00:26
Operator : SY/MD
Sample : M4706-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

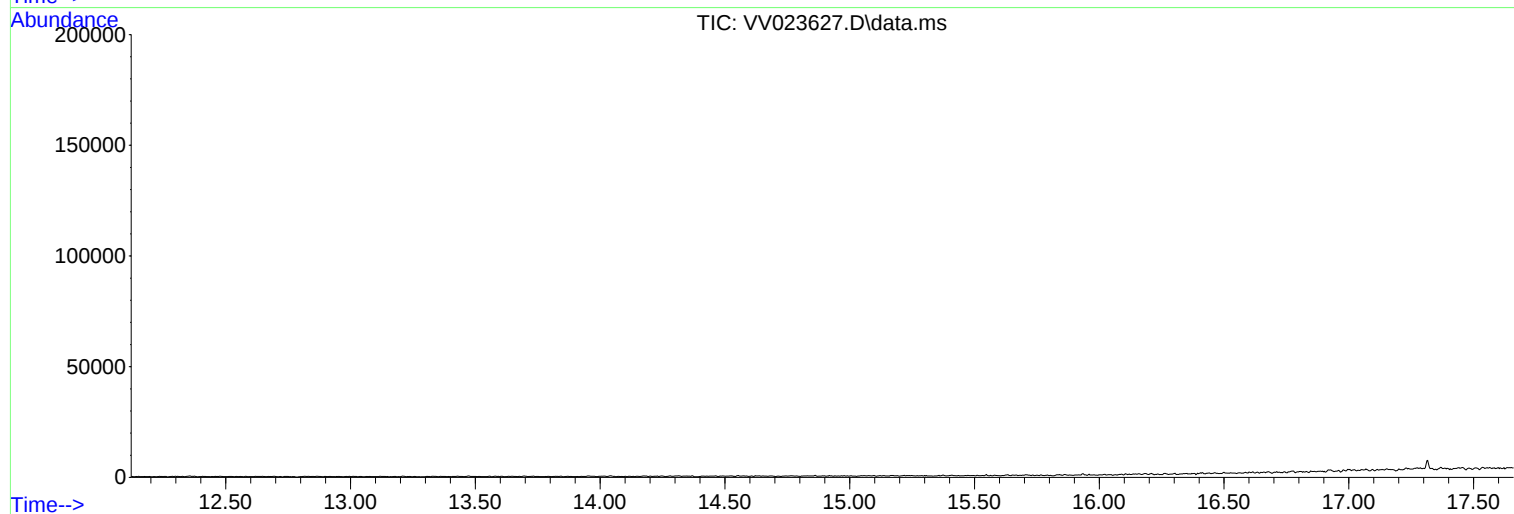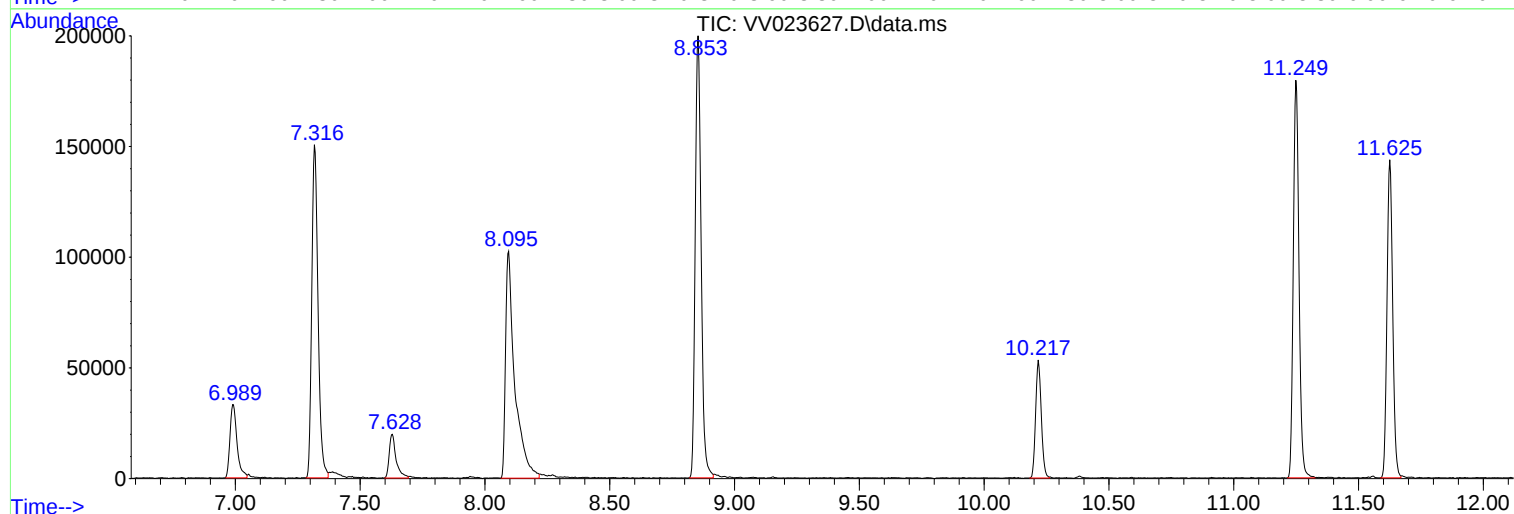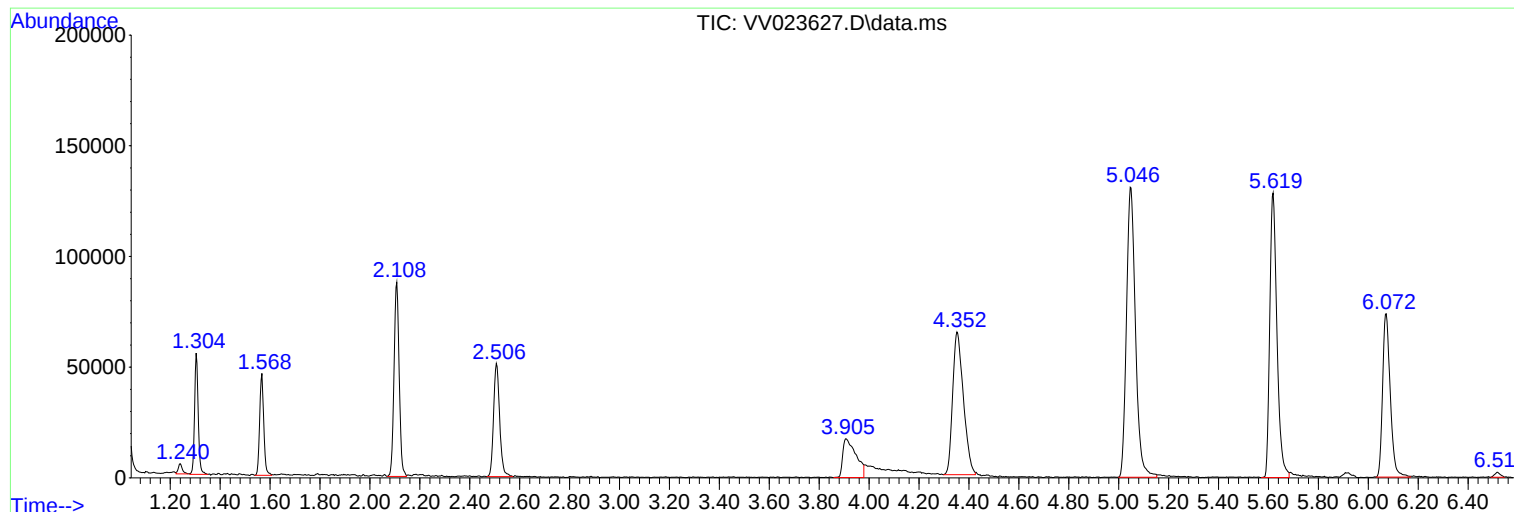

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023627.D
Acq On : 19 Nov 2021 00:26
Operator : SY/MD
Sample : M4706-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023627.D
Acq On : 19 Nov 2021 00:26
Operator : SY/MD
Sample : M4706-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
