

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111823\
 Data File : VW033007.D
 Acq On : 18 Nov 2023 16:45
 Operator : SY/MD
 Sample : 05437-08MERE
 Misc : 6.10g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1E7RE

Quant Time: Nov 20 01:20:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 20 01:19:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	589145	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	607935	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	331095	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	96654	19.398	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	38.800%#
7) Chloroethane-d5	1.507	69	74769	18.111	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	36.220%#
11) 1,1-Dichloroethene-d2	2.037	65	35245	16.235	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	32.460%#
21) 2-Butanone-d5	3.799	46	186097	87.130	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	87.130%
24) Chloroform-d	4.246	84	268265	31.164	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	62.320%#
26) 1,2-Dichloroethane-d4	4.941	65	189663	36.210	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	72.420%
32) Benzene-d6	4.953	84	477594	28.804	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	57.600%#
36) 1,2-Dichloropropane-d6	5.989	67	158240	32.833	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	65.660%#
41) Toluene-d8	7.243	98	420324	27.496	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	55.000%#
43) trans-1,3-Dichloroprop...	7.555	79	90054	35.196	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.400%
47) 2-Hexanone-d5	8.043	63	159253	90.194	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.190%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	254502	36.048	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	72.100%
66) 1,2-Dichlorobenzene-d4	11.564	152	226791	35.252	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	70.500%#
Target Compounds						Qvalue
34) Trichloroethene	5.828	95	435664	97.086	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
Data File : VV033007.D
Acq On : 18 Nov 2023 16:45
Operator : SY/MD
Sample : 05437-08MERE
Misc : 6.10g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1E7RE

Quant Time: Nov 20 01:20:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Nov 20 01:19:10 2023
Response via : Initial Calibration

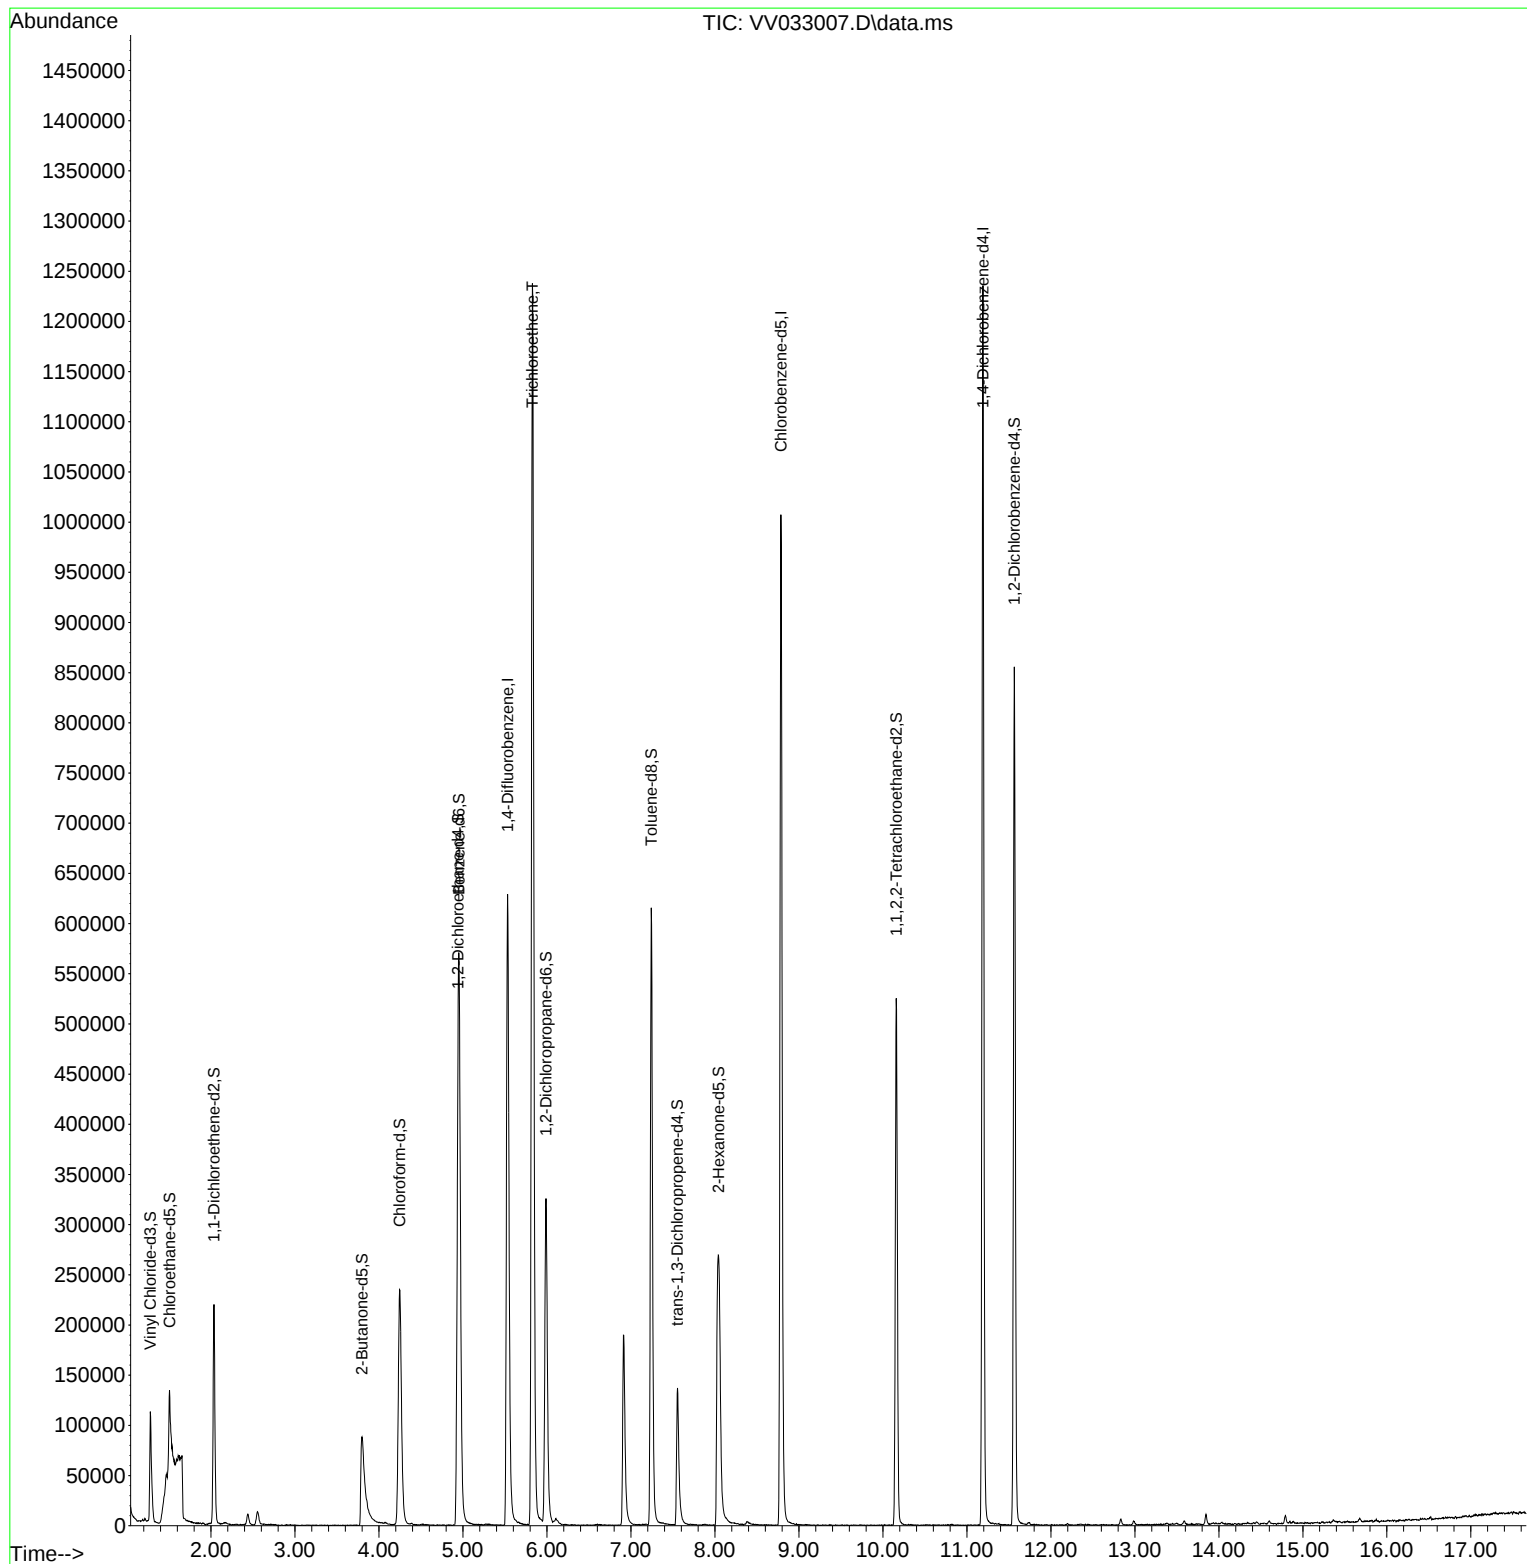

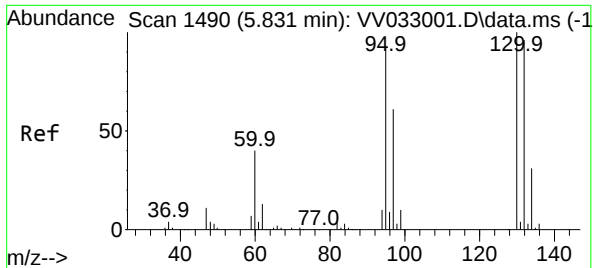

#34
 Trichloroethene
 Concen: 97.086 ug/L
 RT: 5.828 min Scan# 14
 Delta R.T. -0.003 min
 Lab File: VV033007.D
 Acq: 18 Nov 2023 16:45

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1E7RE

Tgt Ion: 95 Resp: 435664
 Ion Ratio Lower Upper
 95 100
 97 63.9 45.7 84.9
 132 101.4 70.0 130.0
 130 106.4 72.2 134.0

