

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
 Data File : VV033002.D
 Acq On : 18 Nov 2023 12:42
 Operator : SY/MD
 Sample : VV1118MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK220

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

Signal : TIC: VV033002.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	194328	208011	14.16%	1.821%
2	1.529	145	152	170	rVB	146299	181309	12.35%	1.587%
3	2.056	306	316	333	rBV	291866	427303	29.09%	3.740%
4	2.397	419	422	424	rBV2	709	403	0.03%	0.004%
5	2.606	484	487	489	rBV2	661	362	0.02%	0.003%
6	2.622	489	492	495	rVV3	989	596	0.04%	0.005%
7	2.687	509	512	513	rBV3	1083	570	0.04%	0.005%
8	2.892	574	576	577	rBV	630	295	0.02%	0.003%
9	2.925	583	586	588	rVB2	510	273	0.02%	0.002%
10	2.944	588	592	594	rVB4	767	466	0.03%	0.004%
11	2.995	605	608	609	rBV	563	285	0.02%	0.002%
12	3.130	645	650	653	rBV3	1063	879	0.06%	0.008%
13	3.355	716	720	722	rBV3	506	313	0.02%	0.003%
14	3.368	722	724	728	rVB2	627	375	0.03%	0.003%
15	3.407	733	736	739	rBV3	426	317	0.02%	0.003%
16	3.497	760	764	769	rBV5	628	675	0.05%	0.006%
17	3.529	771	774	777	rVB3	716	412	0.03%	0.004%
18	3.552	777	781	786	rVB3	487	380	0.03%	0.003%
19	3.587	790	792	796	rVB3	541	256	0.02%	0.002%
20	3.609	796	799	802	rBV4	646	501	0.03%	0.004%
21	3.651	810	812	817	rVB3	614	326	0.02%	0.003%
22	3.780	843	852	886	rBV	100934	273084	18.59%	2.390%
23	4.246	983	997	1024	rVB	240304	597611	40.69%	5.231%
24	4.851	1183	1185	1186	rBV2	576	307	0.02%	0.003%
25	4.953	1200	1217	1250	rBV2	554539	1468683	100.00%	12.855%
26	5.532	1385	1397	1428	rBV	451298	923966	62.91%	8.087%
27	5.828	1479	1489	1499	rBV8	8600	17637	1.20%	0.154%
28	5.934	1519	1522	1525	rBV4	651	523	0.04%	0.005%
29	5.986	1525	1538	1562	rBV	317387	660385	44.96%	5.780%
30	6.256	1616	1622	1624	rBV5	848	838	0.06%	0.007%
31	6.326	1641	1644	1647	rBV2	777	458	0.03%	0.004%
32	6.381	1656	1661	1662	rBV3	398	329	0.02%	0.003%
33	6.397	1662	1666	1669	rBV5	632	440	0.03%	0.004%
34	6.516	1700	1703	1705	rBV	505	279	0.02%	0.002%
35	6.609	1728	1732	1735	rBV3	783	683	0.05%	0.006%
36	6.844	1802	1805	1809	rBV3	468	388	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
 Data File : VV033002.D
 Acq On : 18 Nov 2023 12:42
 Operator : SY/MD
 Sample : VV1118MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK220

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

37	6.912	1814	1826	1850	rBV	174247	332107	22.61%	2.907%
38	7.243	1917	1929	1950	rBV	642154	1125557	76.64%	9.852%
39	7.551	2016	2025	2053	rBV	127559	225285	15.34%	1.972%
40	7.822	2106	2109	2113	rBV2	743	548	0.04%	0.005%
41	8.021	2162	2171	2212	rBV	347794	657295	44.75%	5.753%
42	8.474	2308	2312	2317	rVB6	1001	1032	0.07%	0.009%
43	8.535	2329	2331	2334	rBV3	573	303	0.02%	0.003%
44	8.625	2356	2359	2363	rVB3	878	570	0.04%	0.005%
45	8.651	2363	2367	2371	rBV5	750	790	0.05%	0.007%
46	8.677	2371	2375	2378	rBV4	499	484	0.03%	0.004%
47	8.735	2389	2393	2395	rBV3	577	375	0.03%	0.003%
48	8.783	2395	2408	2437	rBV	710294	1171865	79.79%	10.257%
49	9.175	2528	2530	2533	rBV2	868	521	0.04%	0.005%
50	9.214	2540	2542	2546	rVB2	383	270	0.02%	0.002%
51	9.233	2546	2548	2551	rBV2	595	257	0.02%	0.002%
52	9.249	2551	2553	2555	rBV	586	289	0.02%	0.003%
53	9.381	2591	2594	2595	rBV	677	386	0.03%	0.003%
54	9.452	2614	2616	2620	rVB2	489	290	0.02%	0.003%
55	9.477	2621	2624	2630	rBV5	961	1236	0.08%	0.011%
56	9.657	2678	2680	2683	rBV2	554	345	0.02%	0.003%
57	9.706	2692	2695	2697	rVB2	754	336	0.02%	0.003%
58	9.834	2732	2735	2737	rBV	744	336	0.02%	0.003%
59	9.870	2742	2746	2748	rBV3	762	633	0.04%	0.006%
60	10.153	2821	2834	2864	rBV	460988	727195	49.51%	6.365%
61	10.329	2882	2889	2894	rVB4	1542	1956	0.13%	0.017%
62	10.481	2930	2936	2942	rBV6	1347	1907	0.13%	0.017%
63	10.574	2963	2965	2968	rBV2	765	453	0.03%	0.004%
64	10.677	2995	2997	2999	rBV2	515	273	0.02%	0.002%
65	10.735	3013	3015	3017	rVB2	721	307	0.02%	0.003%
66	10.751	3017	3020	3021	rBV2	508	296	0.02%	0.003%
67	10.792	3030	3033	3034	rBV2	540	331	0.02%	0.003%
68	10.854	3047	3052	3053	rBV3	1173	995	0.07%	0.009%
69	10.918	3069	3072	3076	rVB2	455	265	0.02%	0.002%
70	10.940	3077	3079	3083	rVB4	802	524	0.04%	0.005%
71	10.966	3084	3087	3089	rVV2	557	304	0.02%	0.003%
72	10.979	3089	3091	3095	rVB2	618	349	0.02%	0.003%
73	11.008	3095	3100	3101	rBV3	722	516	0.04%	0.005%
74	11.127	3129	3137	3144	rBV8	2870	4565	0.31%	0.040%
75	11.188	3144	3156	3179	rVV	744017	1156201	78.72%	10.120%
76	11.490	3248	3250	3256	rVB3	746	596	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
 Data File : VV033002.D
 Acq On : 18 Nov 2023 12:42
 Operator : SY/MD
 Sample : VV1118MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK220

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

77	11.516	3256	3258	3260	rBV	1030	498	0.03%	0.004%
78	11.561	3260	3272	3292	rBV	730995	1141361	77.71%	9.990%
79	11.763	3333	3335	3339	rBV2	653	628	0.04%	0.005%
80	12.017	3411	3414	3419	rVB5	666	465	0.03%	0.004%
81	12.252	3485	3487	3492	rBV2	451	438	0.03%	0.004%
82	12.336	3511	3513	3516	rBV2	414	289	0.02%	0.003%
83	12.590	3587	3592	3603	rVB5	3785	5875	0.40%	0.051%
84	12.651	3605	3611	3615	rBV3	857	963	0.07%	0.008%
85	12.686	3620	3622	3626	rVB3	655	331	0.02%	0.003%
86	12.780	3648	3651	3655	rVB3	835	565	0.04%	0.005%
87	12.844	3668	3671	3672	rBV	526	269	0.02%	0.002%
88	12.902	3685	3689	3691	rBV2	714	592	0.04%	0.005%
89	12.966	3707	3709	3713	rBV3	582	359	0.02%	0.003%
90	13.149	3758	3766	3768	rBV4	501	731	0.05%	0.006%
91	13.207	3775	3784	3792	rBV4	9811	14418	0.98%	0.126%
92	13.275	3802	3805	3808	rBV3	592	495	0.03%	0.004%
93	13.345	3821	3827	3832	rBV5	695	799	0.05%	0.007%
94	13.445	3848	3858	3873	rBV2	27010	46854	3.19%	0.410%
95	13.651	3920	3922	3924	rBV2	619	401	0.03%	0.004%
96	13.686	3924	3933	3942	rVV3	11780	17880	1.22%	0.157%
97	13.815	3971	3973	3976	rVB2	737	285	0.02%	0.002%
98	13.834	3976	3979	3983	rBV2	807	659	0.04%	0.006%
99	14.612	4219	4221	4225	rBV	797	645	0.04%	0.006%
100	14.734	4256	4259	4262	rBV4	862	773	0.05%	0.007%

Sum of corrected areas: 11424634




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
Data File : VV033002.D
Acq On : 18 Nov 2023 12:42
Operator : SY/MD
Sample : VV1118MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK220

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

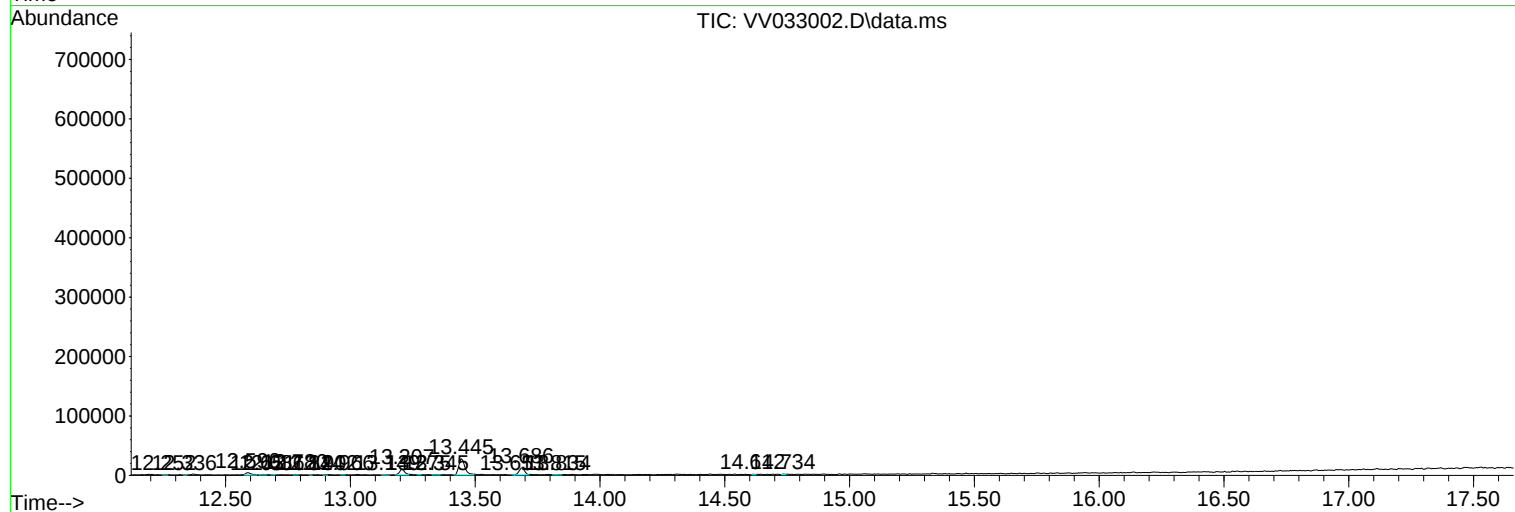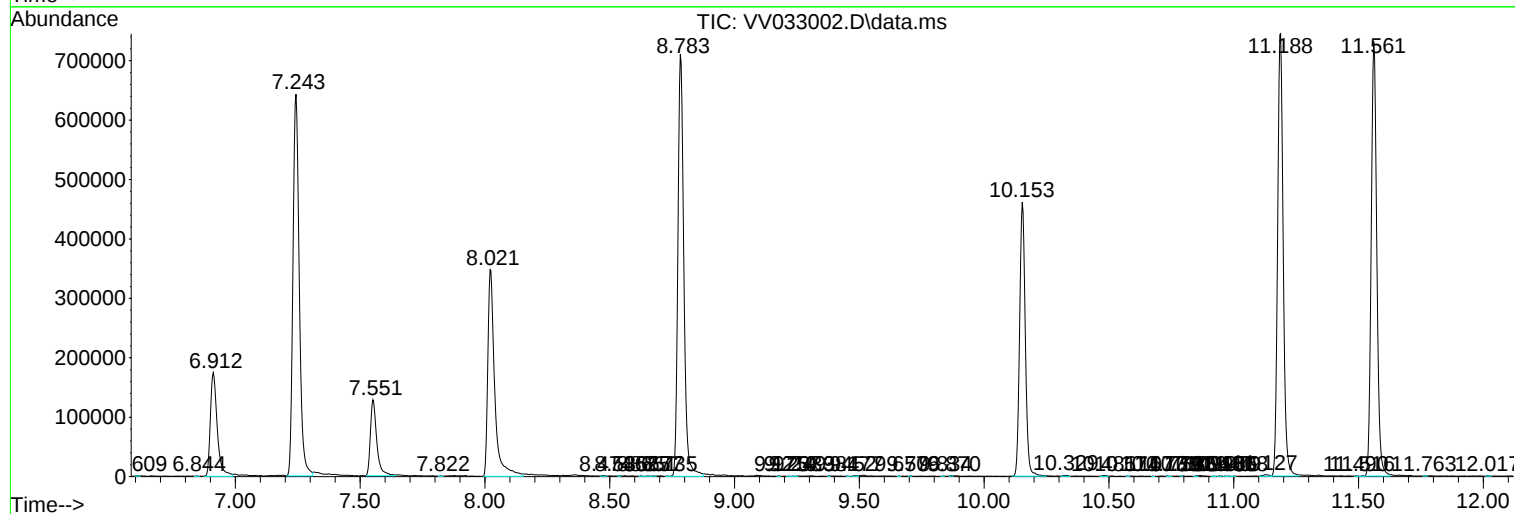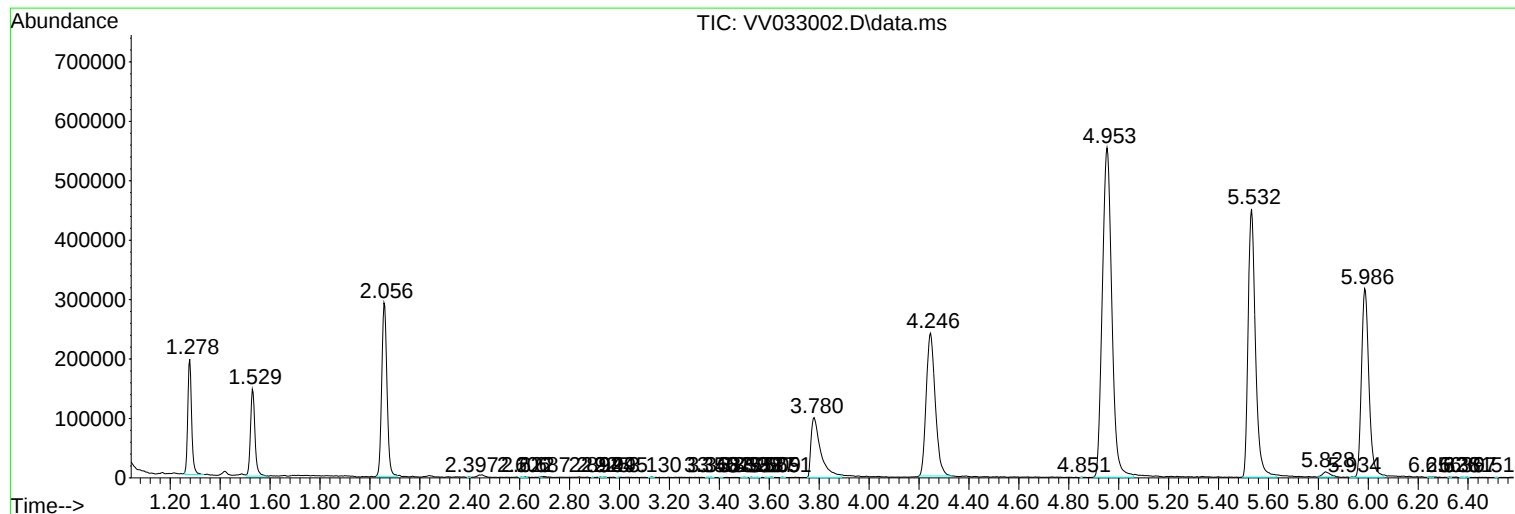

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
Data File : VV033002.D
Acq On : 18 Nov 2023 12:42
Operator : SY/MD
Sample : VV1118MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK220

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
Data File : VV033002.D
Acq On : 18 Nov 2023 12:42
Operator : SY/MD
Sample : VV1118MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK220

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc