

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
 Data File : VV033003.D
 Acq On : 18 Nov 2023 13:45
 Operator : SY/MD
 Sample : VV1118WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK221

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

Signal : TIC: VV033003.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	190616	195397	13.96%	1.838%
2	1.529	145	152	165	rVB	135767	159474	11.40%	1.500%
3	1.989	288	295	296	rBV5	1085	1045	0.07%	0.010%
4	2.056	307	316	336	rVB	281878	407832	29.14%	3.837%
5	2.272	381	383	386	rBV2	568	424	0.03%	0.004%
6	2.307	391	394	397	rBV4	807	695	0.05%	0.007%
7	2.375	413	415	418	rBV2	562	408	0.03%	0.004%
8	2.407	422	425	427	rBV	523	368	0.03%	0.003%
9	2.449	430	438	443	rBV5	2952	4660	0.33%	0.044%
10	2.519	458	460	463	rVB2	765	360	0.03%	0.003%
11	2.616	485	490	492	rBV4	508	479	0.03%	0.005%
12	2.690	510	513	516	rVB5	980	649	0.05%	0.006%
13	2.889	571	575	579	rBV4	490	363	0.03%	0.003%
14	2.921	581	585	588	rBV2	720	471	0.03%	0.004%
15	3.259	686	690	693	rVB5	784	643	0.05%	0.006%
16	3.371	721	725	728	rBV2	526	502	0.04%	0.005%
17	3.529	766	774	777	rBV3	571	527	0.04%	0.005%
18	3.561	781	784	790	rVB3	492	404	0.03%	0.004%
19	3.625	800	804	810	rVB3	645	600	0.04%	0.006%
20	3.661	810	815	819	rBV3	699	493	0.04%	0.005%
21	3.712	826	831	832	rBV2	539	301	0.02%	0.003%
22	3.783	844	853	884	rBV2	85176	231417	16.54%	2.177%
23	4.246	980	997	1026	rBV	224068	573302	40.97%	5.394%
24	4.667	1124	1128	1131	rBV3	686	557	0.04%	0.005%
25	4.741	1147	1151	1155	rBV3	604	559	0.04%	0.005%
26	4.799	1166	1169	1171	rBV2	659	390	0.03%	0.004%
27	4.850	1182	1185	1187	rBV3	609	340	0.02%	0.003%
28	4.953	1200	1217	1248	rBV2	533544	1399460	100.00%	13.167%
29	5.333	1332	1335	1338	rBV3	1043	772	0.06%	0.007%
30	5.378	1347	1349	1351	rBV2	734	368	0.03%	0.003%
31	5.532	1385	1397	1428	rBV	413818	856558	61.21%	8.059%
32	5.828	1479	1489	1502	rBV3	10289	21790	1.56%	0.205%
33	5.908	1512	1514	1518	rVB3	840	472	0.03%	0.004%
34	5.989	1525	1539	1562	rBV	295841	612171	43.74%	5.760%
35	6.307	1634	1638	1640	rBV4	725	552	0.04%	0.005%
36	6.365	1654	1656	1658	rBV3	822	495	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
 Data File : VV033003.D
 Acq On : 18 Nov 2023 13:45
 Operator : SY/MD
 Sample : VV1118WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK221

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

37	6.596	1722	1728	1731	rVV5	832	900	0.06%	0.008%
38	6.680	1752	1754	1761	rVB3	645	548	0.04%	0.005%
39	6.776	1782	1784	1786	rBV	779	300	0.02%	0.003%
40	6.821	1794	1798	1801	rBV4	470	321	0.02%	0.003%
41	6.911	1814	1826	1846	rBV2	165115	310893	22.22%	2.925%
42	7.243	1917	1929	1953	rBV	648175	1135568	81.14%	10.684%
43	7.551	2016	2025	2046	rBV	122481	217043	15.51%	2.042%
44	7.854	2115	2119	2122	rBV	700	602	0.04%	0.006%
45	7.873	2123	2125	2131	rVV2	1320	1147	0.08%	0.011%
46	7.915	2135	2138	2140	rVV3	661	470	0.03%	0.004%
47	8.024	2162	2172	2201	rBV	305579	559629	39.99%	5.265%
48	8.365	2268	2278	2281	rBV8	2211	3531	0.25%	0.033%
49	8.426	2293	2297	2299	rBV3	880	662	0.05%	0.006%
50	8.532	2328	2330	2333	rBV	478	328	0.02%	0.003%
51	8.583	2345	2346	2349	rVB2	858	321	0.02%	0.003%
52	8.622	2354	2358	2359	rBV2	392	288	0.02%	0.003%
53	8.709	2382	2385	2388	rBV3	577	369	0.03%	0.003%
54	8.728	2388	2391	2396	rBV3	354	304	0.02%	0.003%
55	8.786	2396	2409	2429	rBV	653174	1079295	77.12%	10.154%
56	9.075	2496	2499	2502	rBV4	604	353	0.03%	0.003%
57	9.172	2525	2529	2530	rBV3	588	402	0.03%	0.004%
58	9.233	2546	2548	2551	rBV2	638	336	0.02%	0.003%
59	9.252	2551	2554	2556	rBV	521	290	0.02%	0.003%
60	9.432	2607	2610	2611	rBV	553	324	0.02%	0.003%
61	9.603	2659	2663	2666	rBV3	632	500	0.04%	0.005%
62	9.677	2681	2686	2690	rBV3	696	675	0.05%	0.006%
63	9.895	2752	2754	2758	rVB2	508	371	0.03%	0.003%
64	10.153	2823	2834	2861	rVV	404586	643370	45.97%	6.053%
65	10.326	2884	2888	2895	rVB4	1405	1431	0.10%	0.013%
66	10.419	2914	2917	2921	rVB4	543	370	0.03%	0.003%
67	10.464	2926	2931	2940	rBV5	558	842	0.06%	0.008%
68	10.567	2960	2963	2966	rVB2	810	448	0.03%	0.004%
69	10.587	2966	2969	2971	rBV	500	337	0.02%	0.003%
70	10.779	3026	3029	3031	rBV2	690	479	0.03%	0.005%
71	10.931	3073	3076	3080	rVB3	588	378	0.03%	0.004%
72	11.001	3095	3098	3103	rBV3	494	467	0.03%	0.004%
73	11.188	3144	3156	3185	rBV	690034	1082882	77.38%	10.188%
74	11.406	3221	3224	3227	rVB3	465	307	0.02%	0.003%
75	11.429	3227	3231	3234	rBV3	498	371	0.03%	0.003%
76	11.451	3236	3238	3242	rVV2	497	310	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
 Data File : VV033003.D
 Acq On : 18 Nov 2023 13:45
 Operator : SY/MD
 Sample : VV1118WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK221

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

77	11.561	3261	3272	3290	rBV	700508	1091144	77.97%	10.266%
78	11.895	3374	3376	3382	rVV4	430	295	0.02%	0.003%
79	11.995	3406	3407	3412	rBV3	725	361	0.03%	0.003%
80	12.066	3426	3429	3432	rBV4	537	303	0.02%	0.003%
81	12.120	3442	3446	3450	rBV2	652	463	0.03%	0.004%
82	12.329	3509	3511	3515	rBV	517	297	0.02%	0.003%
83	12.429	3540	3542	3547	rVB2	555	368	0.03%	0.003%
84	12.509	3564	3567	3570	rVB2	564	306	0.02%	0.003%
85	12.548	3576	3579	3586	rBV2	732	581	0.04%	0.005%
86	12.580	3586	3589	3591	rBV3	593	326	0.02%	0.003%
87	12.593	3591	3593	3597	rVV4	589	351	0.03%	0.003%
88	12.664	3613	3615	3619	rBV4	547	381	0.03%	0.004%
89	12.815	3658	3662	3666	rVB4	460	451	0.03%	0.004%
90	12.976	3710	3712	3716	rBV2	630	444	0.03%	0.004%
91	13.059	3736	3738	3741	rBV3	374	292	0.02%	0.003%
92	13.368	3828	3834	3835	rBV3	634	596	0.04%	0.006%
93	13.448	3848	3859	3860	rBV5	2772	3050	0.22%	0.029%
94	13.664	3923	3926	3929	rVB2	733	366	0.03%	0.003%
95	13.693	3929	3935	3943	rBV8	1972	2460	0.18%	0.023%
96	13.741	3947	3950	3958	rVB5	861	785	0.06%	0.007%
97	14.037	4040	4042	4046	rVB2	720	449	0.03%	0.004%
98	14.107	4058	4064	4065	rBV2	891	796	0.06%	0.007%
99	14.204	4092	4094	4097	rBV2	713	325	0.02%	0.003%
100	14.320	4128	4130	4133	rBV3	824	569	0.04%	0.005%




Sum of corrected areas: 10628819

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
Data File : VV033003.D
Acq On : 18 Nov 2023 13:45
Operator : SY/MD
Sample : VV1118WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK221

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

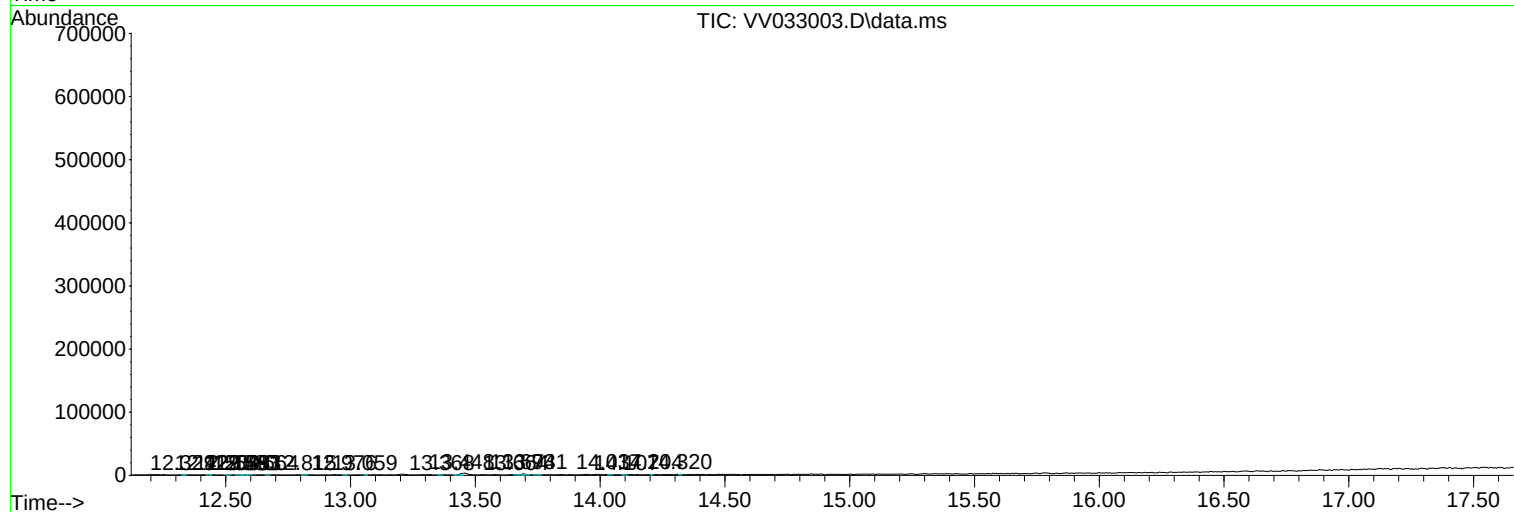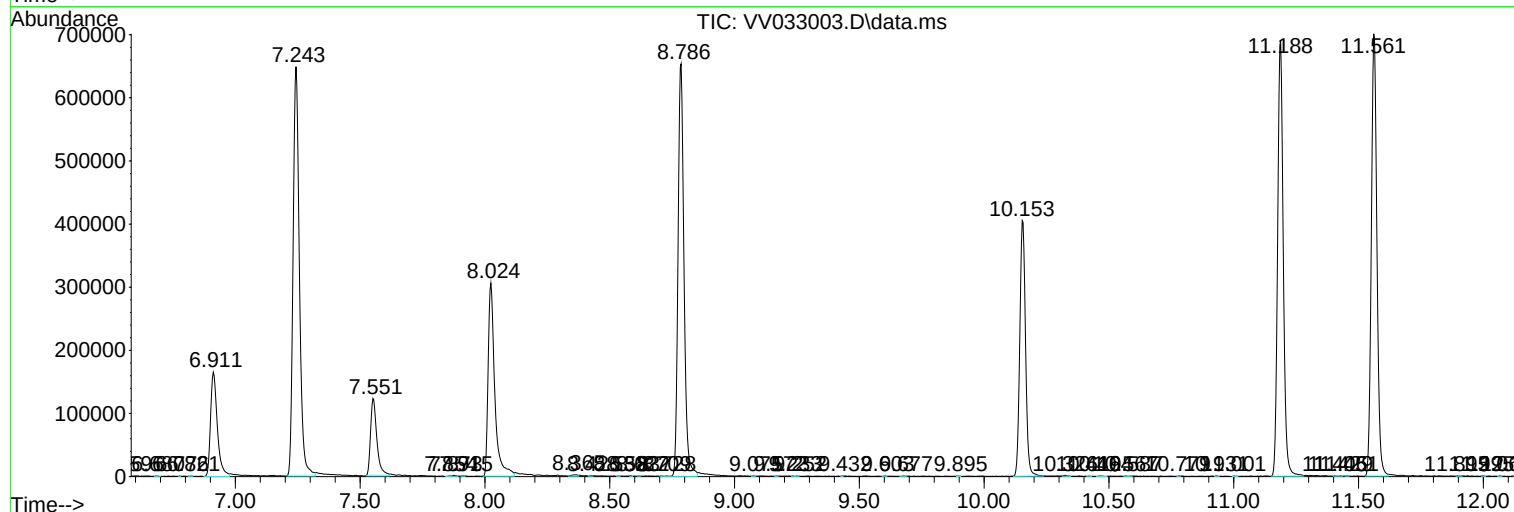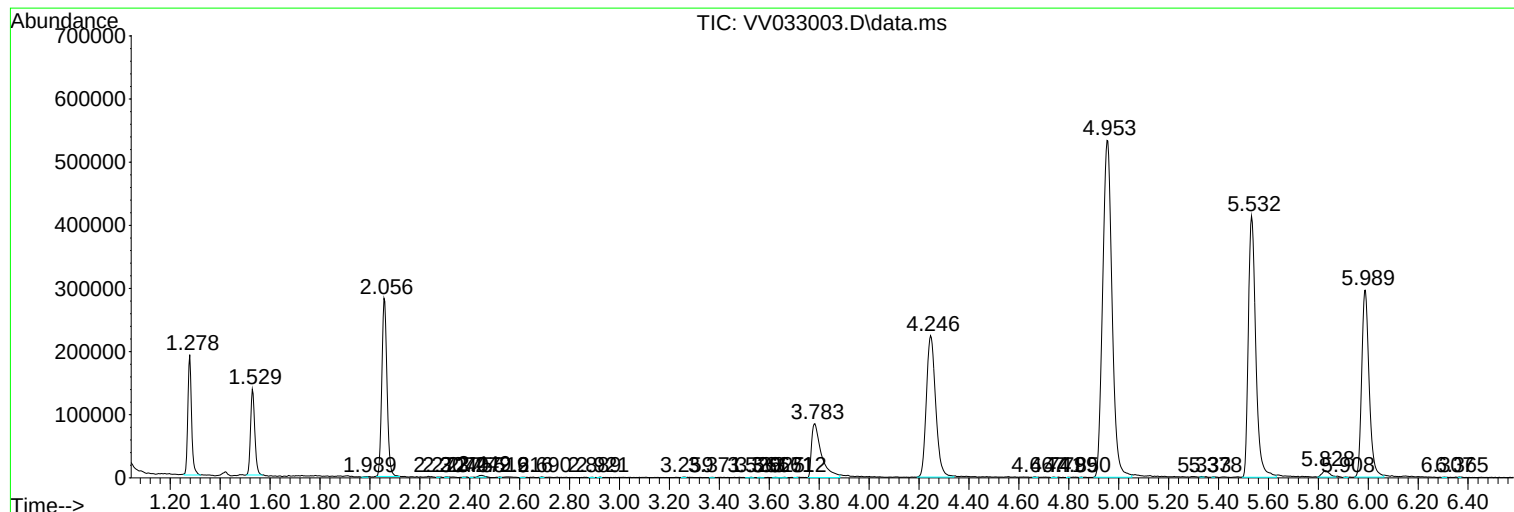

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
Data File : VV033003.D
Acq On : 18 Nov 2023 13:45
Operator : SY/MD
Sample : VV1118WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK221

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
Data File : VV033003.D
Acq On : 18 Nov 2023 13:45
Operator : SY/MD
Sample : VV1118WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK221

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------