

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
 Data File : VV033004.D
 Acq On : 18 Nov 2023 14:35
 Operator : SY/MD
 Sample : VV1118WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK222

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

Signal : TIC: VV033004.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	169630	177525	13.24%	1.742%
2	1.529	145	152	169	rVB	124302	150604	11.24%	1.478%
3	2.059	305	317	340	rBV	266360	394834	29.46%	3.875%
4	2.281	384	386	389	rBV2	520	415	0.03%	0.004%
5	2.449	433	438	448	rVB6	2895	4087	0.30%	0.040%
6	2.696	513	515	519	rVB2	466	258	0.02%	0.003%
7	2.728	523	525	530	rVB2	434	294	0.02%	0.003%
8	2.789	542	544	547	rBV3	601	342	0.03%	0.003%
9	2.838	557	559	561	rBV2	400	252	0.02%	0.002%
10	2.892	572	576	577	rBV2	532	278	0.02%	0.003%
11	2.908	579	581	584	rVB2	634	252	0.02%	0.002%
12	2.928	584	587	588	rBV2	324	195	0.01%	0.002%
13	2.973	599	601	605	rVB2	446	195	0.01%	0.002%
14	3.024	614	617	621	rBV4	529	391	0.03%	0.004%
15	3.108	640	643	644	rVB	435	232	0.02%	0.002%
16	3.291	695	700	701	rBV3	530	365	0.03%	0.004%
17	3.355	715	720	723	rBV2	519	446	0.03%	0.004%
18	3.458	746	752	757	rVB4	761	829	0.06%	0.008%
19	3.580	786	790	792	rBV	470	251	0.02%	0.002%
20	3.600	792	796	799	rBV2	383	323	0.02%	0.003%
21	3.683	816	822	825	rVB4	520	564	0.04%	0.006%
22	3.712	828	831	834	rBV	381	223	0.02%	0.002%
23	3.744	838	841	844	rVB	380	195	0.01%	0.002%
24	3.783	844	853	880	rBV	83898	227611	16.98%	2.234%
25	4.124	957	959	962	rBV3	527	247	0.02%	0.002%
26	4.249	982	998	1025	rBV	215618	548931	40.95%	5.388%
27	4.738	1148	1150	1155	rVB4	814	501	0.04%	0.005%
28	4.760	1155	1157	1162	rBV4	355	291	0.02%	0.003%
29	4.786	1162	1165	1167	rBV2	602	405	0.03%	0.004%
30	4.831	1174	1179	1181	rBV3	833	780	0.06%	0.008%
31	4.866	1188	1190	1193	rBV	475	233	0.02%	0.002%
32	4.956	1202	1218	1247	rBV2	506957	1340331	100.00%	13.156%
33	5.535	1385	1398	1426	rBV	387674	800592	59.73%	7.858%
34	5.989	1526	1539	1562	rBV	290044	592005	44.17%	5.811%
35	6.297	1632	1635	1638	rBV3	901	721	0.05%	0.007%
36	6.329	1640	1645	1648	rBV2	748	755	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
 Data File : VV033004.D
 Acq On : 18 Nov 2023 14:35
 Operator : SY/MD
 Sample : VV1118WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK222

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

37	6.378	1658	1660	1664	rBV2	529	312	0.02%	0.003%
38	6.419	1671	1673	1677	rVB2	362	203	0.02%	0.002%
39	6.455	1682	1684	1688	rBV	388	261	0.02%	0.003%
40	6.471	1688	1689	1694	rVB2	592	412	0.03%	0.004%
41	6.506	1697	1700	1703	rBV	452	294	0.02%	0.003%
42	6.583	1719	1724	1725	rBV4	844	662	0.05%	0.006%
43	6.677	1751	1753	1755	rVB2	494	244	0.02%	0.002%
44	6.735	1766	1771	1773	rBV2	672	441	0.03%	0.004%
45	6.915	1811	1827	1850	rBV	161367	302253	22.55%	2.967%
46	7.243	1918	1929	1955	rBV	631256	1110662	82.86%	10.902%
47	7.551	2016	2025	2055	rVV	114456	209939	15.66%	2.061%
48	7.754	2086	2088	2090	rBV3	827	414	0.03%	0.004%
49	7.825	2106	2110	2112	rBV2	514	313	0.02%	0.003%
50	7.834	2112	2113	2116	rVB2	781	207	0.02%	0.002%
51	7.860	2117	2121	2122	rBV2	601	376	0.03%	0.004%
52	8.024	2163	2172	2193	rBV	312854	547980	40.88%	5.379%
53	8.423	2294	2296	2300	rBV2	646	473	0.04%	0.005%
54	8.516	2321	2325	2327	rVB2	382	221	0.02%	0.002%
55	8.599	2349	2351	2353	rBV	559	199	0.01%	0.002%
56	8.680	2372	2376	2378	rBV2	928	599	0.04%	0.006%
57	8.786	2397	2409	2442	rBV	616498	1029891	76.84%	10.109%
58	9.095	2503	2505	2508	rBV4	495	316	0.02%	0.003%
59	9.133	2515	2517	2519	rBV2	661	316	0.02%	0.003%
60	9.223	2543	2545	2548	rVB2	499	211	0.02%	0.002%
61	9.259	2554	2556	2560	rBV3	338	224	0.02%	0.002%
62	9.355	2584	2586	2589	rVB2	638	298	0.02%	0.003%
63	9.381	2589	2594	2595	rBV3	546	313	0.02%	0.003%
64	9.480	2620	2625	2627	rBV	728	487	0.04%	0.005%
65	9.506	2631	2633	2635	rBV	381	196	0.01%	0.002%
66	9.545	2643	2645	2648	rBV	383	215	0.02%	0.002%
67	9.625	2666	2670	2672	rBV	473	355	0.03%	0.003%
68	9.648	2675	2677	2679	rBV	453	230	0.02%	0.002%
69	10.004	2787	2788	2793	rVB3	446	259	0.02%	0.003%
70	10.152	2822	2834	2857	rBV	390186	629243	46.95%	6.176%
71	10.387	2903	2907	2908	rBV2	559	345	0.03%	0.003%
72	10.474	2932	2934	2941	rBV3	539	650	0.05%	0.006%
73	10.570	2958	2964	2966	rBV2	705	523	0.04%	0.005%
74	10.583	2966	2968	2971	rBV2	347	203	0.02%	0.002%
75	10.750	3018	3020	3023	rBV2	464	231	0.02%	0.002%
76	10.767	3023	3025	3031	rBV2	368	320	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
 Data File : VV033004.D
 Acq On : 18 Nov 2023 14:35
 Operator : SY/MD
 Sample : VV1118WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK222

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

77	10.850	3048	3051	3054	rBV	413	319	0.02%	0.003%
78	11.139	3138	3141	3144	rBV	433	300	0.02%	0.003%
79	11.188	3144	3156	3177	rBV	664516	1019678	76.08%	10.009%
80	11.474	3243	3245	3248	rBV3	644	329	0.02%	0.003%
81	11.561	3260	3272	3298	rBV	676510	1072455	80.01%	10.527%
82	11.850	3358	3362	3363	rBV	381	251	0.02%	0.002%
83	11.924	3382	3385	3387	rBV	416	196	0.01%	0.002%
84	11.979	3398	3402	3403	rBV2	387	234	0.02%	0.002%
85	12.255	3485	3488	3489	rBV2	492	274	0.02%	0.003%
86	12.291	3494	3499	3504	rBV2	538	595	0.04%	0.006%
87	12.329	3509	3511	3514	rBV	398	233	0.02%	0.002%
88	12.712	3627	3630	3633	rBV2	613	465	0.03%	0.005%
89	12.901	3687	3689	3693	rBV2	392	229	0.02%	0.002%
90	12.969	3706	3710	3711	rBV2	517	318	0.02%	0.003%
91	13.088	3745	3747	3749	rBV	498	216	0.02%	0.002%
92	13.201	3780	3782	3784	rBV	469	255	0.02%	0.003%
93	13.265	3799	3802	3805	rVB2	801	498	0.04%	0.005%
94	13.445	3854	3858	3860	rBV3	486	428	0.03%	0.004%
95	13.516	3877	3880	3881	rBV2	300	199	0.01%	0.002%
96	13.583	3899	3901	3904	rVB3	939	472	0.04%	0.005%
97	13.599	3904	3906	3907	rBV	499	208	0.02%	0.002%
98	13.686	3930	3933	3936	rBV3	1013	772	0.06%	0.008%
99	14.130	4066	4071	4073	rBV3	552	601	0.04%	0.006%
100	15.030	4349	4351	4353	rBV3	887	432	0.03%	0.004%




Sum of corrected areas: 10188001

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
Data File : VV033004.D
Acq On : 18 Nov 2023 14:35
Operator : SY/MD
Sample : VV1118WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK222

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

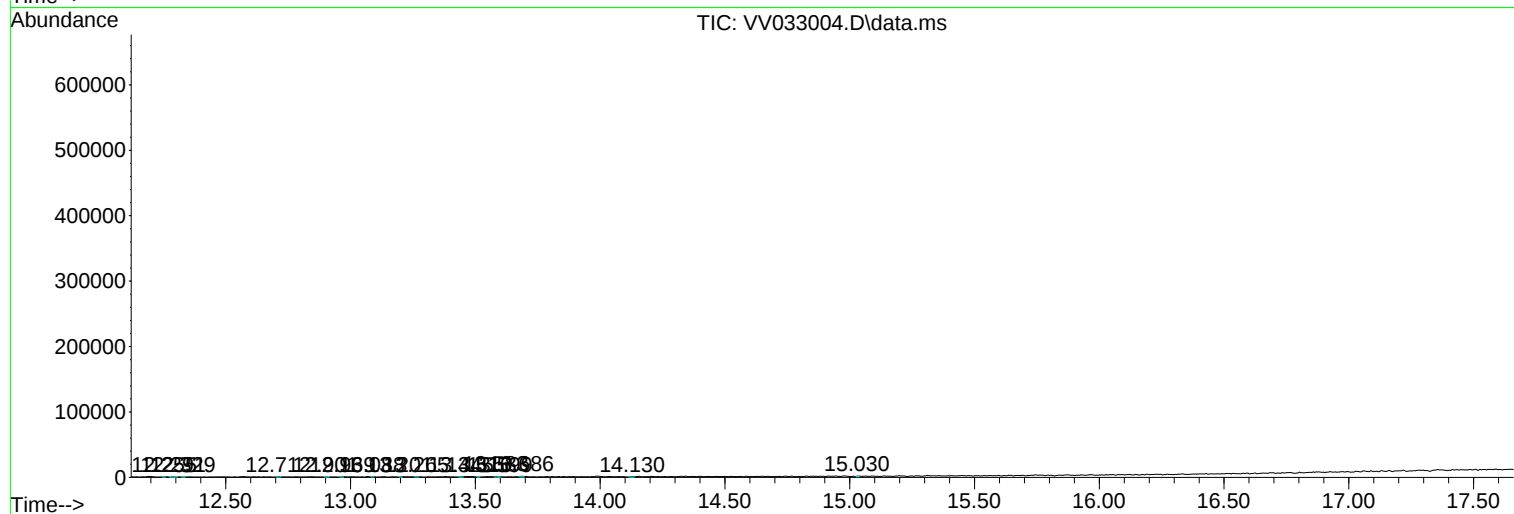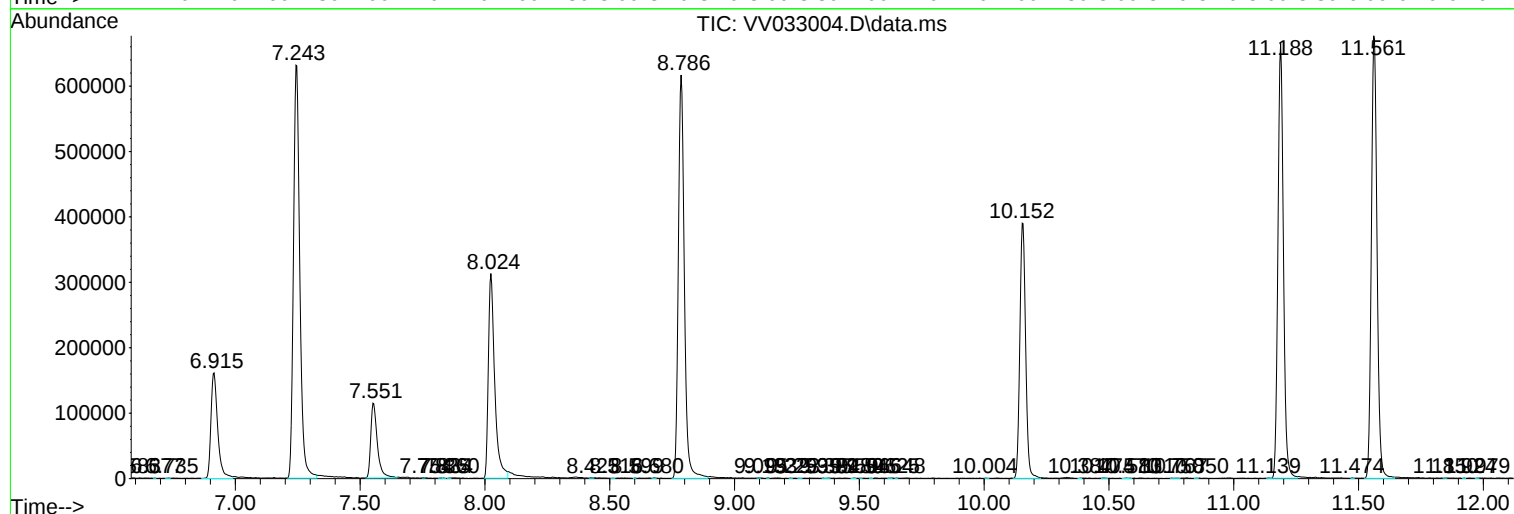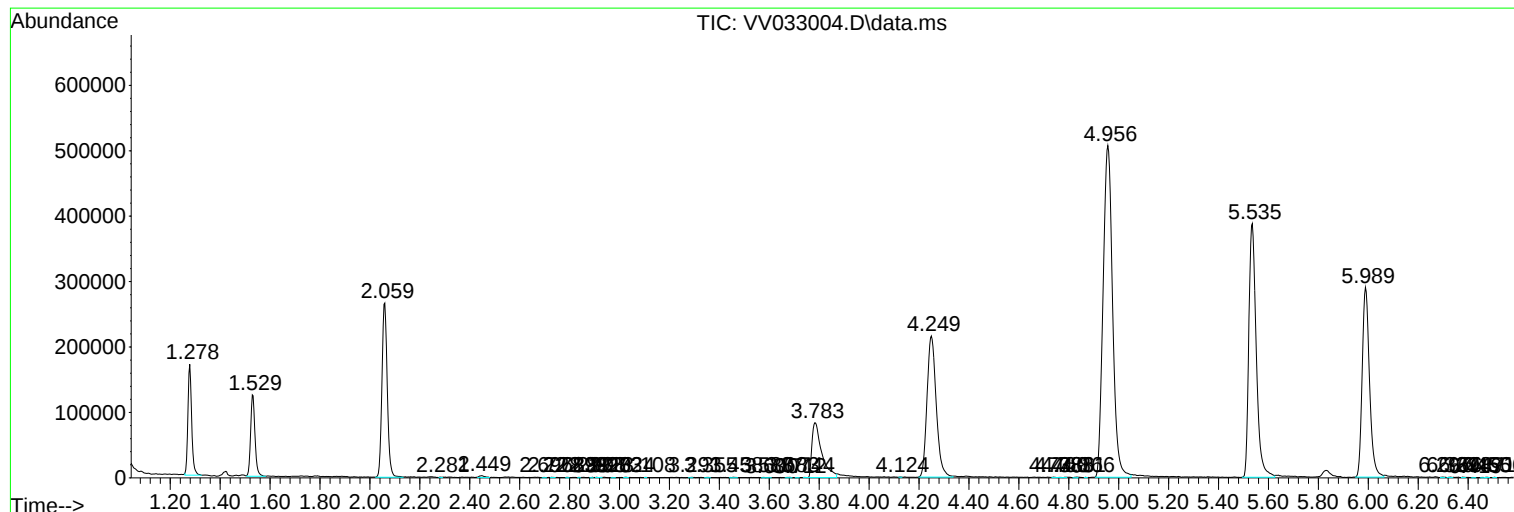

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
Data File : VV033004.D
Acq On : 18 Nov 2023 14:35
Operator : SY/MD
Sample : VV1118WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK222

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
Data File : VV033004.D
Acq On : 18 Nov 2023 14:35
Operator : SY/MD
Sample : VV1118WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK222

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc