

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
 Data File : VV033009.D
 Acq On : 18 Nov 2023 17:32
 Operator : SY/MD
 Sample : VIBLK248
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK248

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

Signal : TIC: VV033009.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	129258	135711	11.33%	1.521%
2	1.529	145	152	163	rBV	103285	121969	10.18%	1.367%
3	2.059	303	317	331	rBV	205382	301812	25.19%	3.382%
4	2.185	354	356	361	rVB3	617	281	0.02%	0.003%
5	2.217	361	366	368	rBV4	794	868	0.07%	0.010%
6	2.278	382	385	390	rVB2	662	495	0.04%	0.006%
7	2.307	392	394	398	rVV3	454	349	0.03%	0.004%
8	2.346	404	406	407	rBV3	477	224	0.02%	0.003%
9	2.449	430	438	449	rVB3	3376	5698	0.48%	0.064%
10	2.664	504	505	508	rVB	402	195	0.02%	0.002%
11	2.767	534	537	541	rVB3	344	236	0.02%	0.003%
12	2.950	591	594	595	rBV2	341	213	0.02%	0.002%
13	2.992	603	607	610	rVB	303	265	0.02%	0.003%
14	3.056	624	627	629	rBV	260	212	0.02%	0.002%
15	3.146	653	655	658	rVB	492	242	0.02%	0.003%
16	3.178	663	665	671	rVB	505	388	0.03%	0.004%
17	3.214	671	676	678	rBV2	324	304	0.03%	0.003%
18	3.362	718	722	726	rVB2	351	284	0.02%	0.003%
19	3.387	726	730	731	rBV	334	196	0.02%	0.002%
20	3.539	774	777	780	rBV3	302	199	0.02%	0.002%
21	3.558	781	783	790	rBV4	202	202	0.02%	0.002%
22	3.619	798	802	805	rBV2	291	262	0.02%	0.003%
23	3.783	843	853	890	rBV	85134	233507	19.49%	2.617%
24	4.249	982	998	1025	rBV	192941	493070	41.15%	5.526%
25	4.702	1136	1139	1140	rBV	543	241	0.02%	0.003%
26	4.744	1150	1152	1155	rBV2	398	285	0.02%	0.003%
27	4.815	1172	1174	1177	rBV2	366	191	0.02%	0.002%
28	4.847	1179	1184	1188	rVB3	435	487	0.04%	0.005%
29	4.956	1201	1218	1249	rBV2	453166	1198247	100.00%	13.428%
30	5.423	1360	1363	1365	rBV4	517	300	0.03%	0.003%
31	5.455	1371	1373	1376	rBV	351	210	0.02%	0.002%
32	5.493	1381	1385	1386	rBV2	448	341	0.03%	0.004%
33	5.535	1386	1398	1424	rBV	320749	666844	55.65%	7.473%
34	5.989	1526	1539	1565	rBV	256546	531384	44.35%	5.955%
35	6.362	1652	1655	1656	rBV	495	218	0.02%	0.002%
36	6.419	1671	1673	1675	rVB	705	324	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111823\
 Data File : VW033009.D
 Acq On : 18 Nov 2023 17:32
 Operator : SY/MD
 Sample : VIBLK248
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK248

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

37	6.442	1675	1680	1685	rBV3	447	561	0.05%	0.006%
38	6.516	1700	1703	1705	rBV	398	225	0.02%	0.003%
39	6.683	1747	1755	1757	rBV3	355	429	0.04%	0.005%
40	6.915	1816	1827	1853	rBV	143986	271448	22.65%	3.042%
41	7.243	1918	1929	1951	rBV	534504	937706	78.26%	10.508%
42	7.554	2016	2026	2044	rBV	106207	187386	15.64%	2.100%
43	7.718	2075	2077	2079	rBV2	658	277	0.02%	0.003%
44	7.831	2110	2112	2116	rBV	366	218	0.02%	0.002%
45	7.876	2119	2126	2130	rVV4	650	739	0.06%	0.008%
46	7.895	2130	2132	2135	rVB3	843	398	0.03%	0.004%
47	8.024	2162	2172	2197	rBV	305534	543874	45.39%	6.095%
48	8.371	2271	2280	2285	rBV6	1566	3012	0.25%	0.034%
49	8.558	2336	2338	2341	rBV2	415	269	0.02%	0.003%
50	8.583	2344	2346	2349	rBV	350	233	0.02%	0.003%
51	8.744	2393	2396	2398	rBV2	541	364	0.03%	0.004%
52	8.786	2398	2409	2436	rBV	537585	868401	72.47%	9.732%
53	9.024	2480	2483	2486	rBV2	853	468	0.04%	0.005%
54	9.098	2501	2506	2508	rBV4	461	394	0.03%	0.004%
55	9.133	2515	2517	2520	rBV	404	195	0.02%	0.002%
56	9.162	2524	2526	2529	rBV2	369	210	0.02%	0.002%
57	9.201	2536	2538	2541	rBV2	452	336	0.03%	0.004%
58	9.394	2594	2598	2602	rBV2	371	341	0.03%	0.004%
59	9.458	2613	2618	2622	rBV2	458	417	0.03%	0.005%
60	9.622	2665	2669	2671	rBV2	364	272	0.02%	0.003%
61	9.760	2708	2712	2713	rBV	422	240	0.02%	0.003%
62	9.815	2723	2729	2731	rBV2	851	492	0.04%	0.006%
63	9.828	2731	2733	2735	rVB	453	209	0.02%	0.002%
64	9.940	2765	2768	2771	rVB3	422	322	0.03%	0.004%
65	9.959	2771	2774	2776	rBV2	258	193	0.02%	0.002%
66	9.982	2776	2781	2784	rBV2	592	390	0.03%	0.004%
67	10.085	2811	2813	2816	rBV2	354	217	0.02%	0.002%
68	10.152	2820	2834	2860	rBV	387079	613448	51.20%	6.875%
69	10.329	2886	2889	2890	rBV	684	408	0.03%	0.005%
70	10.422	2911	2918	2924	rBV2	378	407	0.03%	0.005%
71	10.451	2925	2927	2931	rVB2	410	291	0.02%	0.003%
72	10.480	2931	2936	2937	rBV2	464	346	0.03%	0.004%
73	10.857	3047	3053	3056	rBV4	451	608	0.05%	0.007%
74	10.976	3088	3090	3095	rVB2	344	229	0.02%	0.003%
75	11.188	3144	3156	3177	rBV	541663	847869	70.76%	9.502%
76	11.403	3221	3223	3225	rBV	705	339	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111823\
 Data File : VV033009.D
 Acq On : 18 Nov 2023 17:32
 Operator : SY/MD
 Sample : VIBLK248
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK248

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

77	11.429	3228	3231	3234	rBV2	407	235	0.02%	0.003%
78	11.442	3234	3235	3238	rBV2	414	228	0.02%	0.003%
79	11.564	3260	3273	3295	rBV	591159	936304	78.14%	10.493%
80	11.866	3362	3367	3369	rBV2	478	339	0.03%	0.004%
81	11.902	3376	3378	3382	rVB3	538	230	0.02%	0.003%
82	11.921	3382	3384	3386	rBV	520	273	0.02%	0.003%
83	11.950	3390	3393	3395	rBV	493	292	0.02%	0.003%
84	12.024	3412	3416	3420	rBV2	430	346	0.03%	0.004%
85	12.053	3423	3425	3427	rBV	376	223	0.02%	0.002%
86	12.181	3463	3465	3467	rBV2	596	344	0.03%	0.004%
87	12.358	3518	3520	3524	rBV	355	252	0.02%	0.003%
88	12.461	3549	3552	3556	rBV2	357	240	0.02%	0.003%
89	12.647	3608	3610	3613	rVB	570	295	0.02%	0.003%
90	12.828	3663	3666	3668	rBV2	310	244	0.02%	0.003%
91	13.062	3736	3739	3741	rBV	448	234	0.02%	0.003%
92	13.130	3757	3760	3762	rBV2	386	258	0.02%	0.003%
93	13.143	3762	3764	3767	rVB2	560	274	0.02%	0.003%
94	13.165	3767	3771	3772	rBV2	494	292	0.02%	0.003%
95	13.406	3842	3846	3851	rBV5	554	430	0.04%	0.005%
96	13.432	3851	3854	3857	rBV4	484	338	0.03%	0.004%
97	13.866	3987	3989	3990	rBV4	626	225	0.02%	0.003%
98	14.319	4128	4130	4132	rVB2	732	230	0.02%	0.003%
99	14.355	4138	4141	4145	rBV3	698	532	0.04%	0.006%
100	14.737	4259	4260	4261	rBV	700	244	0.02%	0.003%




Sum of corrected areas: 8923337

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
Data File : VV033009.D
Acq On : 18 Nov 2023 17:32
Operator : SY/MD
Sample : VIBLK248
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK248

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

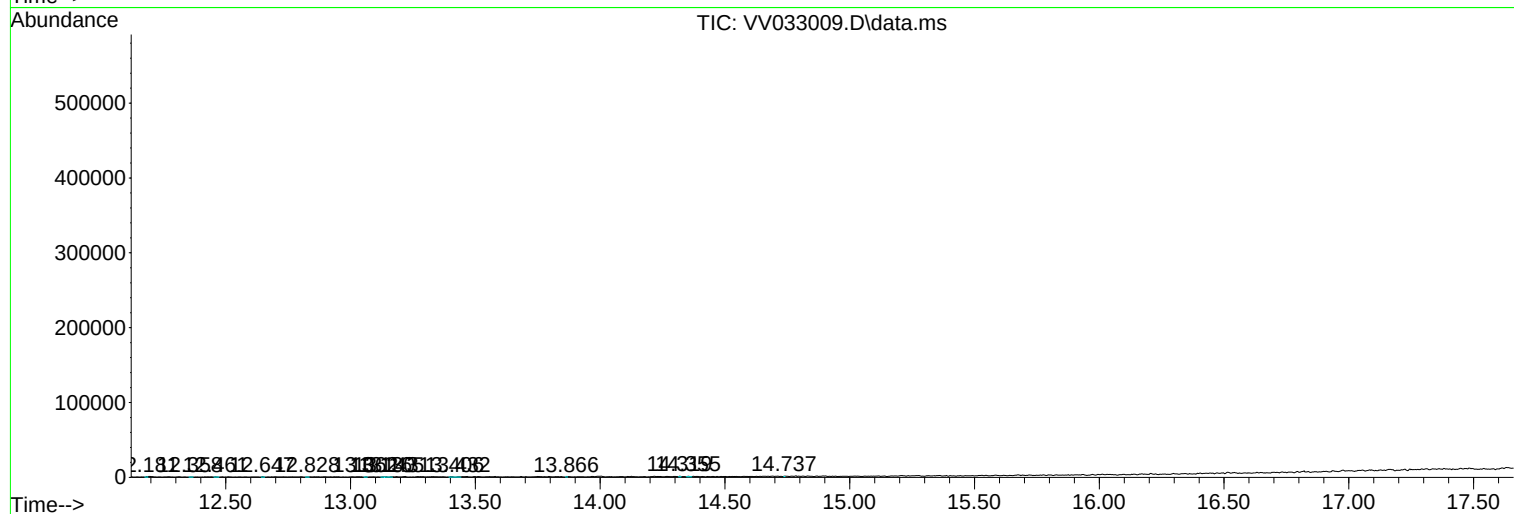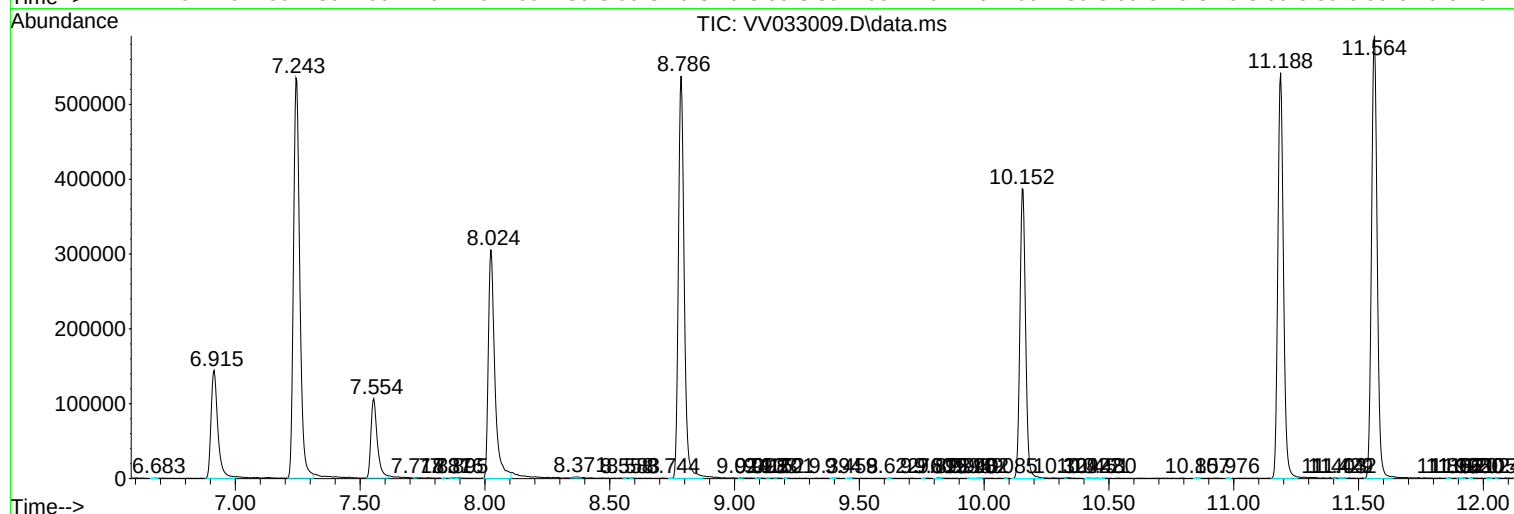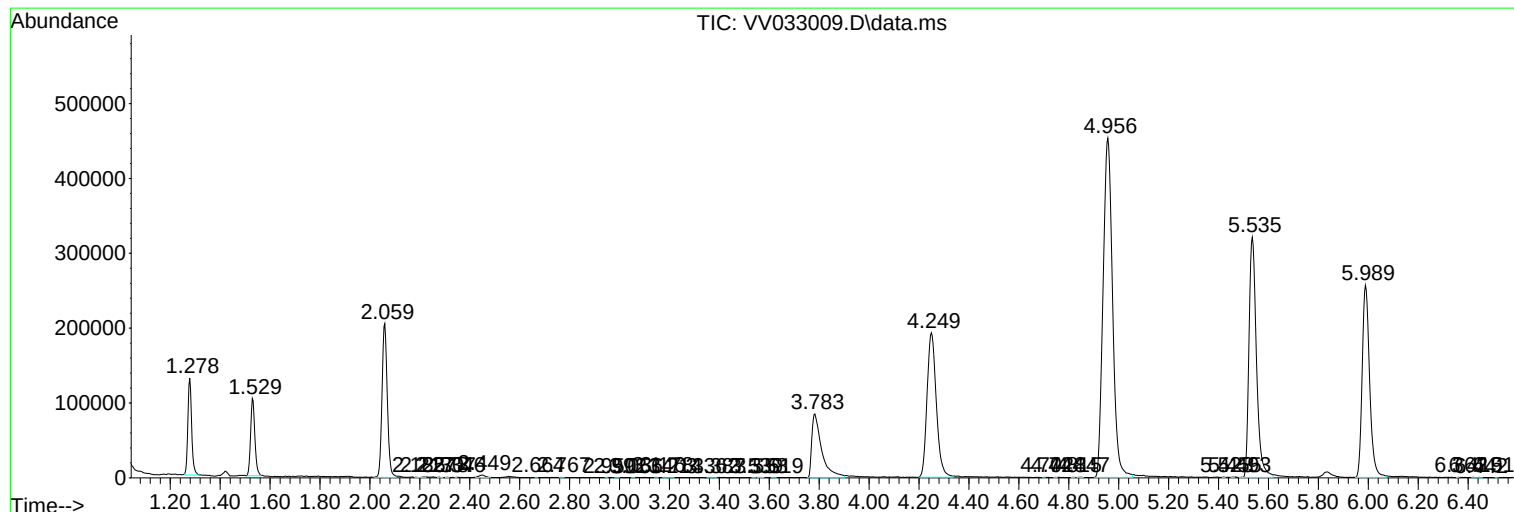

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
Data File : VV033009.D
Acq On : 18 Nov 2023 17:32
Operator : SY/MD
Sample : VIBLK248
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK248

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
Data File : VV033009.D
Acq On : 18 Nov 2023 17:32
Operator : SY/MD
Sample : VIBLK248
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK248

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc