


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111823\
Data File : VV033000.D
Acq On : 18 Nov 2023 08:54
Operator : SY/MD
Sample : BFB233
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB233

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Title : VOC Analysis
Last Update : Mon Nov 20 01:19:10 2023

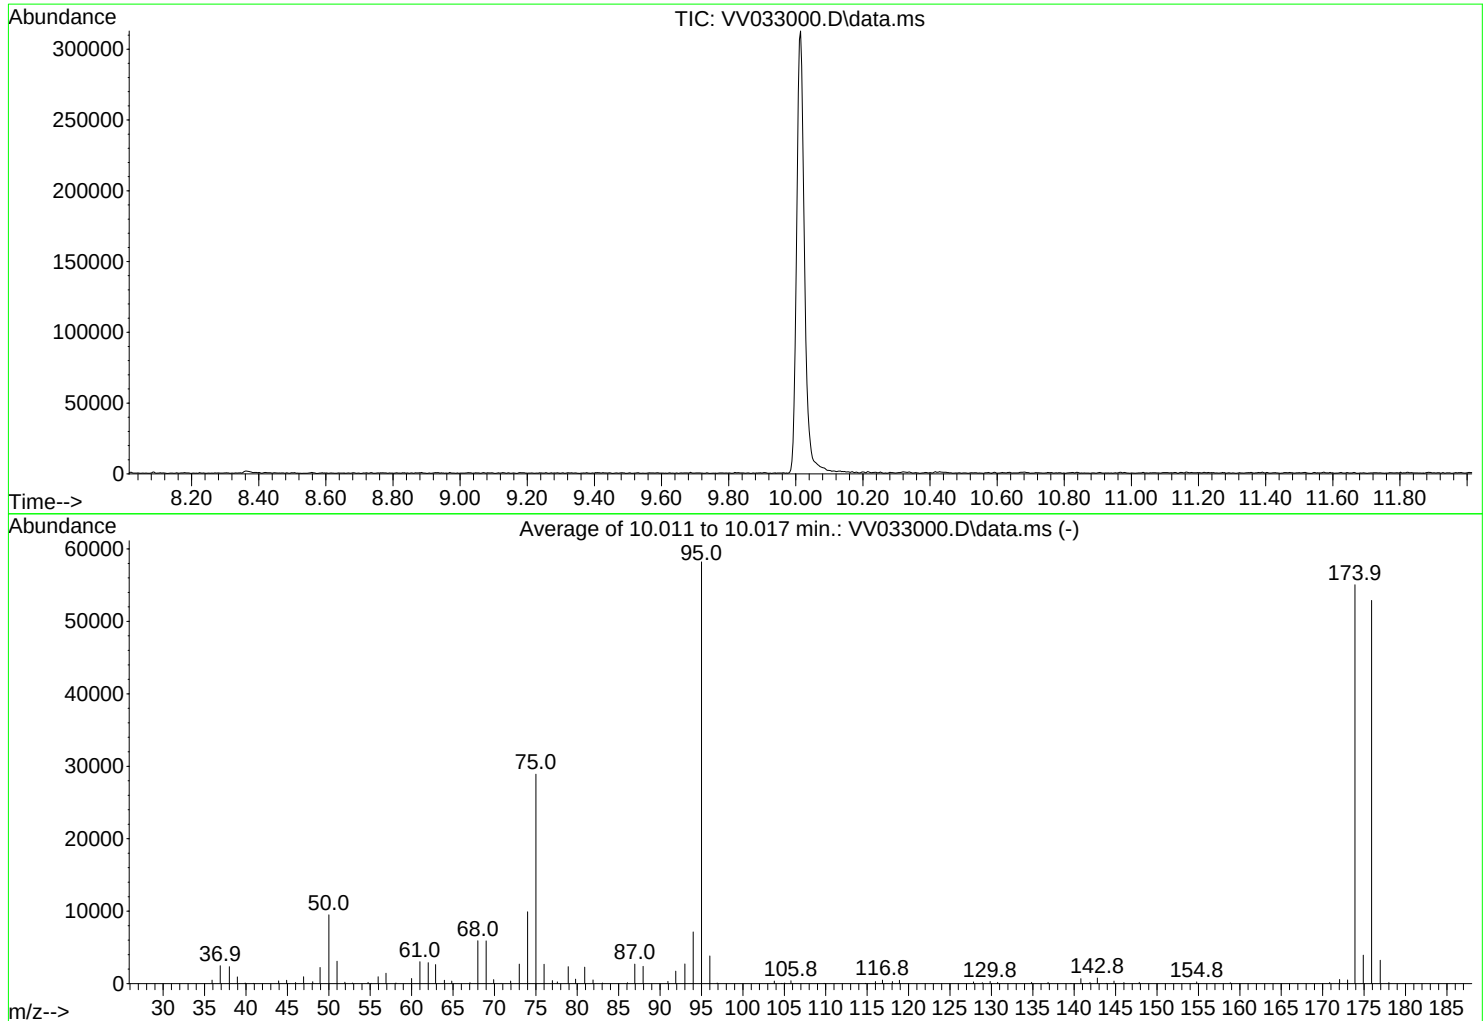

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	9488	PASS
75	95	30	80	49.7	28915	PASS
95	95	100	100	100.0	58216	PASS
96	95	5	9	6.5	3812	PASS
173	174	0.00	2	0.9	507	PASS
174	95	50	120	94.6	55064	PASS
175	174	5	9	7.2	3940	PASS
176	174	95	105	96.1	52896	PASS
177	176	5	10	6.1	3216	PASS

m/z	Abundance
39.90	184.0
43.90	277.0

Instrument :
MSVOA_V
ClientSampleId :
BFB233

m/z	Abundance
35.90	550.0
36.90	2521.0
38.00	2232.0
39.00	934.0
40.00	238.0
44.00	563.0
44.90	453.0
46.00	166.0
47.00	987.0
48.00	285.0
48.90	2341.0
50.00	9894.0
51.00	3280.0
52.00	200.0
54.70	182.0
55.10	136.0
55.90	978.0
56.90	1562.0
58.10	124.0
60.00	795.0
61.00	3089.0
62.00	2923.0
62.90	2697.0
63.90	517.0
64.80	364.0
67.00	136.0
68.00	5810.0
69.00	5758.0
69.90	541.0
72.00	359.0
73.00	2736.0
74.00	10294.0
75.00	28904.0
76.00	2866.0
77.00	396.0
77.60	215.0
78.90	2396.0
79.80	615.0
80.90	2433.0
81.90	523.0
83.00	136.0
86.10	117.0
86.90	2630.0
87.90	2423.0
90.90	390.0
91.90	1644.0
93.00	2816.0
94.00	7340.0
95.00	59776.0
96.00	4008.0
96.90	144.0
103.80	348.0
105.10	135.0
105.70	373.0
114.80	105.0
116.00	324.0
116.80	472.0
118.00	276.0
118.90	456.0
127.80	248.0
128.90	118.0
129.80	292.0
130.80	191.0
134.90	201.0
136.80	204.0
140.80	766.0
141.90	173.0
142.80	839.0
144.90	340.0
146.00	151.0
147.80	198.0
154.80	212.0
158.90	114.0
170.80	194.0
172.00	510.0
173.00	736.0
173.90	55472.0
174.90	3913.0
175.90	52632.0
177.00	3177.0
178.00	192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB233

m/z	Abundance
35.90	496.0
36.90	2597.0
38.00	2443.0
39.00	949.0
39.90	267.0
44.00	666.0
44.90	460.0
46.00	159.0
46.90	961.0
48.10	262.0
48.90	2285.0
50.00	9738.0
51.00	3180.0
52.00	199.0
52.80	134.0
54.70	198.0
55.90	1000.0
56.90	1470.0
58.10	109.0
60.00	743.0
61.00	3158.0
62.00	3005.0
62.90	2734.0
63.90	481.0
64.90	350.0
67.10	132.0
68.00	6149.0
69.00	6101.0
69.90	564.0
72.00	380.0
73.00	2760.0
74.00	10199.0
75.00	29688.0
76.00	2758.0
77.00	443.0
77.60	261.0
78.90	2434.0
79.80	647.0
80.90	2278.0
81.90	514.0
83.10	142.0
86.10	129.0
86.90	2795.0
87.90	2514.0
91.00	317.0
91.90	1781.0
93.00	2792.0
94.00	7352.0
95.00	60208.0
96.00	3951.0
96.90	104.0
103.80	368.0
105.00	110.0
105.80	391.0
116.00	299.0
116.90	525.0
118.10	306.0
118.90	463.0
127.90	254.0
128.90	153.0
129.90	316.0
130.80	188.0
134.90	169.0
136.90	175.0
139.60	102.0
140.80	687.0
141.90	164.0
142.80	788.0
143.90	103.0
144.80	357.0
146.00	175.0
147.80	169.0
154.80	262.0
158.80	138.0
170.90	162.0
172.10	605.0
173.00	786.0
173.90	56992.0
174.90	4021.0
175.90	54712.0
177.00	3311.0
178.00	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB233

m/z	Abundance
35.90	399.0
36.90	2304.0
38.00	2367.0
38.90	880.0
39.90	320.0
40.90	108.0
44.00	715.0
44.90	471.0
46.00	114.0
46.90	880.0
48.00	220.0
49.00	2085.0
50.00	8831.0
51.00	2817.0
51.90	205.0
52.90	127.0
54.80	184.0
56.00	892.0
56.90	1259.0
60.00	605.0
61.00	2814.0
62.00	2738.0
62.90	2476.0
64.00	408.0
64.80	364.0
67.10	154.0
68.00	5814.0
69.00	5837.0
69.90	520.0
70.80	120.0
71.90	334.0
73.00	2573.0
74.00	9273.0
75.00	28152.0
76.00	2372.0
77.00	451.0
77.60	280.0
78.90	2216.0
79.80	629.0
80.90	2095.0
81.90	479.0
86.00	154.0
87.00	2627.0
88.00	2204.0
90.90	244.0
91.90	1779.0
93.00	2509.0
94.00	6736.0
95.00	54664.0
96.00	3478.0
103.80	349.0
104.70	145.0
105.90	405.0
109.80	105.0
116.00	227.0
116.90	475.0
118.10	268.0
118.90	449.0
127.90	202.0
128.90	158.0
129.90	297.0
130.70	139.0
134.80	146.0
136.90	124.0
140.80	592.0
141.90	162.0
142.80	685.0
144.70	357.0
146.00	150.0
147.90	160.0
154.80	291.0
158.80	159.0
170.90	123.0
172.10	632.0
173.90	52728.0
174.90	3886.0
175.90	51344.0
176.90	3160.0
178.00	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB233