




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111824\
Data File : VV038161.D
Acq On : 18 Nov 2024 08:53
Operator : SY/MD
Sample : VSTDCCC0.5
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
LabSampleId :
VSTDCCC0.5

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:06:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/19/2024
Supervised By :Mahesh Dadoda 11/19/2024

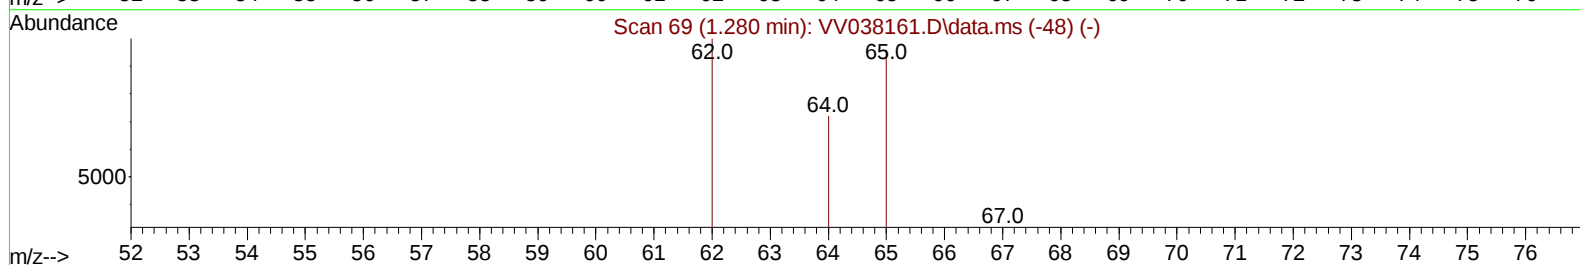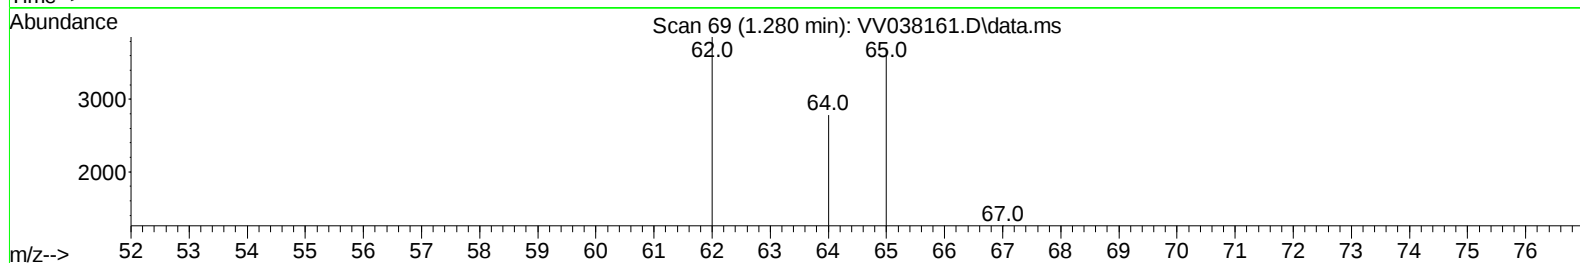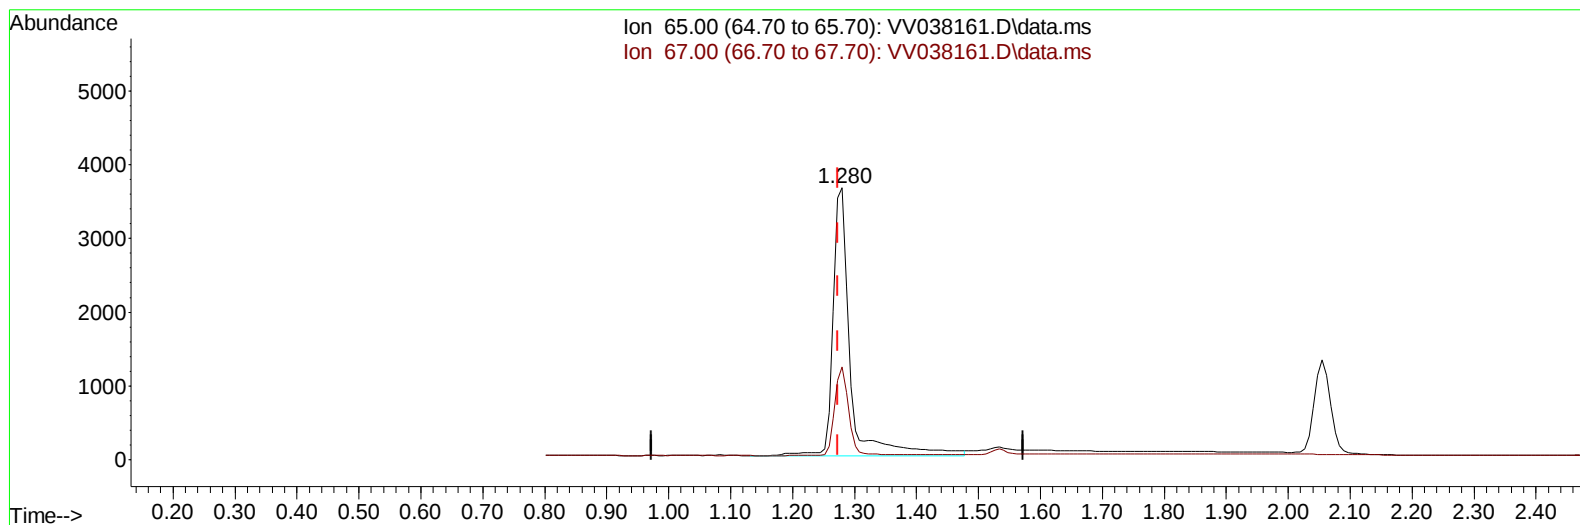

TIC: VV038161.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.280min (+ 0.007) 0.67 ug/L

response 7032

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	33.70	26.95
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111824\
Data File : VV038161.D
Acq On : 18 Nov 2024 08:53
Operator : SY/MD
Sample : VSTDCCC0.5
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
LabSampleId :
VSTDCCC0.5

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:06:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/19/2024
Supervised By :Mahesh Dadoda 11/19/2024

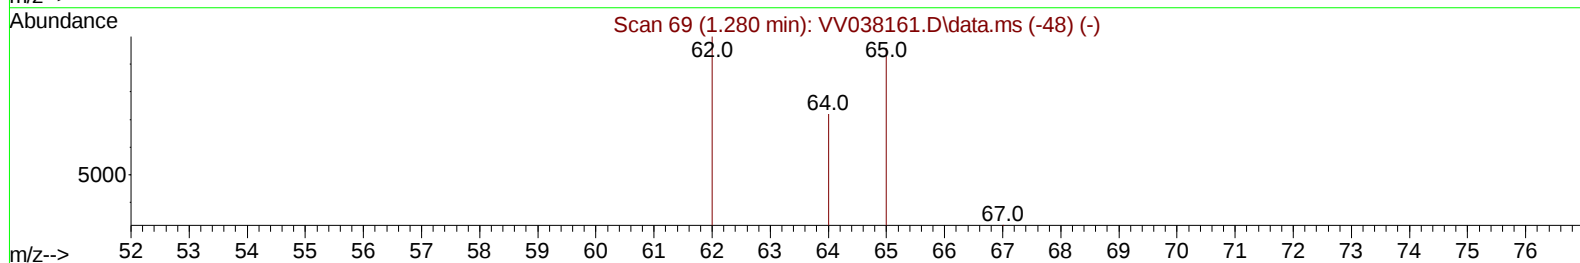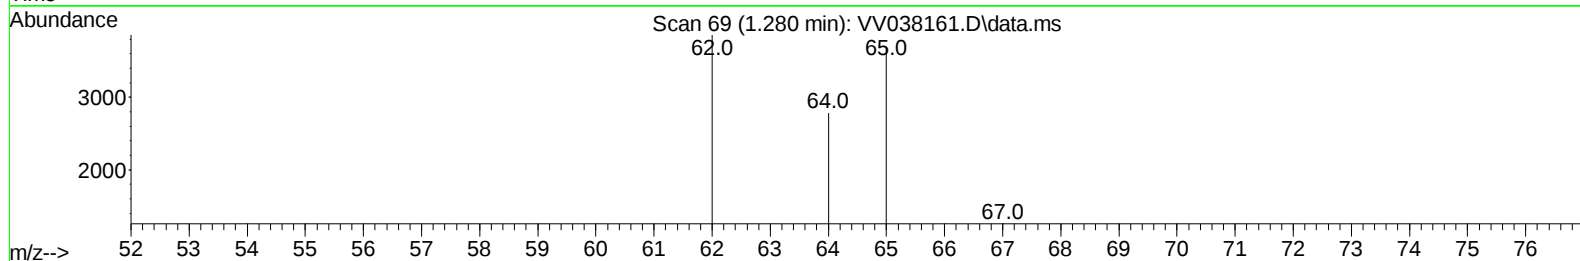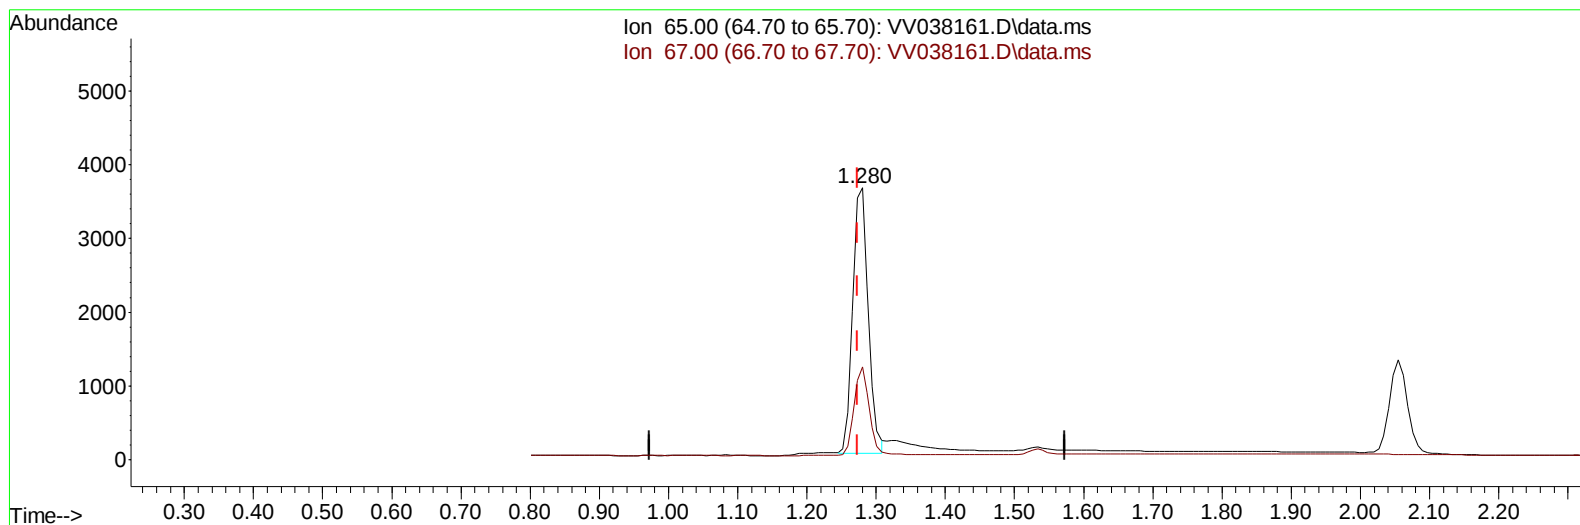

TIC: VV038161.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.280min (+ 0.007) 0.54 ug/L m

response 5600

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	33.70	33.84
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111824\
 Data File : VV038161.D
 Acq On : 18 Nov 2024 08:53
 Operator : SY/MD
 Sample : VSTDCCC0.5
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 LabSampleId :
 VSTDCCC0.5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/19/2024
 Supervised By :Mahesh Dadoda 11/19/2024

Quant Time: Nov 19 00:06:12 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	10085	0.500	ug/L	-0.02
5) Chlorobenzene-d5	8.785	117	10104	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	4982	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	5600m	0.536	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 108.000%			
4) 1,2-Dichloroethane-d4	4.945	65	3334	0.527	ug/L	-0.02
Spiked Amount 0.500	Range 70 - 130		Recovery = 106.000%			
7) 1,2-Dichloropropane-d6	5.995	67	4130	0.505	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 100.000%			
8) Toluene-d8	7.253	98	10386	0.496	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 100.000%			
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3274	0.500	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 100.000%			
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.280	62	5844	0.562	ug/L #	39
6) Trichloroethene	5.852	95	3775	0.511	ug/L	99
9) 1,2-Dibromoethane	8.305	107	2534	0.496	ug/L	99
12) 1,2,3-Trichloropropane	10.197	75	2131	0.489	ug/L	99
13) 1,2-Dibromo-3-chloropr...	12.356	75	414	0.480	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111824\
Data File : VV038161.D
Acq On : 18 Nov 2024 08:53
Operator : SY/MD
Sample : VSTDCCC0.5
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
LabSampleId :
VSTDCCC0.5

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:06:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/19/2024
Supervised By :Mahesh Dadoda 11/19/2024

