
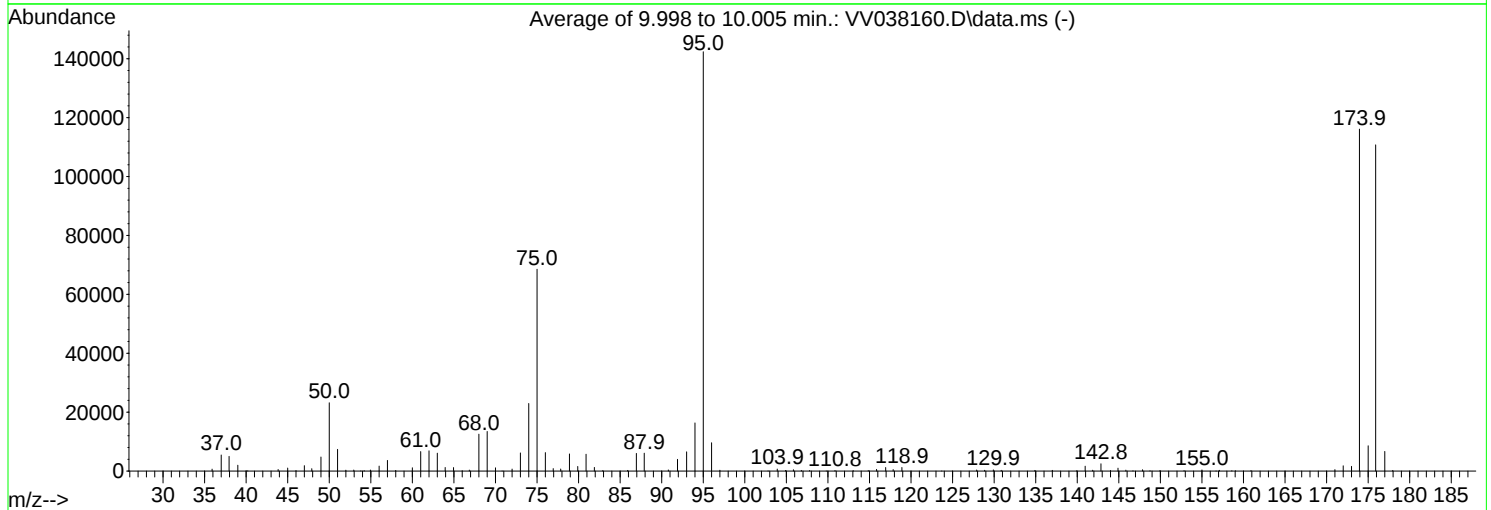


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111824\
Data File : VV038160.D
Acq On : 18 Nov 2024 08:23
Operator : SY/MD
Sample : BFB225
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB225

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Title : TRACE VOA SOM01.0
Last Update : Fri Nov 15 00:15:53 2024

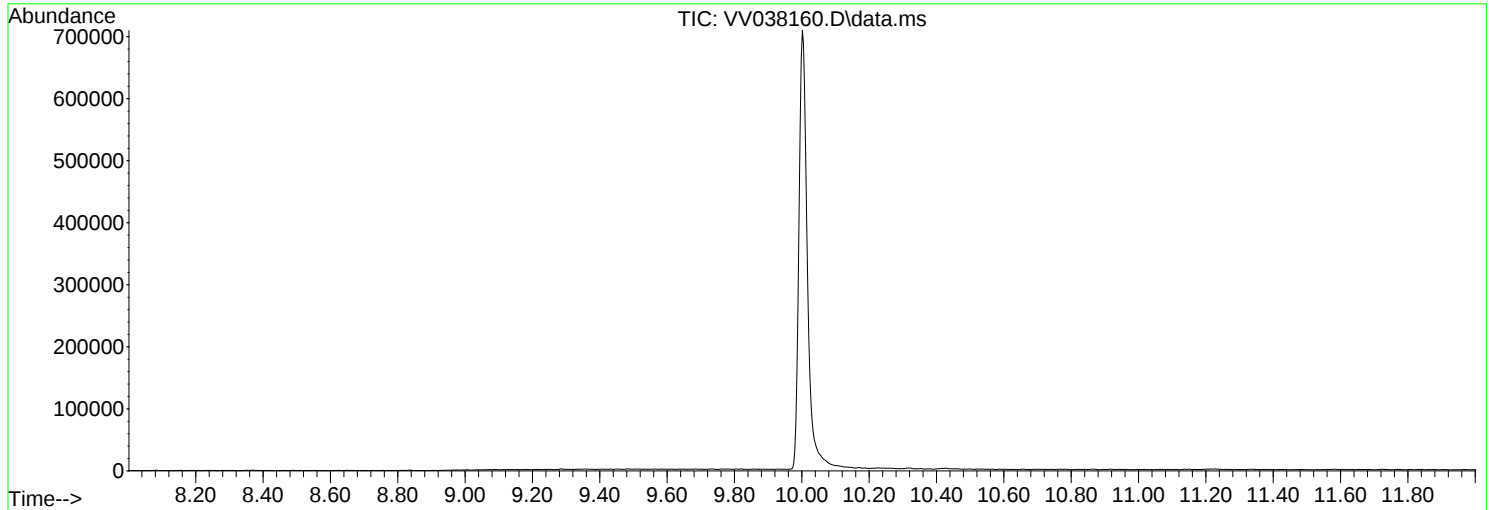

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2774

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	23189	PASS
75	95	30	80	48.1	68528	PASS
95	95	100	100	100.0	142379	PASS
96	95	5	9	6.8	9625	PASS
173	174	0.00	2	1.4	1603	PASS
174	95	50	120	81.5	116109	PASS
175	174	5	9	7.4	8586	PASS
176	174	95	101	95.4	110757	PASS
177	176	5	9	6.0	6675	PASS

m/z	Abundance
35.90	1349.0
37.10	160.0
38.00	487.0
40.10	195.0
43.80	387.0
76.80	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225

m/z	Abundance
36.00	2019.0
37.00	5739.0
37.90	5454.0
39.00	1995.0
40.00	390.0
43.90	891.0
45.00	1024.0
46.00	218.0
47.00	1913.0
47.90	806.0
49.00	4625.0
50.00	22296.0
51.00	7131.0
52.00	318.0
52.90	201.0
53.80	165.0
54.90	419.0
56.00	1738.0
57.00	3787.0
57.90	218.0
60.00	1040.0
61.00	6244.0
62.00	6494.0
63.00	5708.0
64.00	1313.0
65.00	928.0
66.90	284.0
68.00	12154.0
69.00	13174.0
70.00	1110.0
70.80	109.0
72.00	726.0
73.00	5847.0
74.00	22336.0
75.00	67200.0
76.00	6329.0
77.00	986.0
77.90	667.0
78.90	5834.0
79.90	1330.0
80.90	5789.0
81.90	1135.0
82.90	148.0
85.80	242.0
86.90	5964.0
87.90	5602.0
90.80	427.0
91.90	4029.0
93.00	6455.0
94.00	15778.0
95.00	138688.0
96.00	10031.0
97.00	285.0
102.80	115.0
103.90	705.0
104.90	189.0
105.80	534.0
106.80	197.0
107.80	181.0
110.90	187.0
113.00	148.0
114.90	188.0
115.80	574.0
117.00	1315.0
117.80	497.0
118.90	1114.0
127.90	406.0
128.80	258.0
129.90	430.0
130.80	222.0
134.80	197.0
137.00	305.0
139.90	141.0
141.00	1607.0
141.80	276.0
142.90	2334.0
144.10	179.0
144.90	955.0
145.80	323.0
147.80	466.0
148.80	112.0
150.00	175.0
152.80	144.0
155.00	343.0
156.70	119.0
157.10	228.0
158.60	110.0
160.80	137.0
171.00	451.0
172.00	1816.0
173.00	1481.0
173.90	110048.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225

175.00	8393.0
175.90	105184.0
177.00	6514.0
177.90	219.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225

m/z	Abundance
36.00	2042.0
37.00	5776.0
37.90	5522.0
39.00	2036.0
40.00	341.0
43.90	947.0
45.00	1073.0
46.00	183.0
47.00	1880.0
47.90	845.0
49.00	4915.0
50.00	24088.0
51.00	7609.0
52.00	300.0
52.90	218.0
53.00	218.0
53.80	115.0
54.20	196.0
54.90	358.0
56.00	1721.0
57.00	3760.0
58.00	214.0
60.00	1143.0
61.00	6872.0
62.00	7088.0
63.00	6283.0
63.90	1264.0
64.90	1202.0
66.00	117.0
66.90	340.0
68.00	12831.0
69.00	13921.0
70.00	1157.0
72.00	701.0
73.00	6286.0
74.00	23680.0
75.00	70648.0
76.00	6512.0
77.00	1007.0
77.90	741.0
78.90	6015.0
79.90	1618.0
80.90	5896.0
81.90	1278.0
82.90	158.0
85.90	221.0
87.00	6194.0
87.90	6376.0
90.80	395.0
91.90	4107.0
93.00	6820.0
94.00	16936.0
95.00	146880.0
96.00	9852.0
97.00	302.0
102.80	110.0
103.90	710.0
104.90	233.0
105.90	464.0
106.80	242.0
107.80	211.0
110.90	204.0
113.00	151.0
114.80	191.0
115.90	592.0
116.90	1282.0
117.90	548.0
118.90	1286.0
127.90	365.0
128.90	290.0
129.90	432.0
130.90	271.0
134.90	225.0
137.00	262.0
139.90	135.0
140.90	1717.0
141.80	325.0
142.80	2537.0
144.00	197.0
144.90	1066.0
145.80	332.0
146.70	110.0
147.90	486.0
148.70	110.0
149.90	173.0
152.80	161.0
155.00	417.0
157.10	286.0
158.60	161.0
159.00	112.0
160.90	149.0
171.00	530.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225

172.00	1793.0
173.00	1652.0
173.90	119816.0
175.00	8796.0
175.90	114376.0
177.00	6853.0
177.90	205.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225

m/z	Abundance
36.00	2010.0
37.00	5336.0
38.00	5479.0
39.00	1921.0
40.20	290.0
43.90	960.0
45.00	1021.0
46.00	115.0
47.00	1735.0
47.90	789.0
49.00	4798.0
50.00	23184.0
51.00	7352.0
52.00	296.0
52.80	224.0
53.10	238.0
54.20	245.0
55.00	319.0
56.00	1604.0
57.00	3321.0
58.10	226.0
60.00	1210.0
61.00	6759.0
62.00	7052.0
63.00	6263.0
64.00	1096.0
64.90	1441.0
66.00	154.0
66.80	397.0
68.00	12607.0
69.00	13254.0
70.00	1077.0
72.00	612.0
73.00	6363.0
74.00	22840.0
75.00	67736.0
76.00	6015.0
77.00	896.0
77.80	723.0
78.90	5644.0
79.90	1766.0
80.90	5484.0
81.90	1314.0
82.90	134.0
86.00	245.0
86.90	5859.0
87.90	6262.0
90.80	366.0
91.90	3808.0
93.00	6349.0
94.00	16354.0
95.00	141568.0
96.00	8992.0
97.00	279.0
103.90	663.0
104.90	245.0
105.90	403.0
106.80	275.0
107.80	205.0
109.80	109.0
110.80	215.0
113.10	126.0
114.90	155.0
115.90	570.0
116.90	1047.0
117.90	560.0
118.90	1278.0
123.70	107.0
127.90	354.0
128.90	309.0
129.90	393.0
130.90	286.0
135.00	280.0
137.00	174.0
140.90	1689.0
141.90	301.0
142.90	2575.0
143.90	173.0
144.90	989.0
145.90	330.0
146.70	178.0
147.90	422.0
148.70	121.0
149.90	155.0
152.90	148.0
155.00	403.0
157.10	271.0
158.60	153.0
159.10	143.0
161.00	184.0
171.00	556.0
172.00	1798.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225

173.00	1676.0
174.00	118464.0
175.00	8568.0
175.90	112712.0
177.00	6658.0
178.00	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225