




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
 Data File : VV038174.D
 Acq On : 19 Nov 2024 13:17
 Operator : SY/MD
 Sample : VSTD0.519
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 19 21:34:01 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
 Supervised By :Semsettin Yesilyurt 11/21/2024

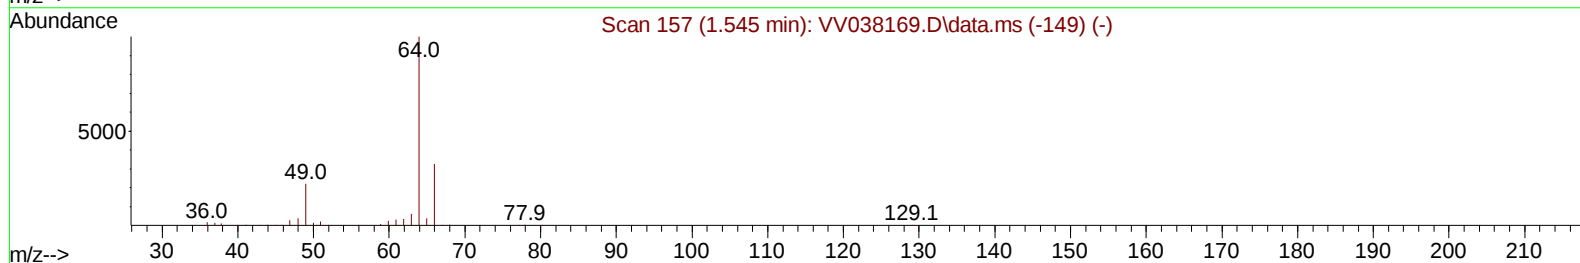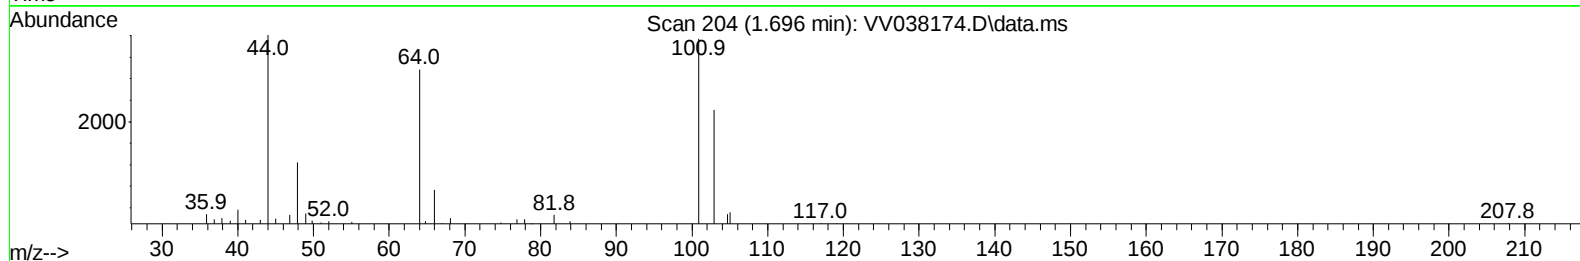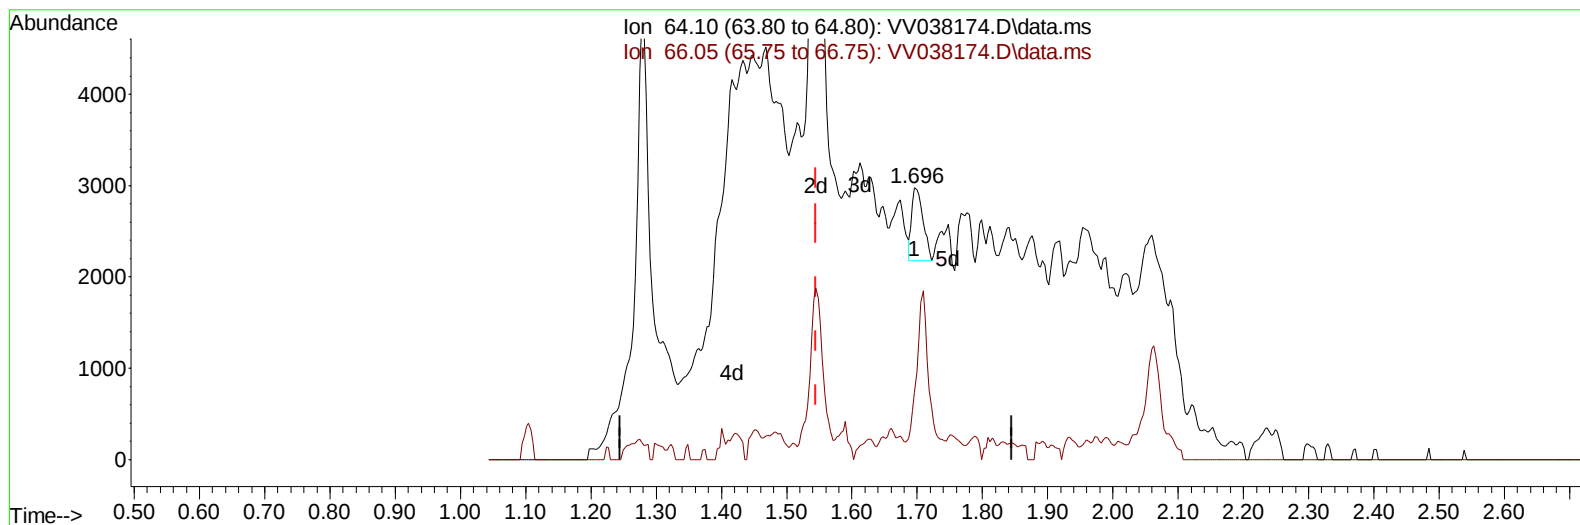

TIC: VV038174.D\data.ms

(8) Chloroethane (T)

1.696min (+ 0.151) 0.06 ug/L

response 956

Ion	Exp%	Act%
64.10	100.00	100.00
66.05	31.40	23.49
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

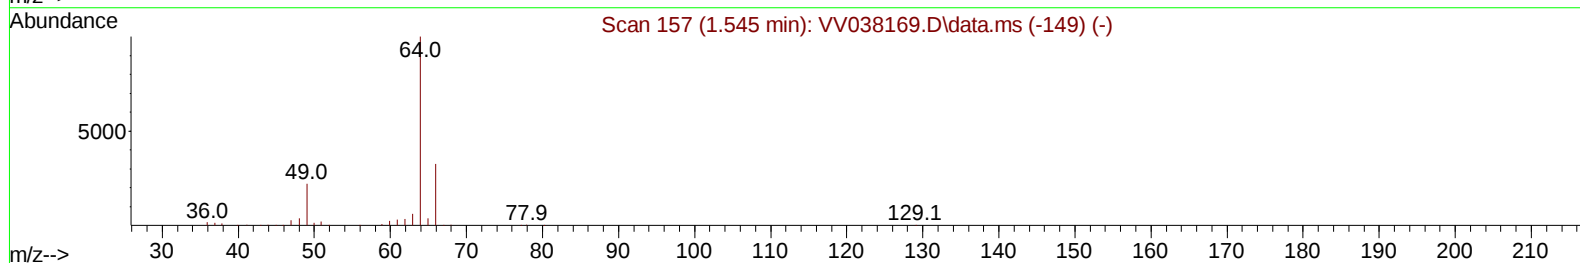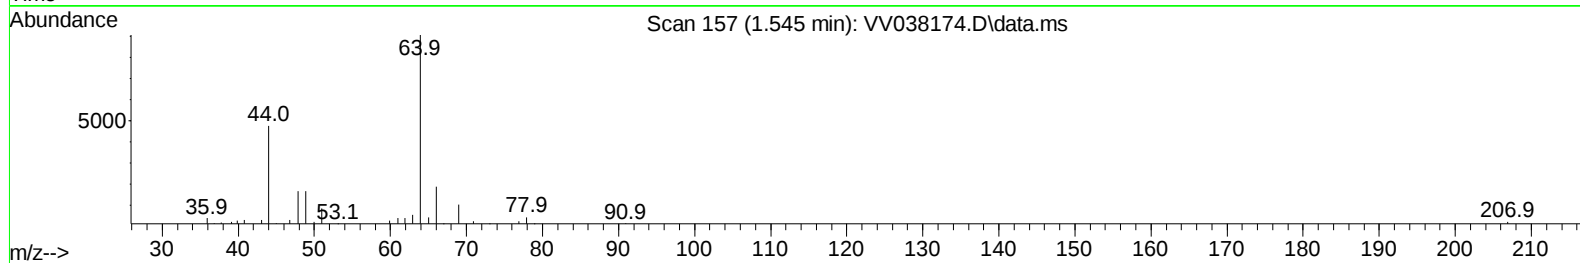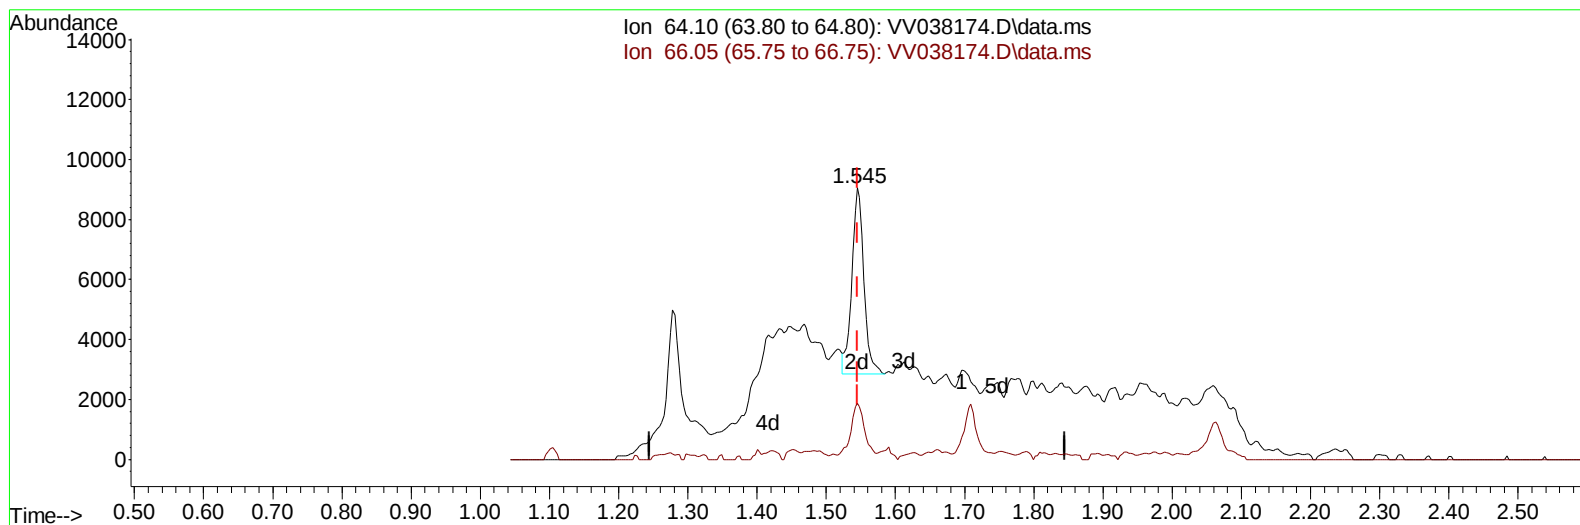

TIC: VV038174.D\data.ms

(8) Chloroethane (T)

1.545min (-0.000) 0.45 ug/L m

response 7559

Ion	Exp%	Act%
64.10	100.00	100.00
66.05	31.40	20.73#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

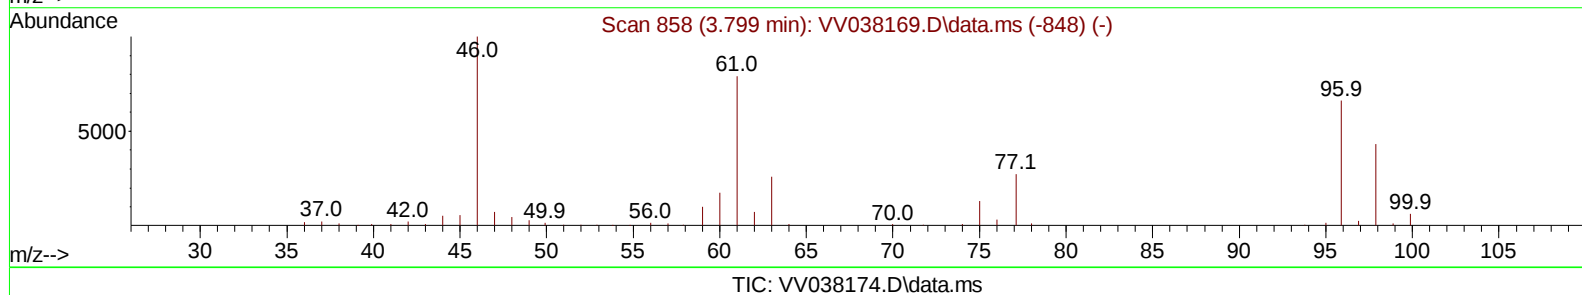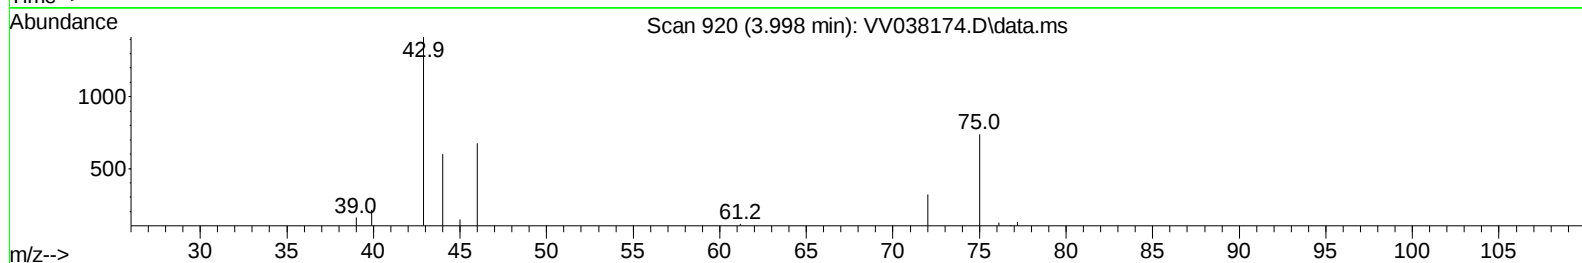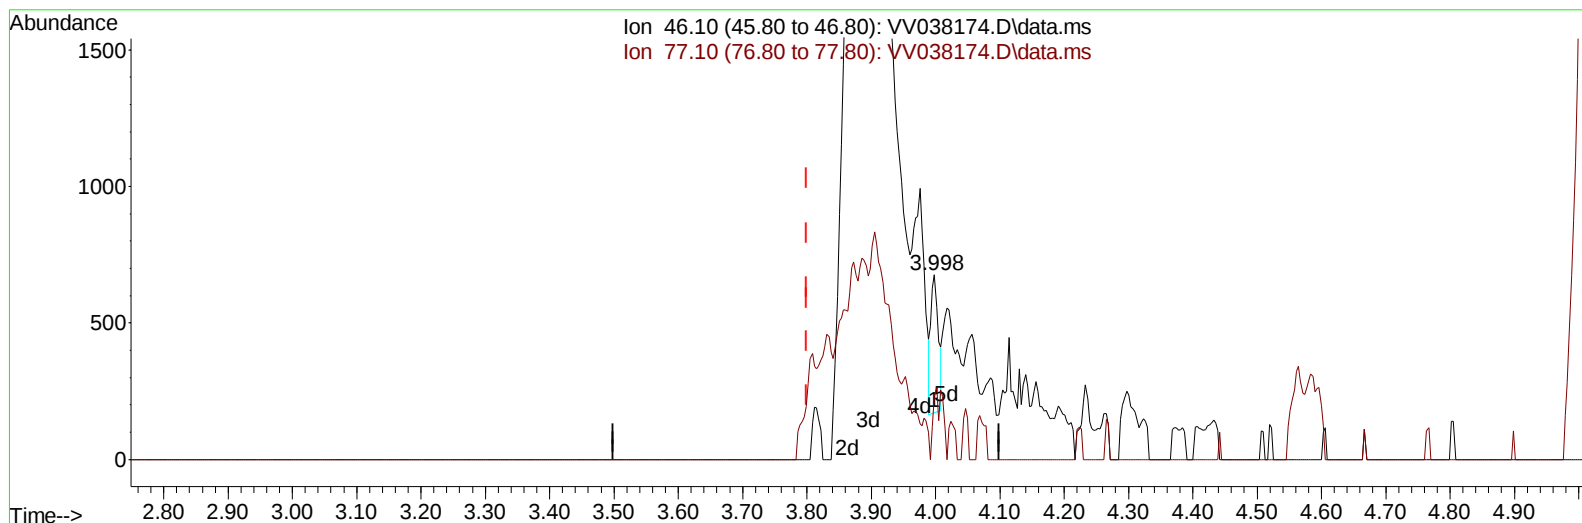

(20) 2-Butanone-d5 (S)

3.998min (+ 0.199) 0.11 ug/L

response 416

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	27.40	35.10
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
 Data File : VV038174.D
 Acq On : 19 Nov 2024 13:17
 Operator : SY/MD
 Sample : VSTD0.519
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 19 21:34:01 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
 Supervised By :Semsettin Yesilyurt 11/21/2024

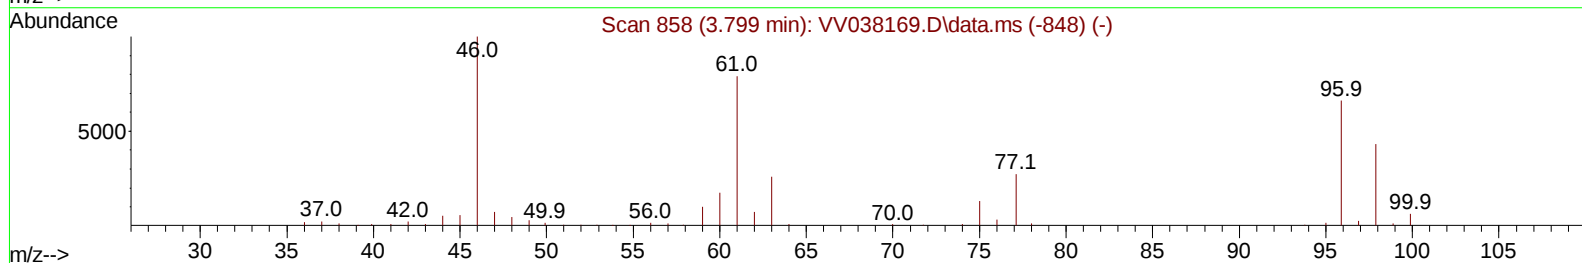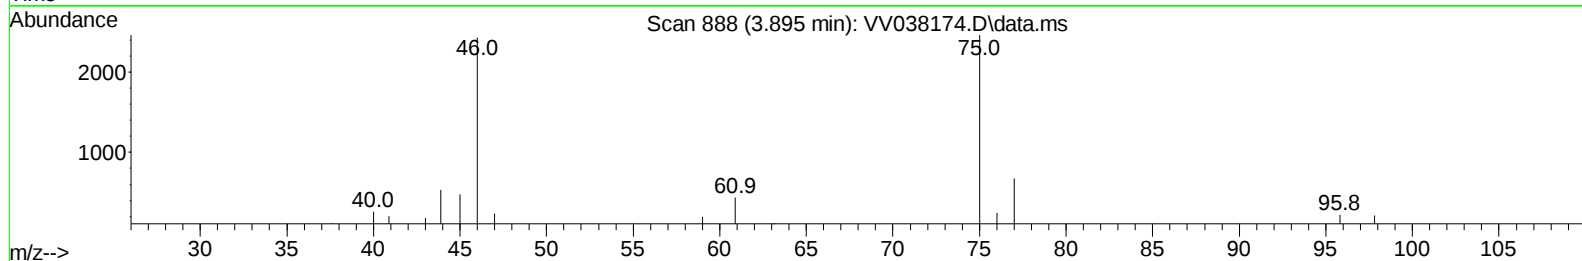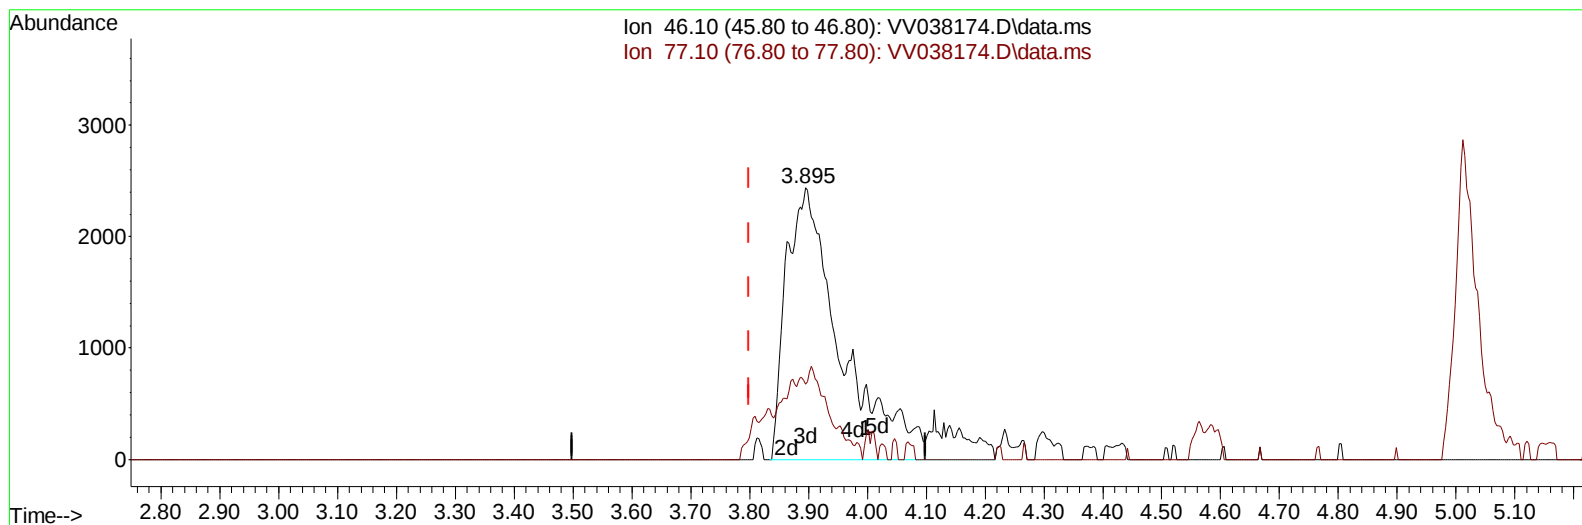

TIC: VV038174.D\data.ms

(20) 2-Butanone-d5 (S)

3.895min (+ 0.096) 4.52 ug/L m

response 17129

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	27.40	0.85#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

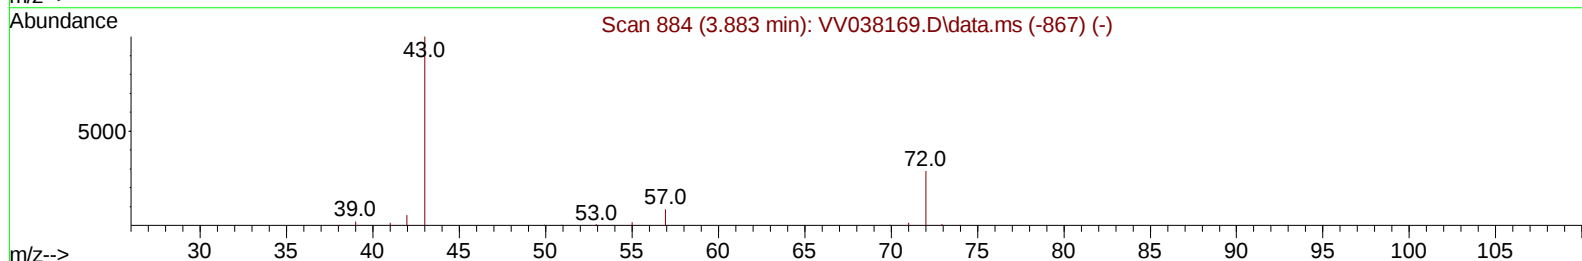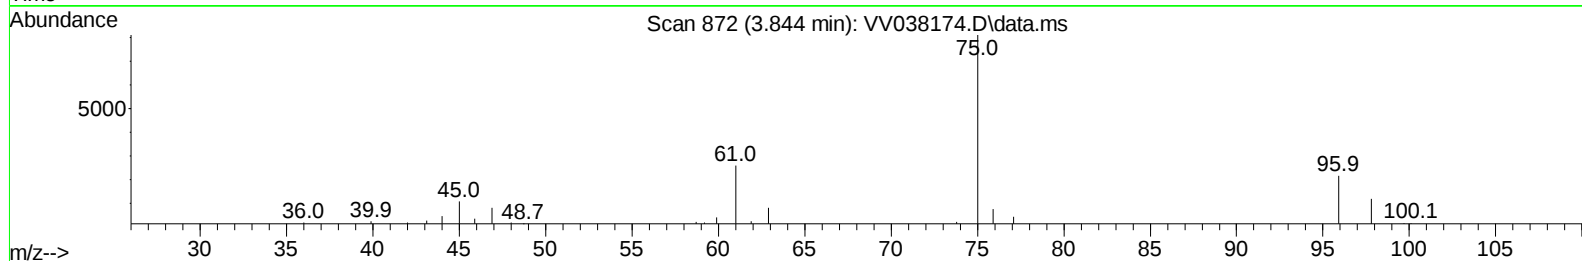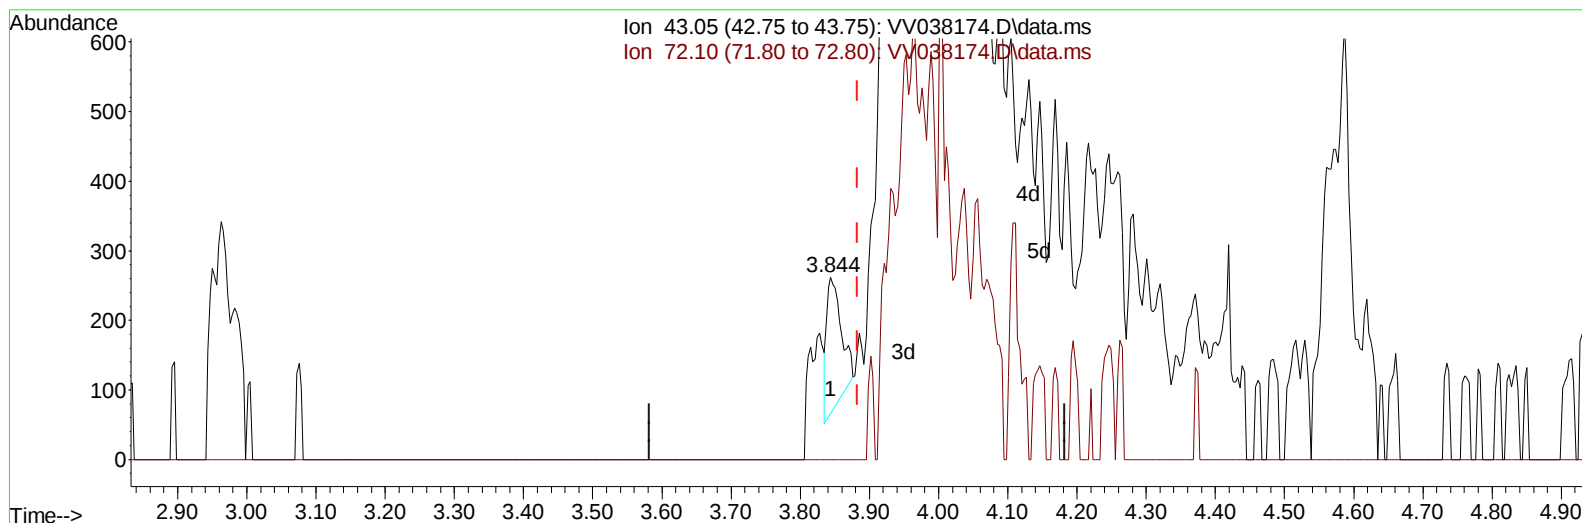

TIC: VV038174.D\data.ms

(21) 2-Butanone (T)

3.844min (-0.039) 0.07 ug/L

response 280

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	26.00	25.71
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

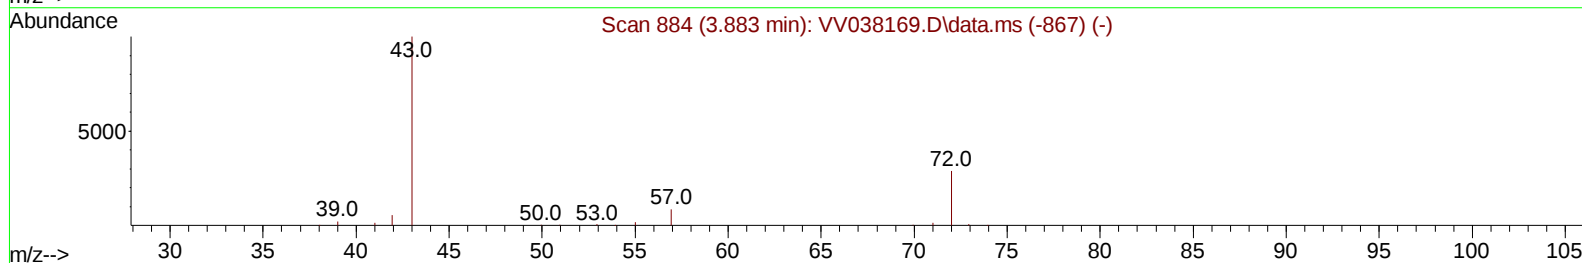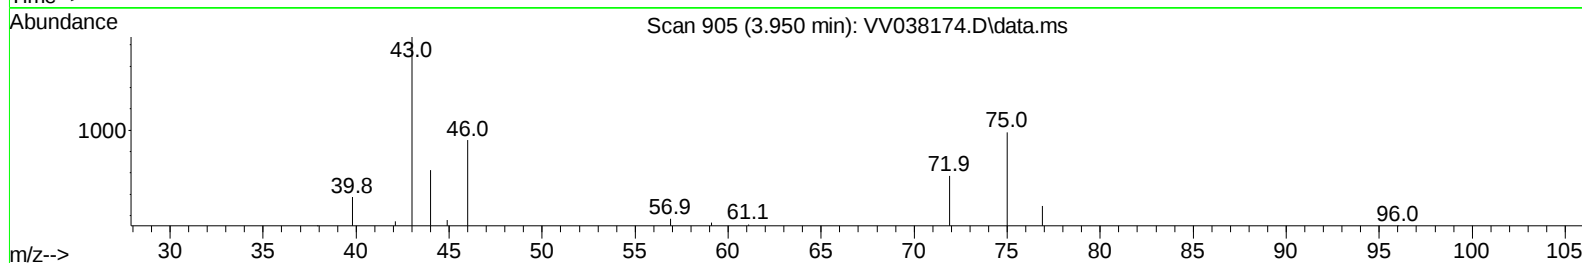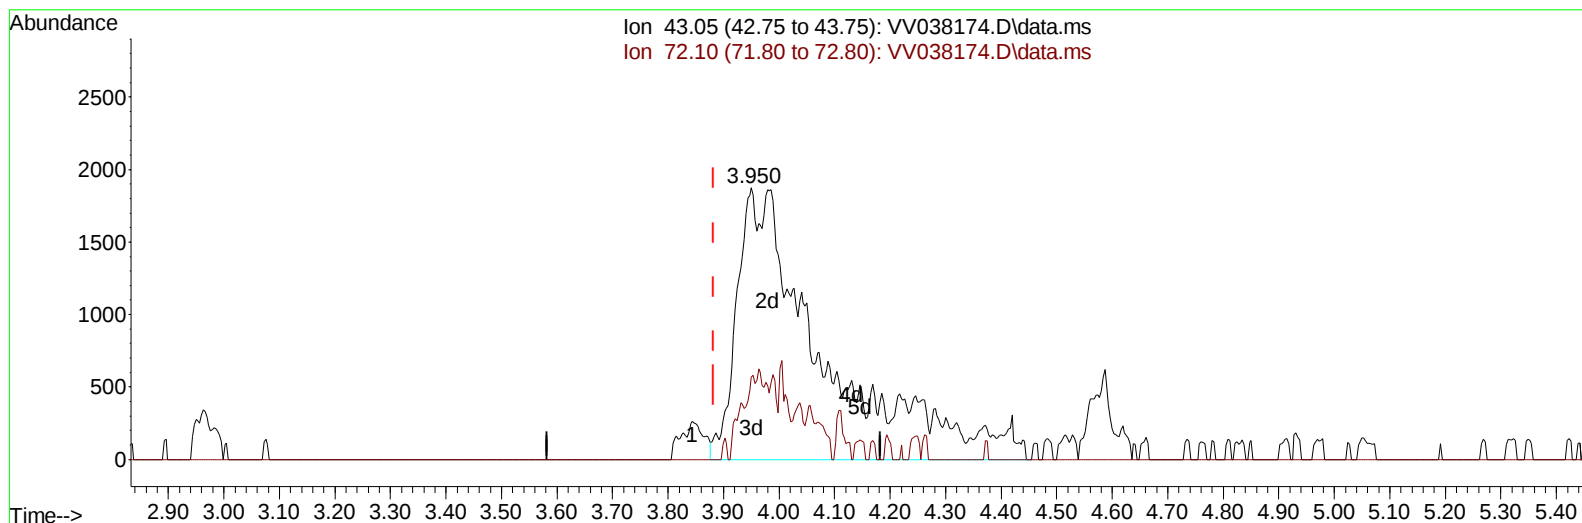

TIC: VV038174.D\data.ms

(21) 2-Butanone (T)

3.950min (+ 0.067) 5.13 ug/L m

response 20103

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	26.00	0.36#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

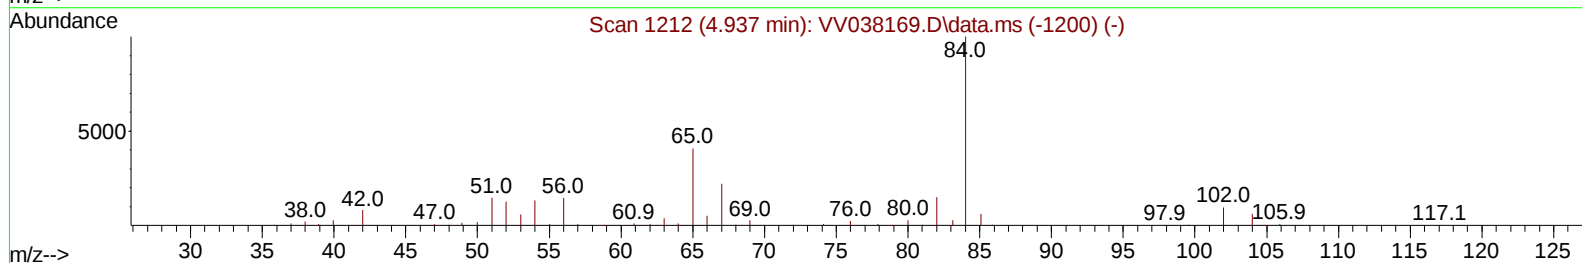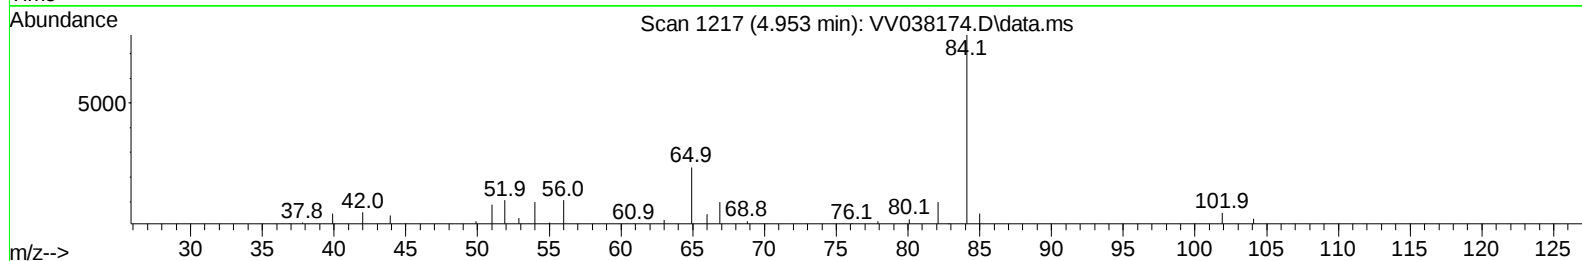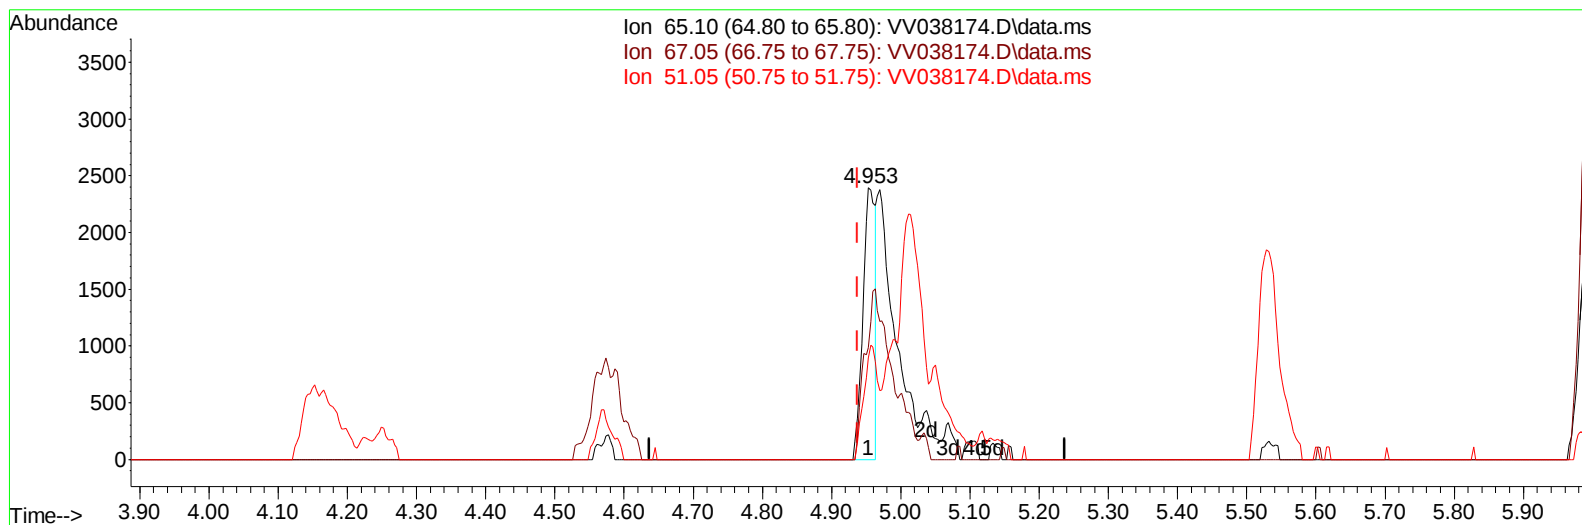

TIC: VV038174.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

4.953min (+ 0.016) 0.17 ug/L

response 2910

Ion	Exp%	Act%
65.10	100.00	100.00
67.05	54.30	142.71#
51.05	33.50	48.01#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

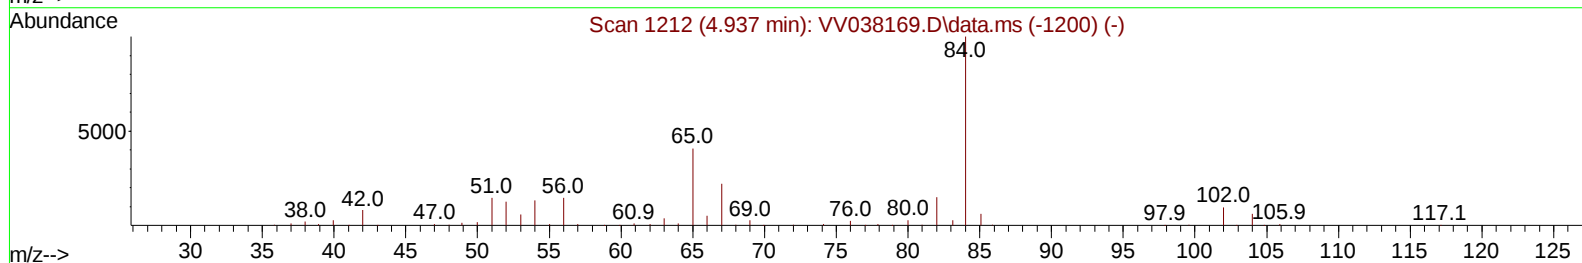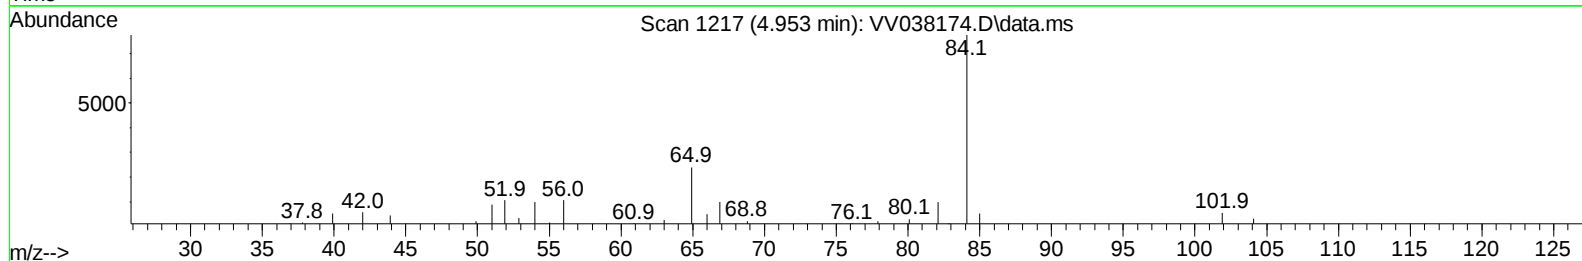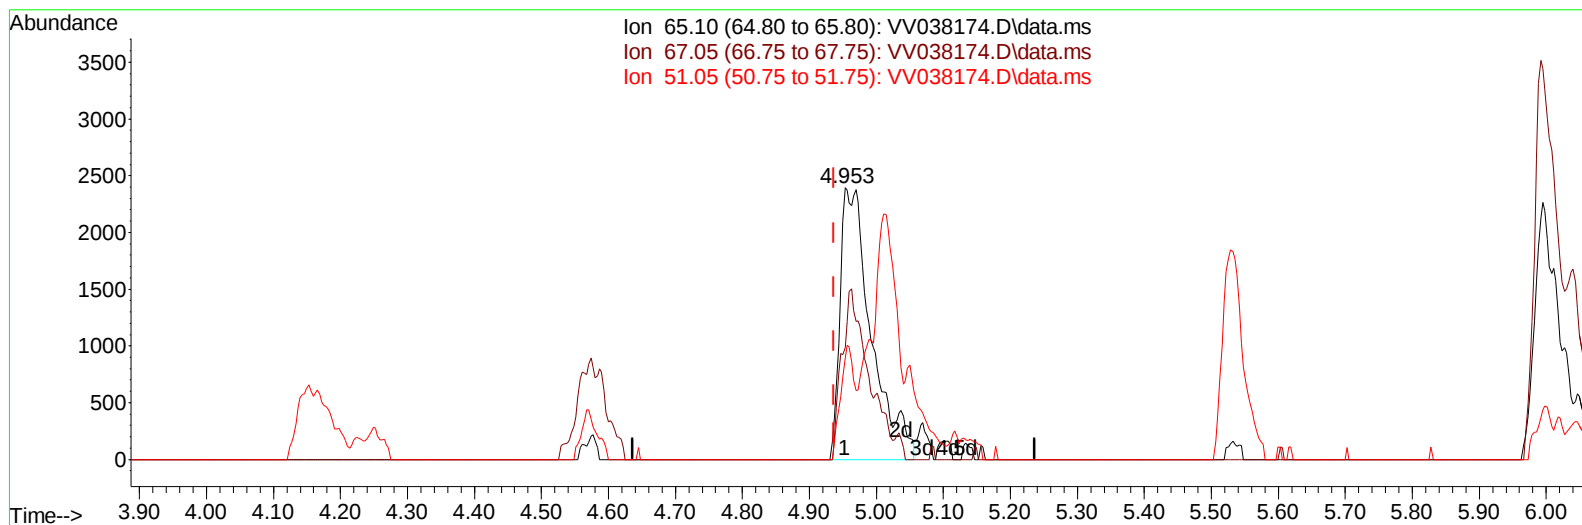

TIC: VV038174.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

4.953min (+ 0.016) 0.44 ug/L m

response 7712

Ion	Exp%	Act%
65.10	100.00	100.00
67.05	54.30	53.85
51.05	33.50	18.11#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

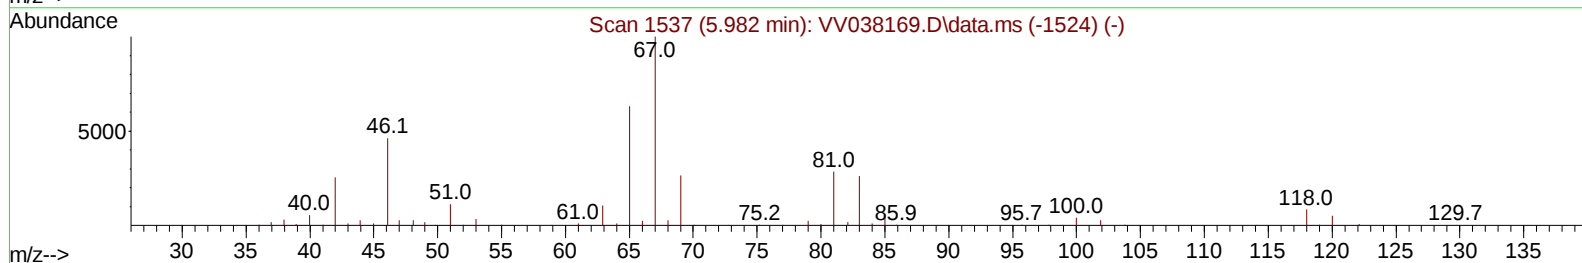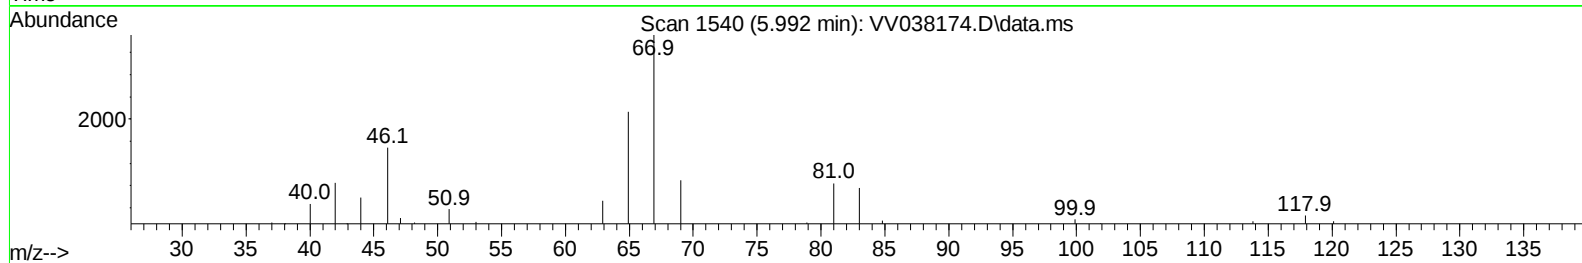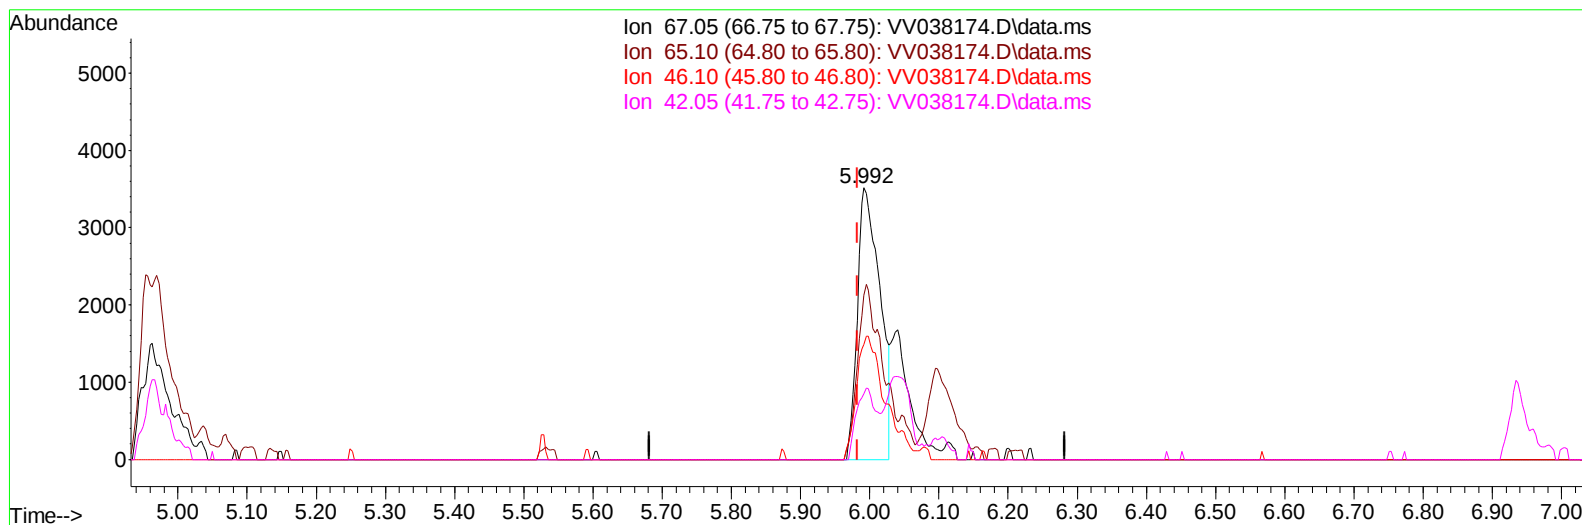

TIC: VV038174.D\data.ms

(36) 1,2-Dichloropropane-d6 (S)

5.992min (+ 0.010) 0.37 ug/L

response 7879

Ion	Exp%	Act%
67.05	100.00	100.00
65.10	69.80	70.92
46.10	47.80	58.15
42.05	25.80	22.87




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

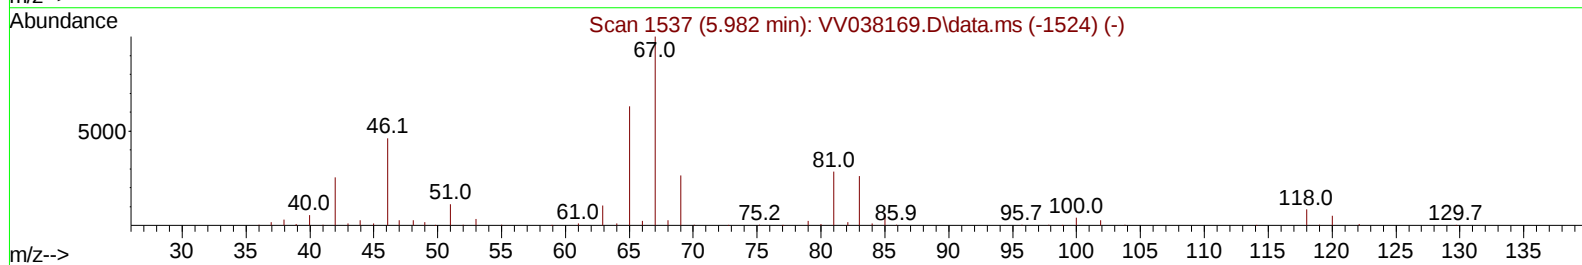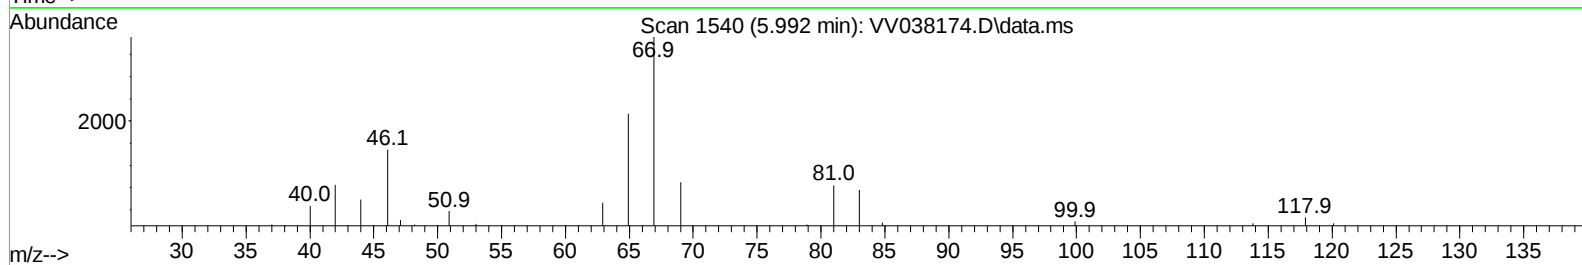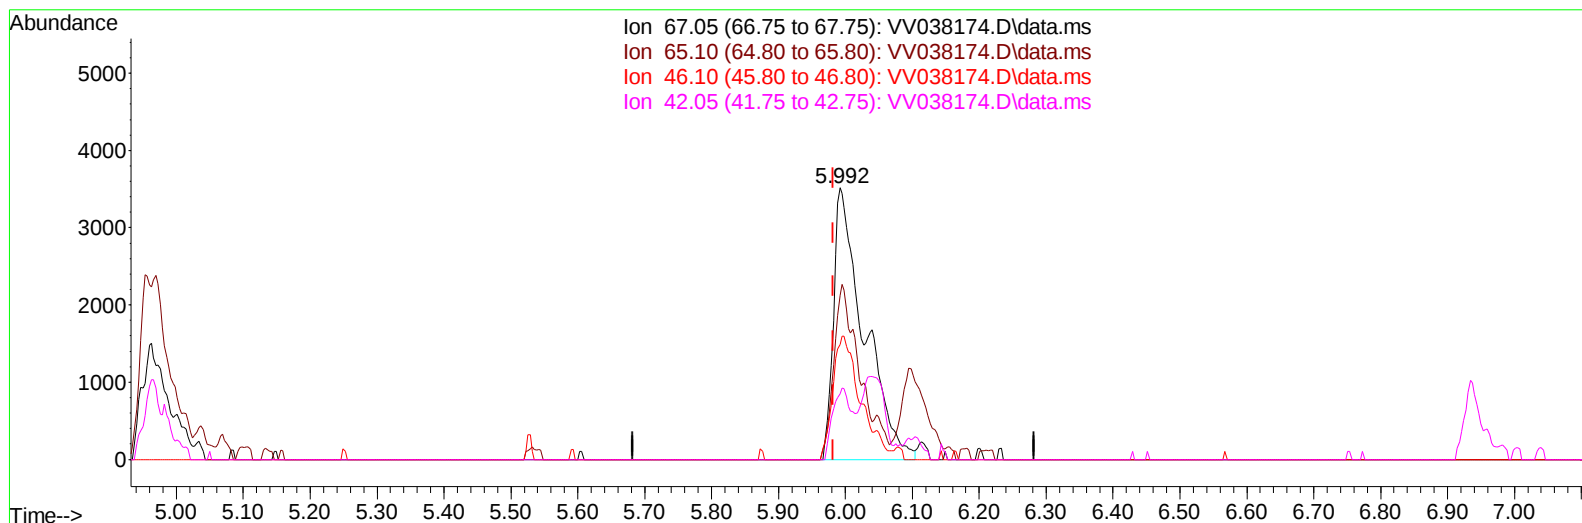

TIC: VV038174.D\data.ms

(36) 1,2-Dichloropropane-d6 (S)

5.992min (+ 0.010) 0.52 ug/L m

response 11098

Ion	Exp%	Act%
67.05	100.00	100.00
65.10	69.80	50.35
46.10	47.80	41.29
42.05	25.80	16.24#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

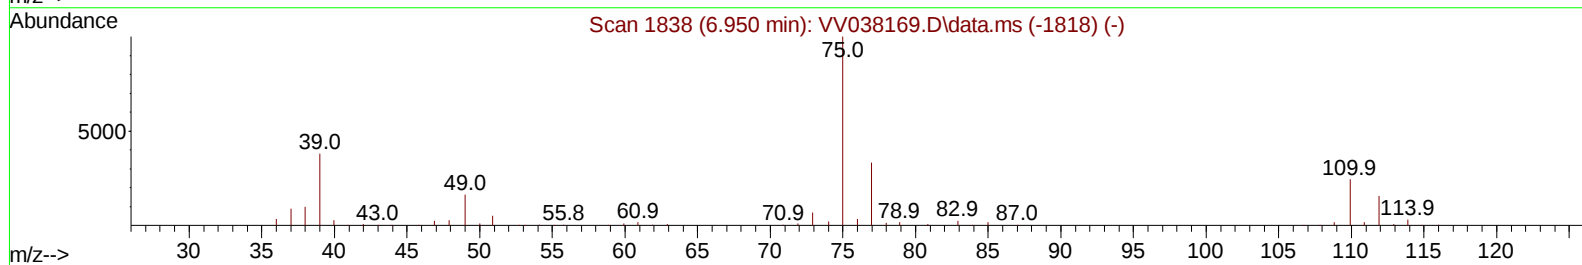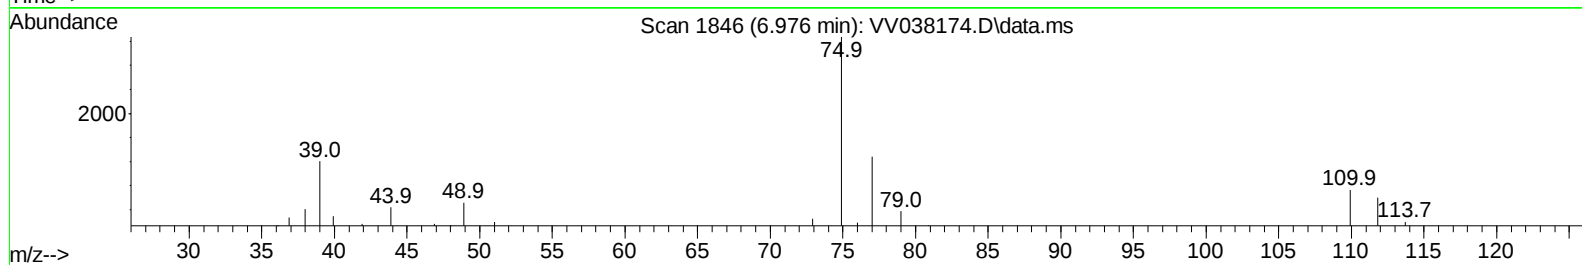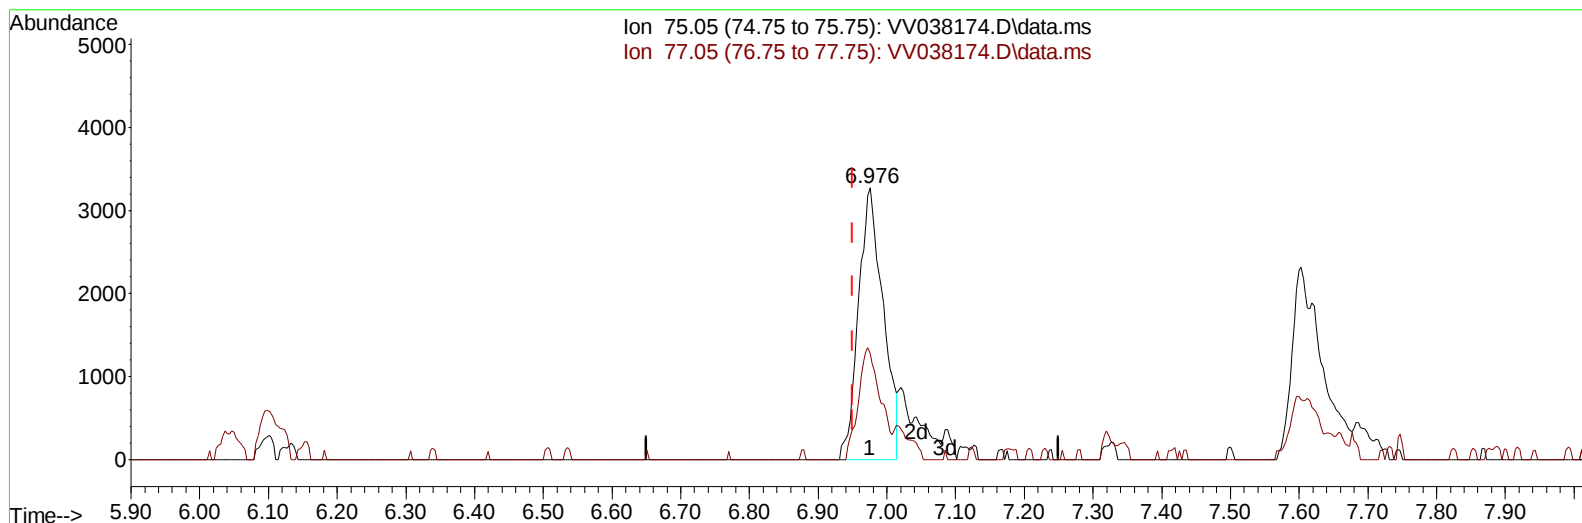

TIC: VV038174.D\data.ms

(39) cis-1,3-Dichloropropene (T)

6.976min (+ 0.026) 0.32 ug/L

response 8150

Ion	Exp%	Act%
75.05	100.00	100.00
77.05	33.50	39.10
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

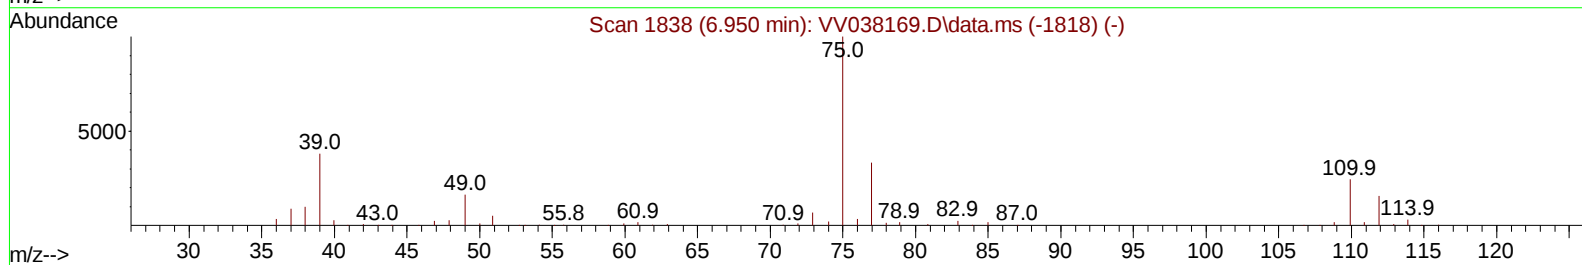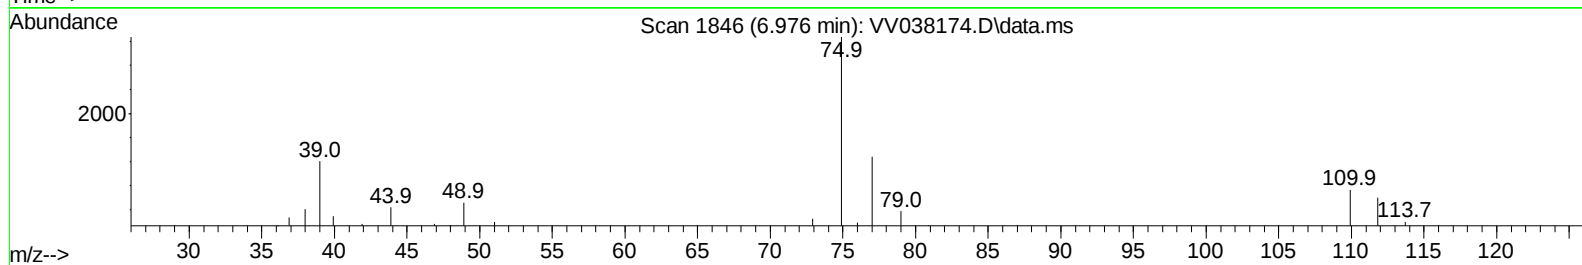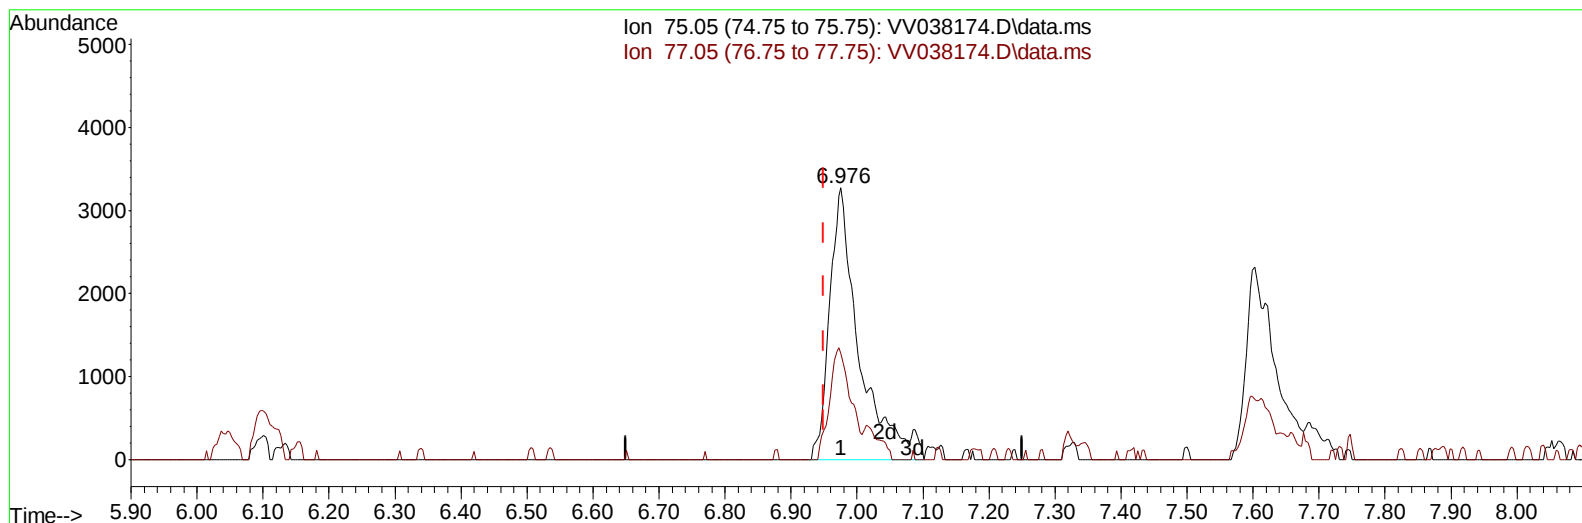

TIC: VV038174.D\data.ms

(39) cis-1,3-Dichloropropene (T)

6.976min (+ 0.026) 0.40 ug/L m

response 10226

Ion	Exp%	Act%
75.05	100.00	100.00
77.05	33.50	39.10
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

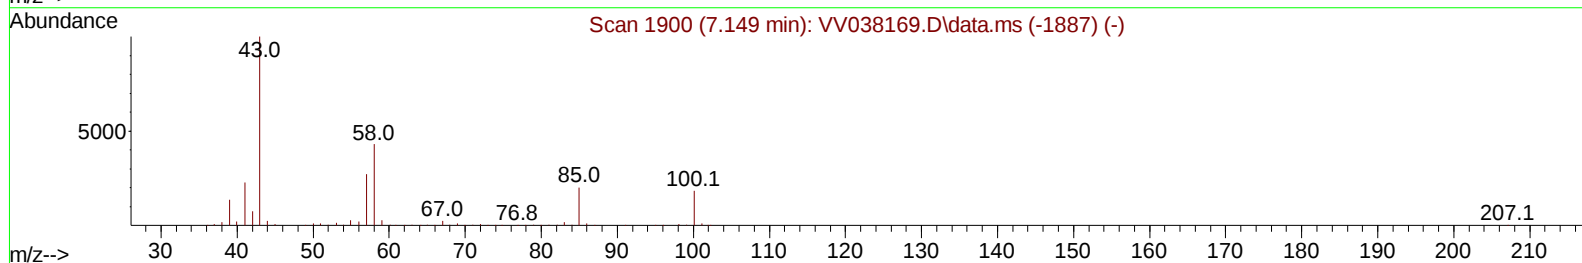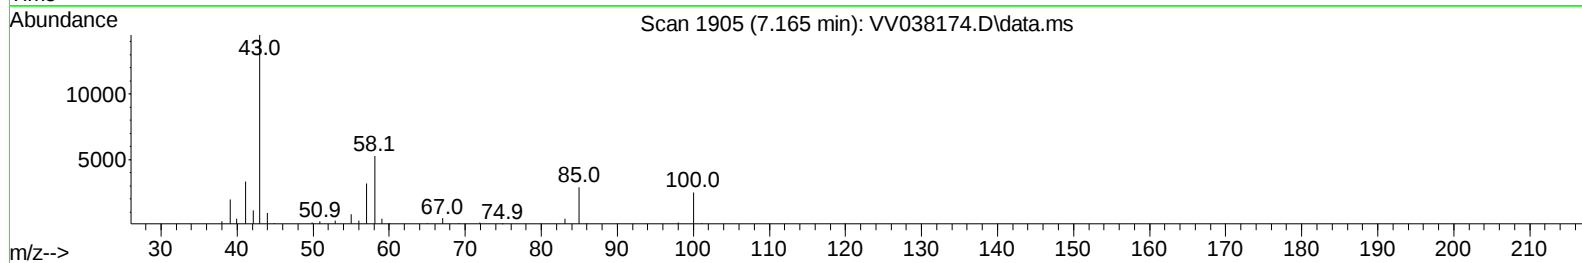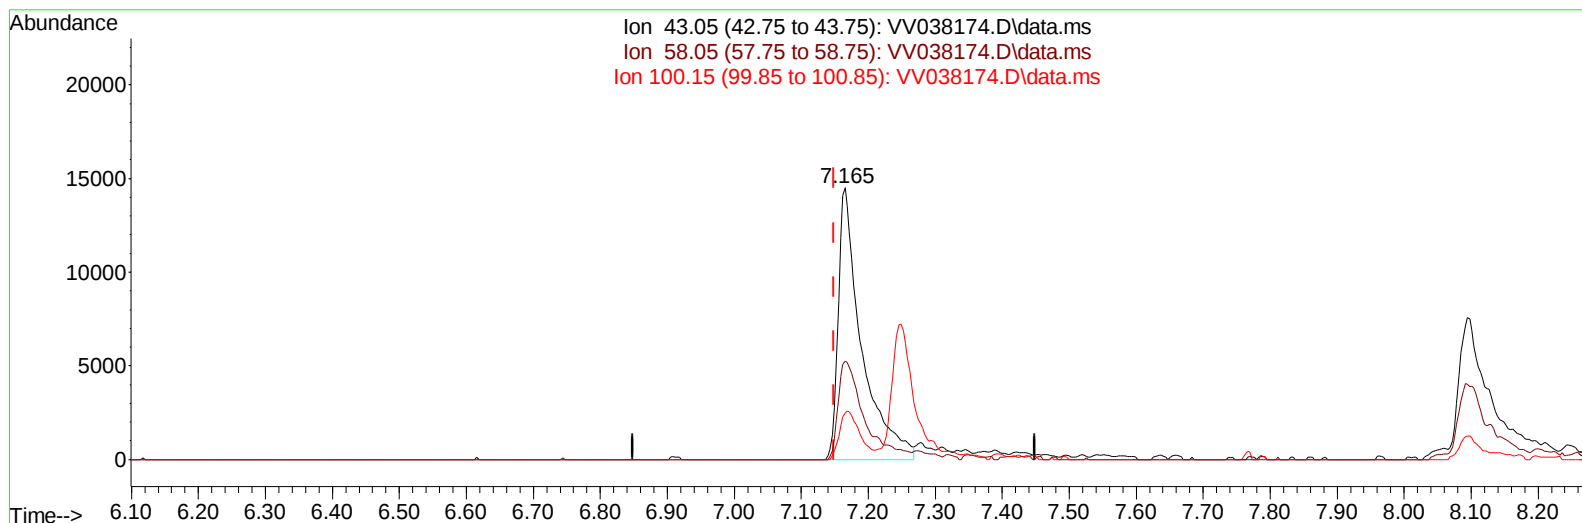

TIC: VV038174.D\data.ms

(40) 4-Methyl-2-pentanone (T)

7.165min (+ 0.016) 3.59 ug/L

response 34972

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.80	40.66
100.15	17.90	15.54
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

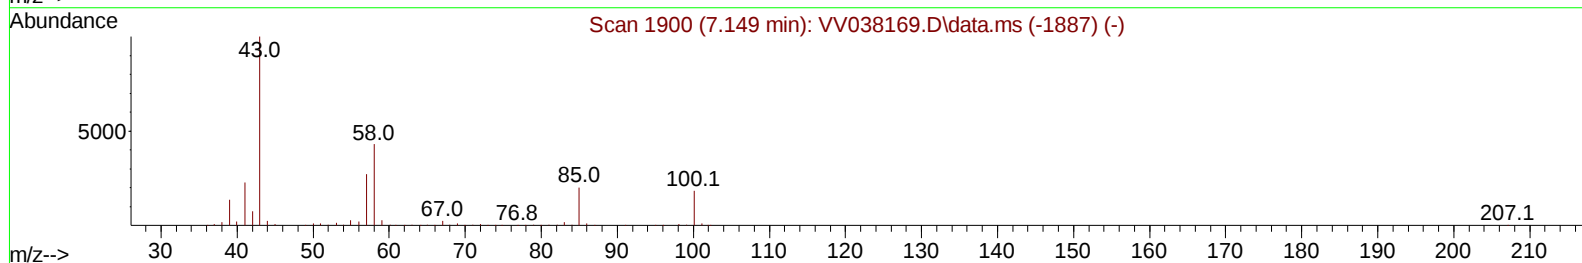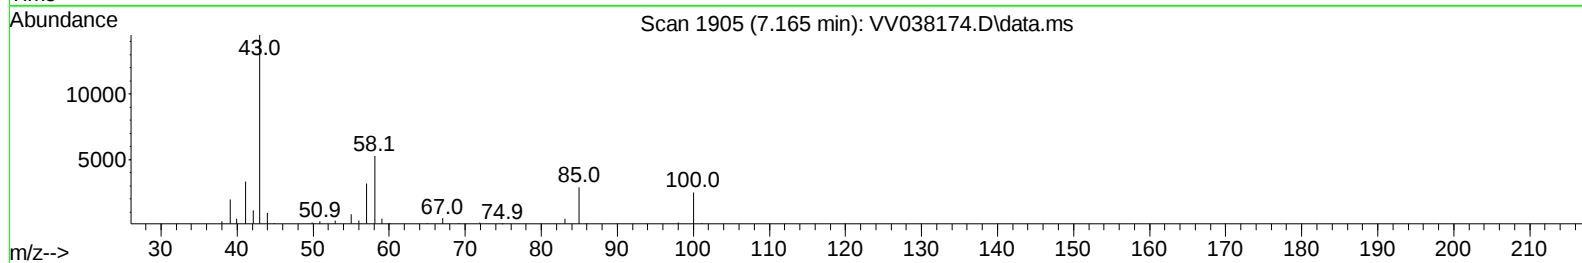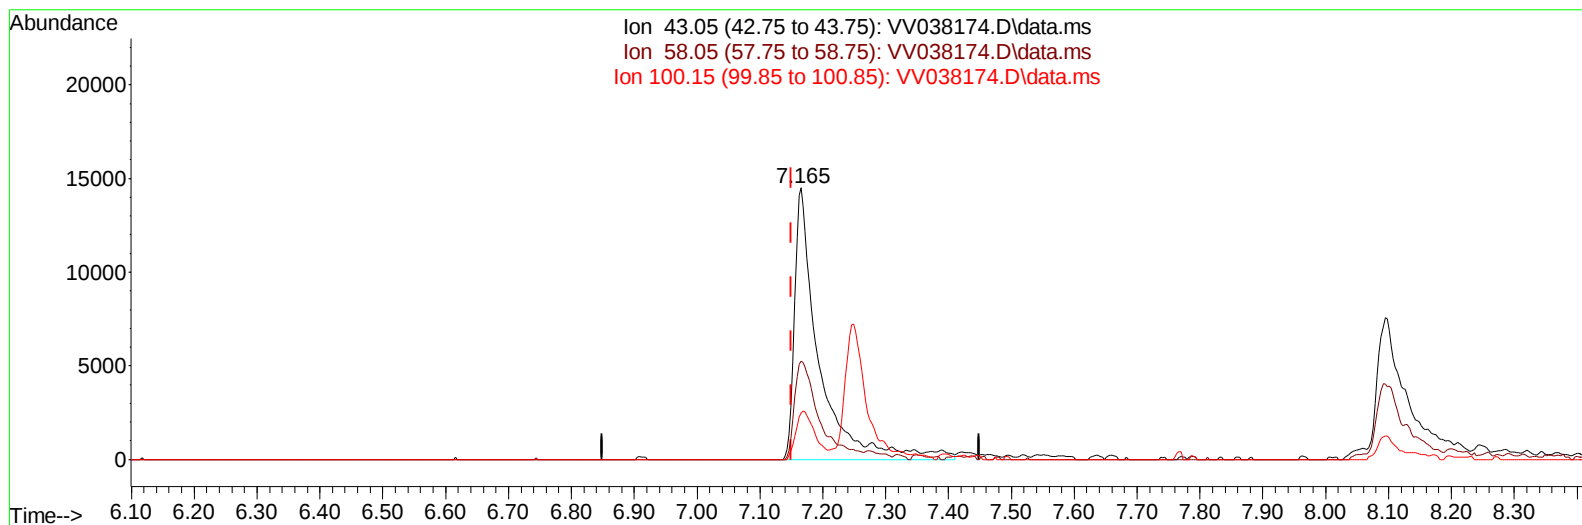

TIC: VV038174.D\data.ms

(40) 4-Methyl-2-pentanone (T)

7.165min (+ 0.016) 4.01 ug/L m

response 39115

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.80	36.35
100.15	17.90	13.89#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

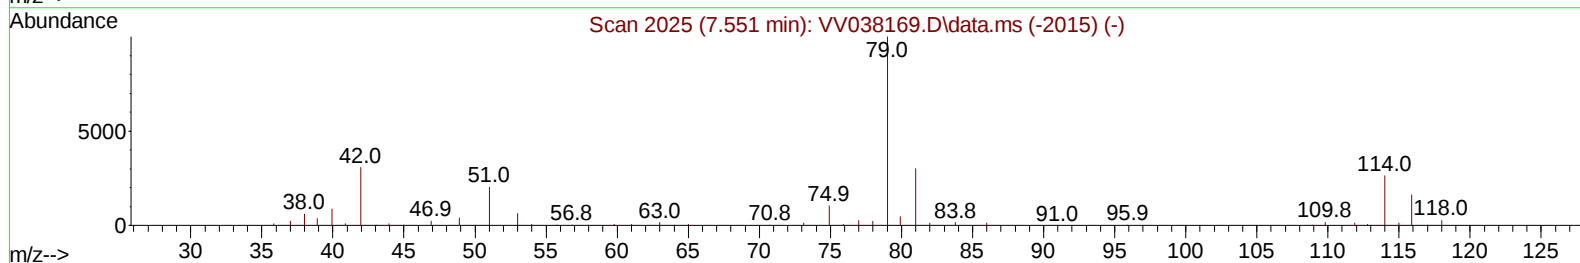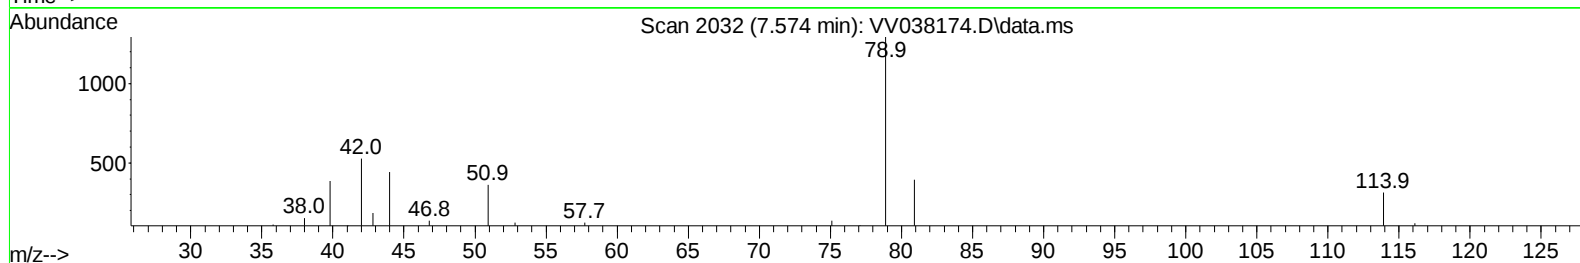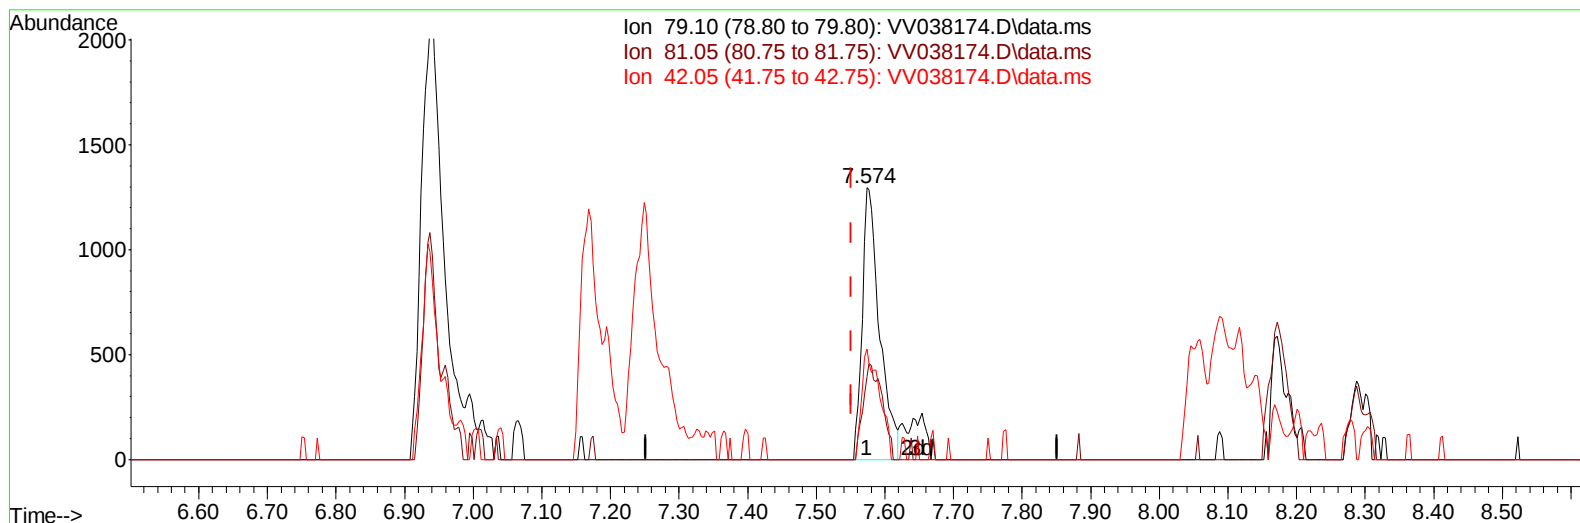

TIC: VV038174.D\data.ms

(43) trans-1,3-Dichloropropene-d4 (S)

7.574min (+ 0.022) 0.29 ug/L

response 2258

Ion	Exp%	Act%
79.10	100.00	100.00
81.05	31.90	38.62
42.05	34.10	41.67
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

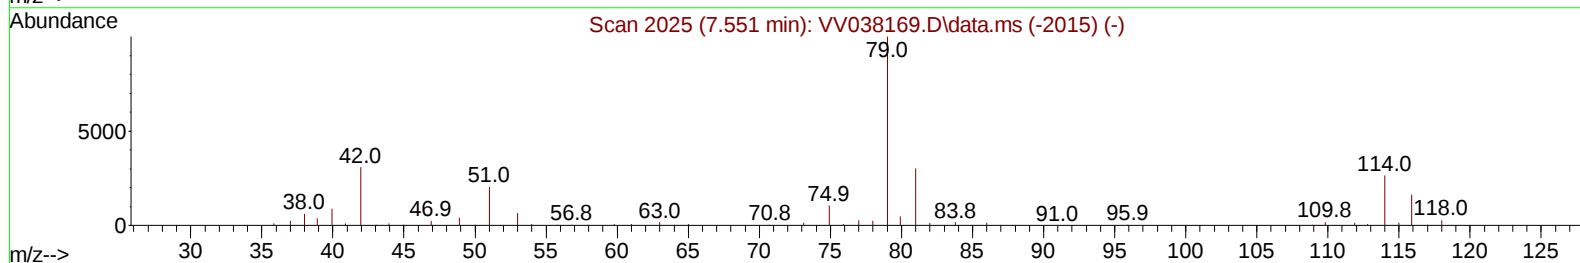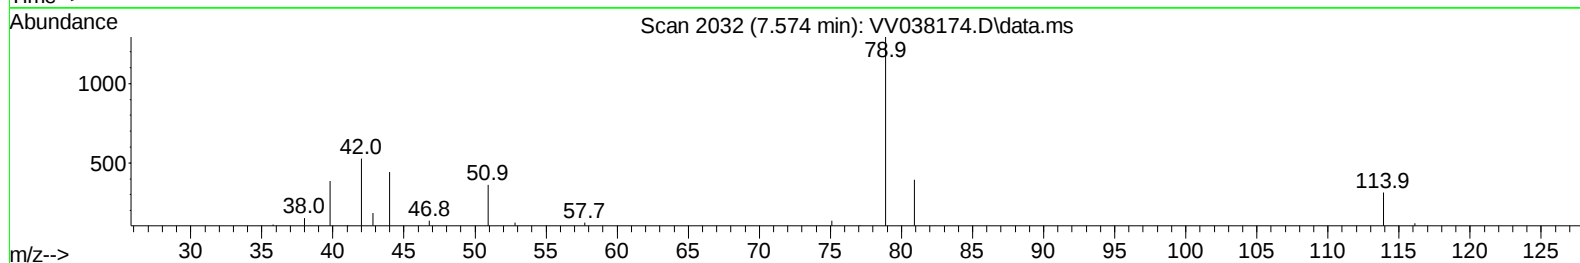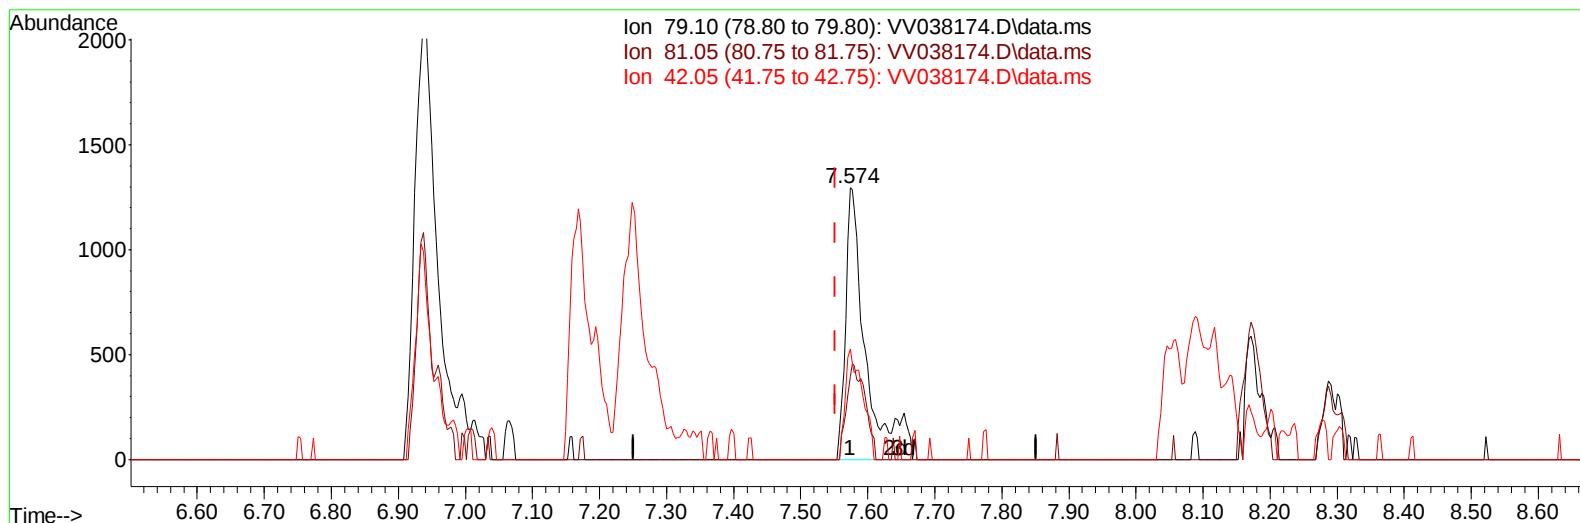

TIC: VV038174.D\data.ms

(43) trans-1,3-Dichloropropene-d4 (S)

7.574min (+ 0.022) 0.35 ug/L m

response 2695

Ion	Exp%	Act%
79.10	100.00	100.00
81.05	31.90	32.36
42.05	34.10	34.92
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

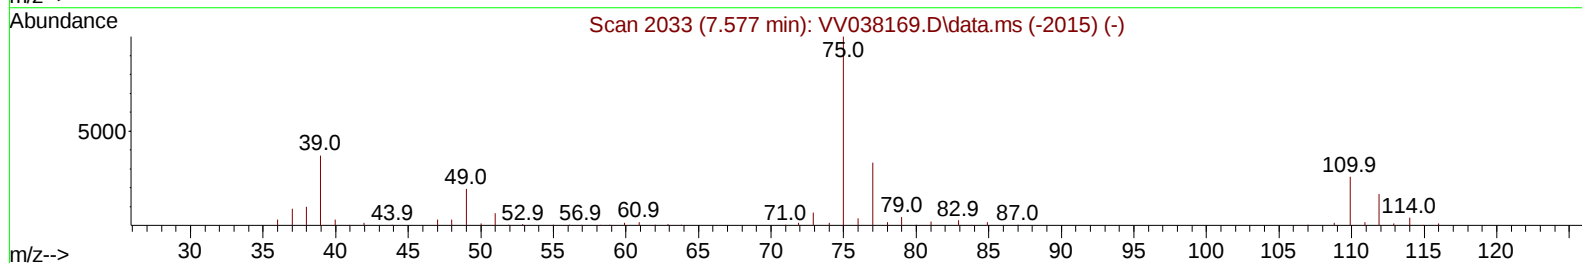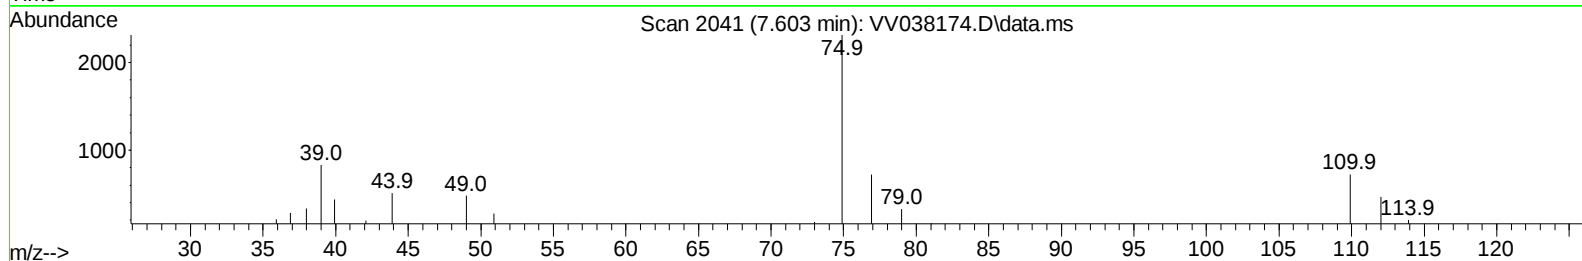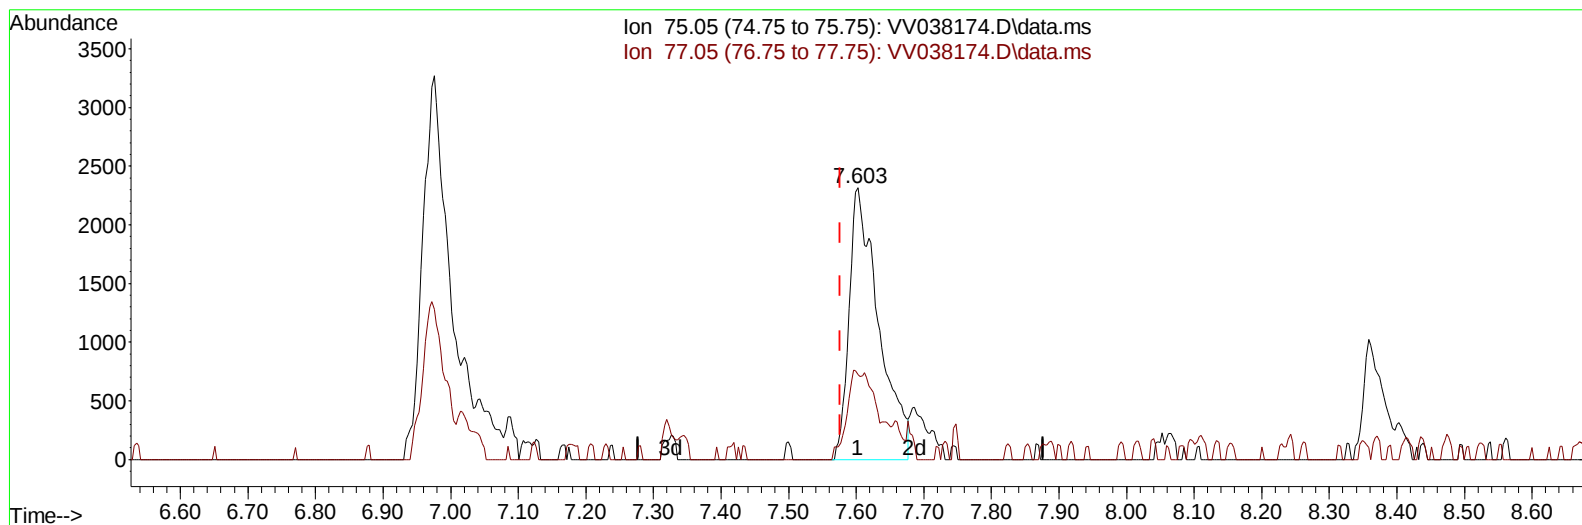

TIC: VV038174.D\data.ms

(44) trans-1,3-Dichloropropene (T)

7.603min (+ 0.026) 0.32 ug/L

response 7021

Ion	Exp%	Act%
75.05	100.00	100.00
77.05	33.40	31.23
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

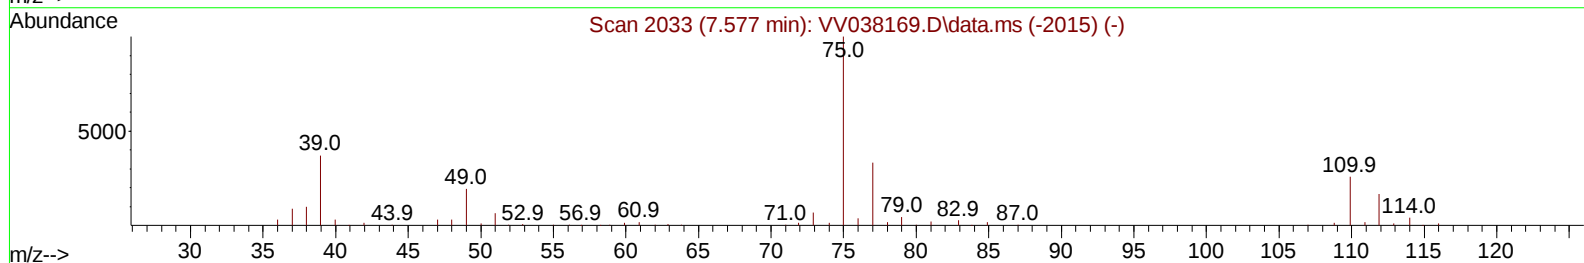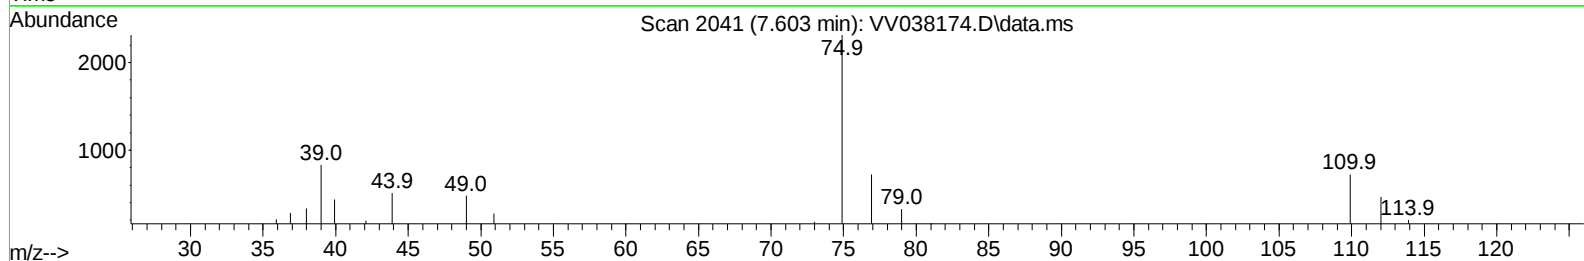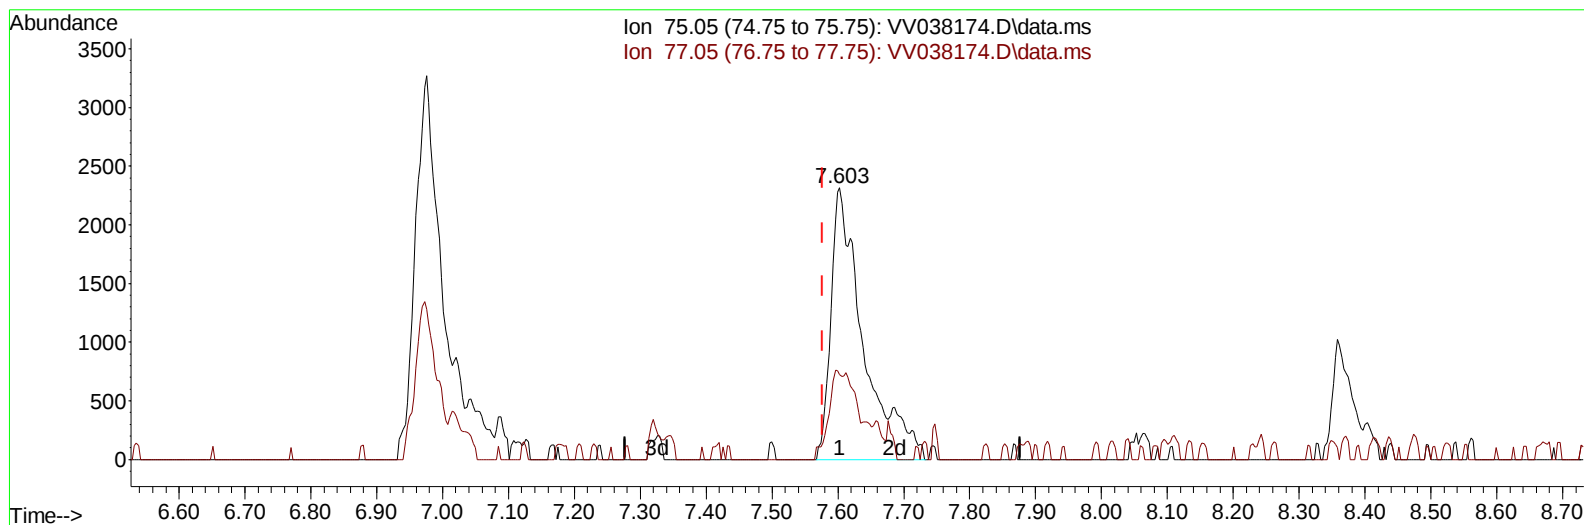

TIC: VV038174.D\data.ms

(44) trans-1,3-Dichloropropene (T)

7.603min (+ 0.026) 0.36 ug/L m

response 7876

Ion	Exp%	Act%
75.05	100.00	100.00
77.05	33.40	31.23
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

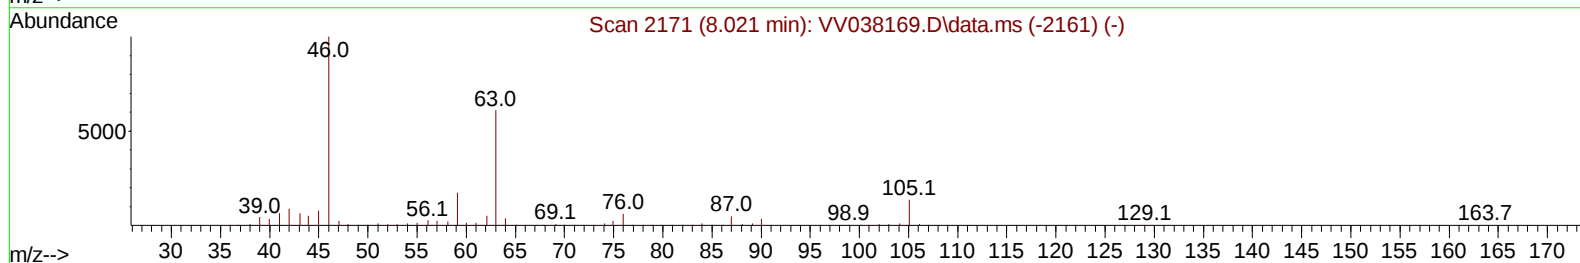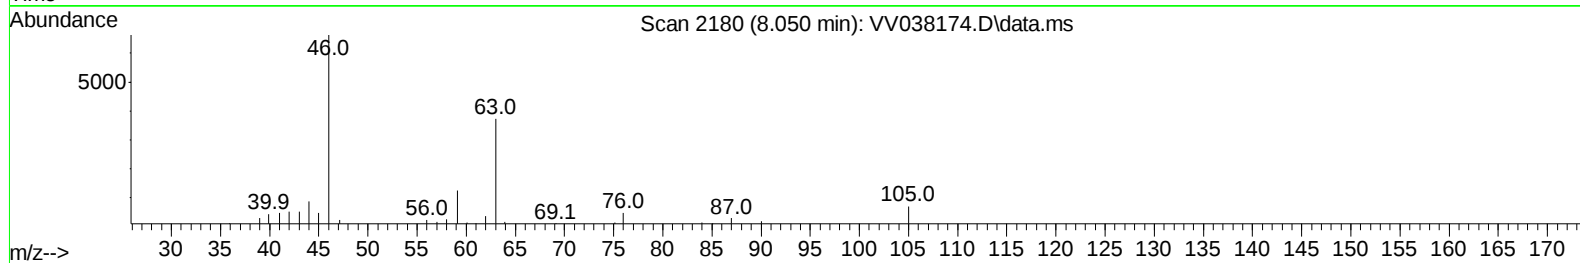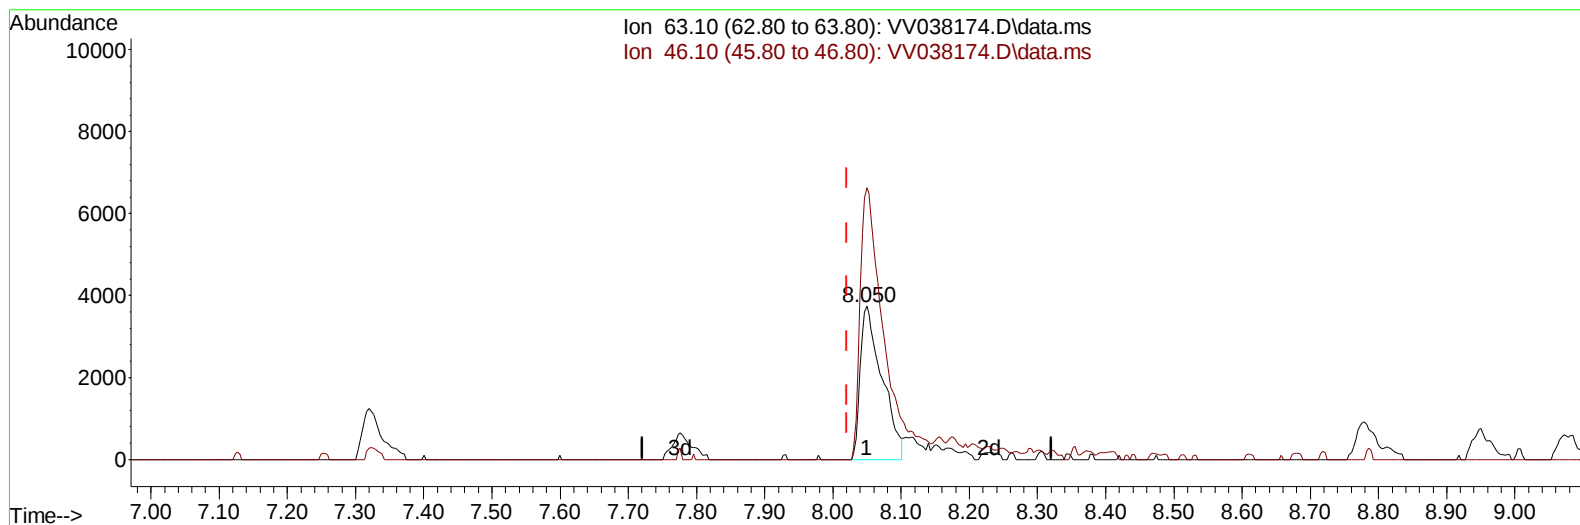

TIC: VV038174.D\data.ms

(46) 2-Hexanone-d5 (S)

8.050min (+ 0.029) 2.81 ug/L

response 8293

Ion	Exp%	Act%
63.10	100.00	100.00
46.10	168.20	194.13
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

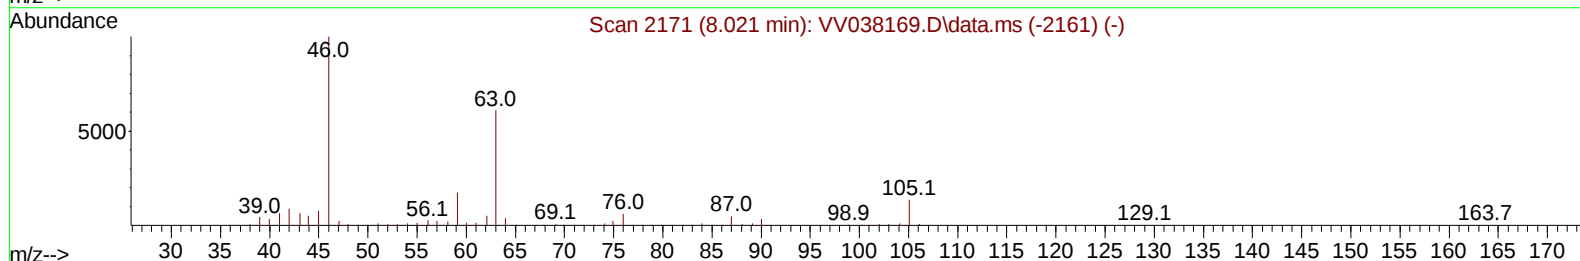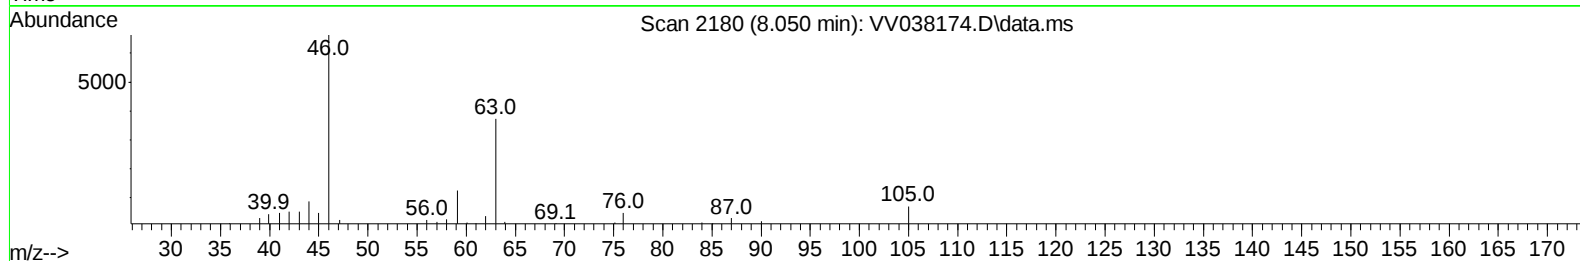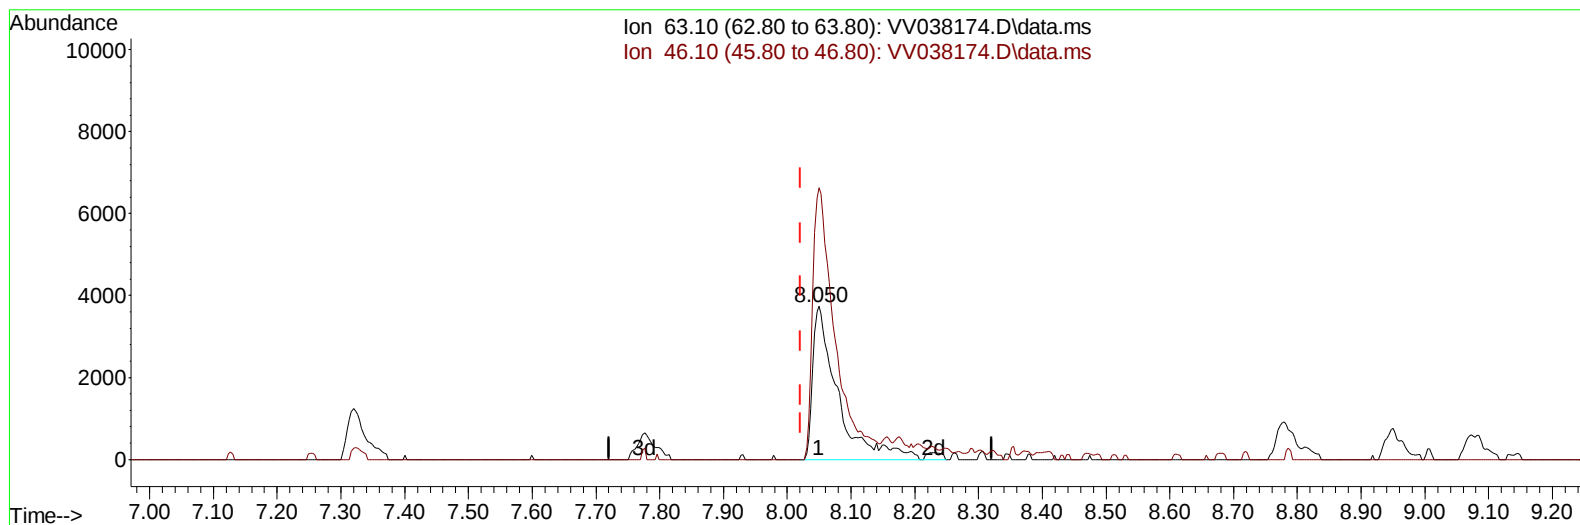

TIC: VV038174.D\data.ms

(46) 2-Hexanone-d5 (S)

8.050min (+ 0.029) 3.54 ug/L m

response 10443

Ion	Exp%	Act%
63.10	100.00	100.00
46.10	168.20	154.16
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
 Data File : VV038174.D
 Acq On : 19 Nov 2024 13:17
 Operator : SY/MD
 Sample : VSTD0.519
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 19 21:34:01 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
 Supervised By :Semsettin Yesilyurt 11/21/2024

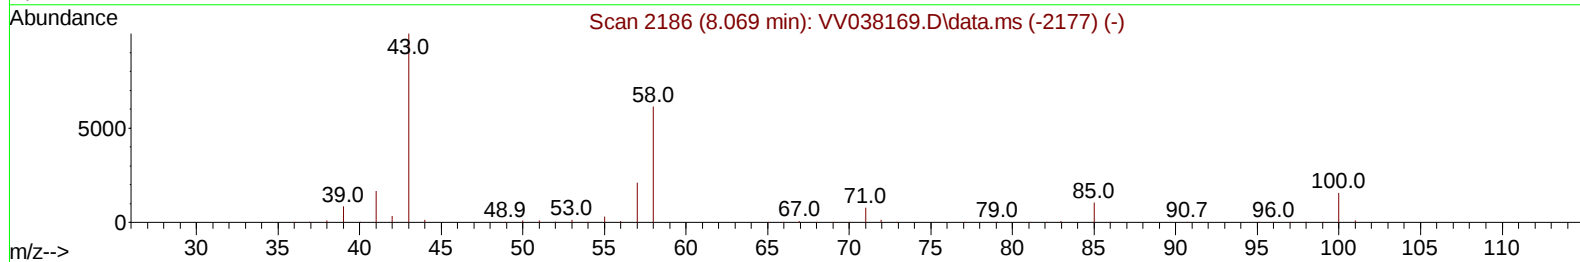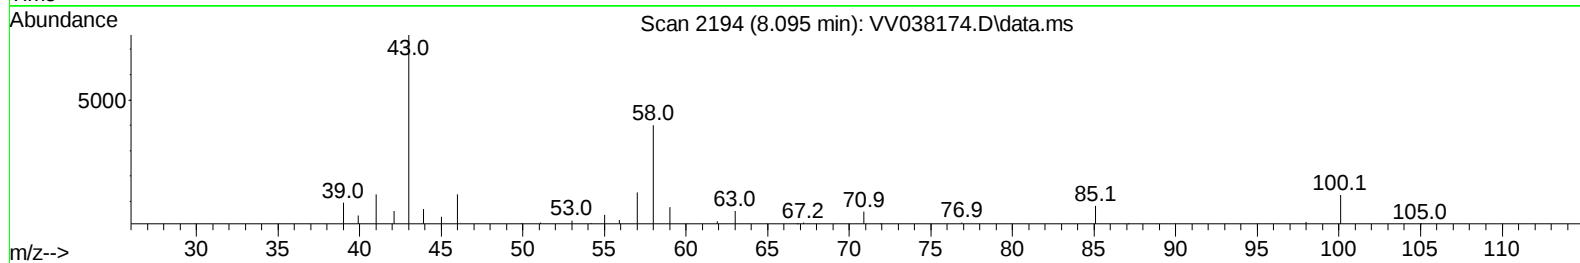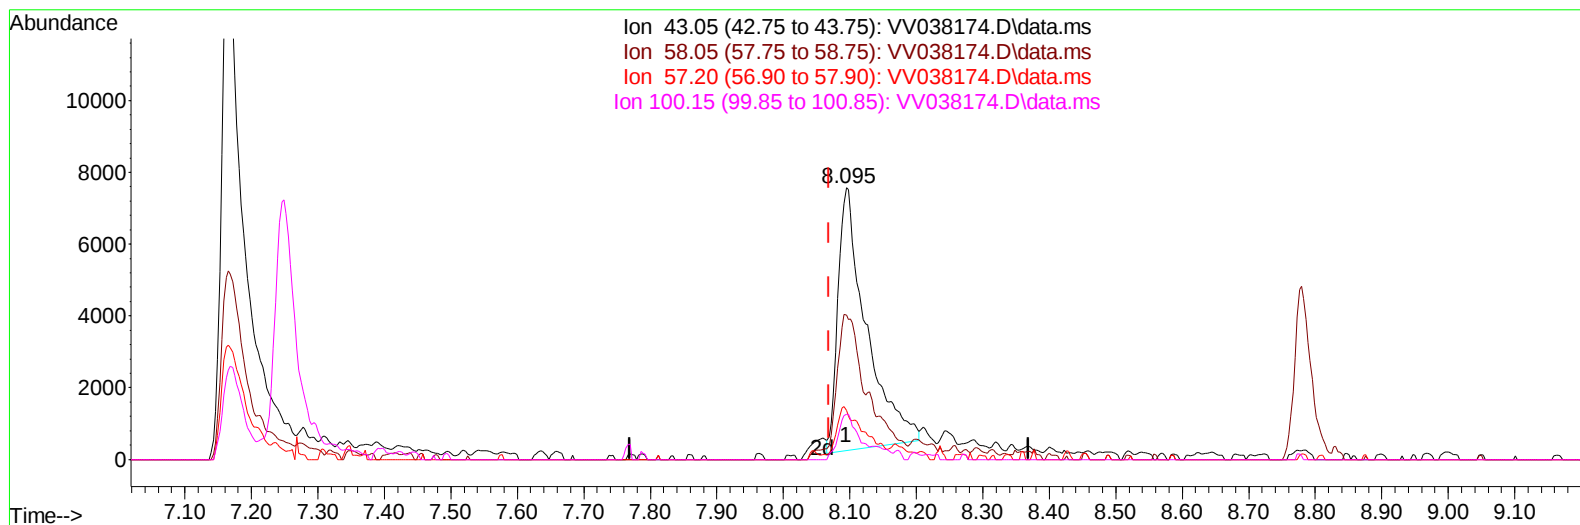

TIC: VV038174.D\data.ms

(48) 2-Hexanone (T)

8.095min (+ 0.026) 3.22 ug/L

response 21681

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	61.50	61.89
57.20	21.10	19.29
100.15	14.80	12.47




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
 Data File : VV038174.D
 Acq On : 19 Nov 2024 13:17
 Operator : SY/MD
 Sample : VSTD0.519
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 19 21:34:01 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
 Supervised By :Semsettin Yesilyurt 11/21/2024

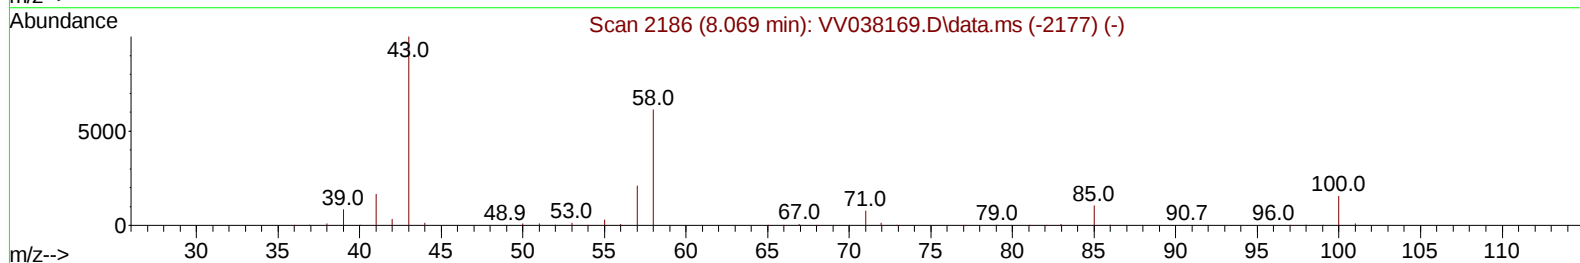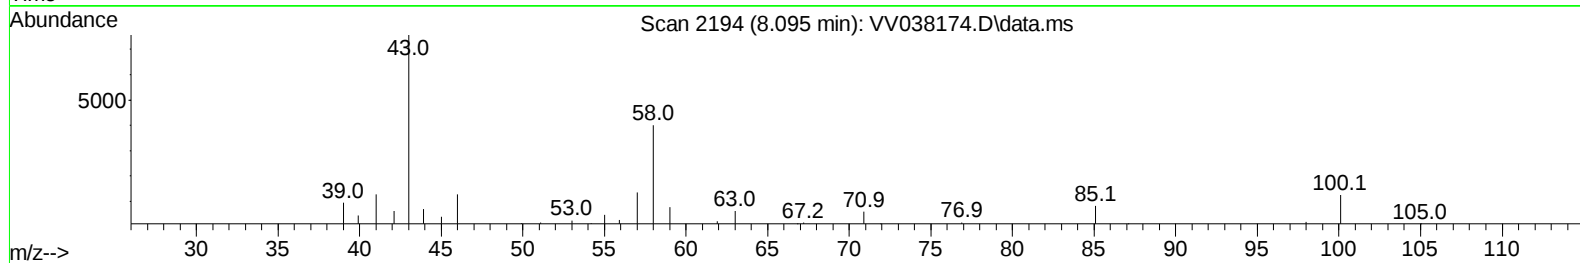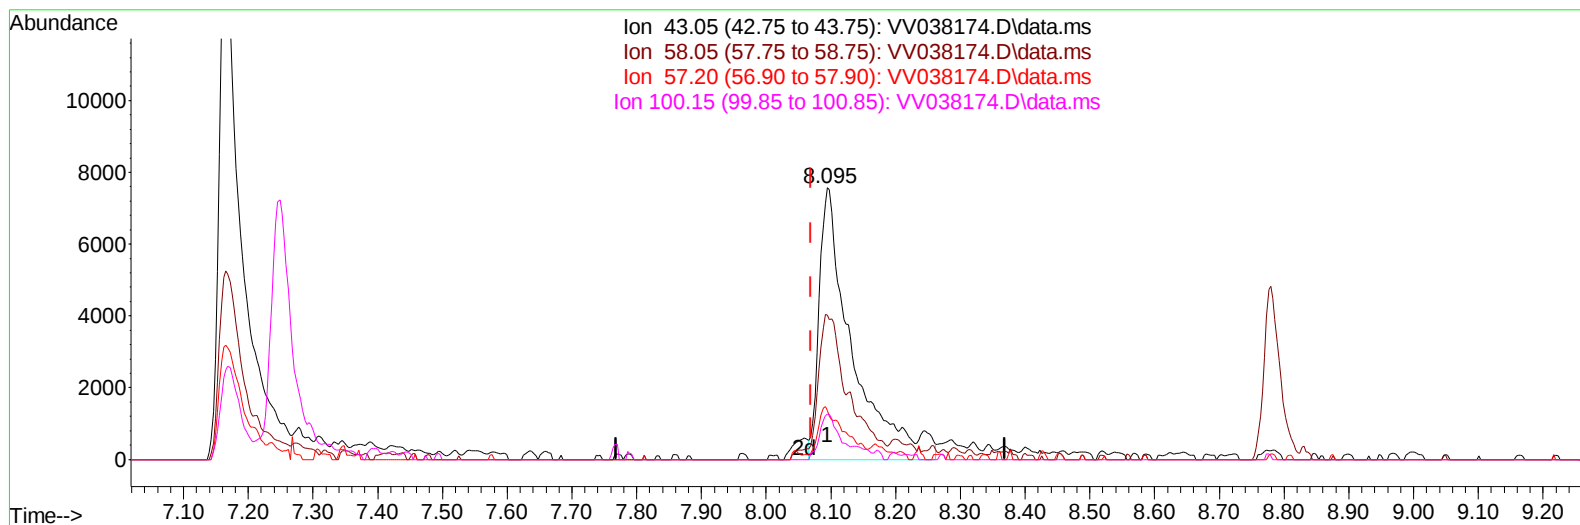

TIC: VV038174.D\data.ms

(48) 2-Hexanone (T)

8.095min (+ 0.026) 3.99 ug/L m

response 26868

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	61.50	49.94
57.20	21.10	15.56#
100.15	14.80	10.06#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

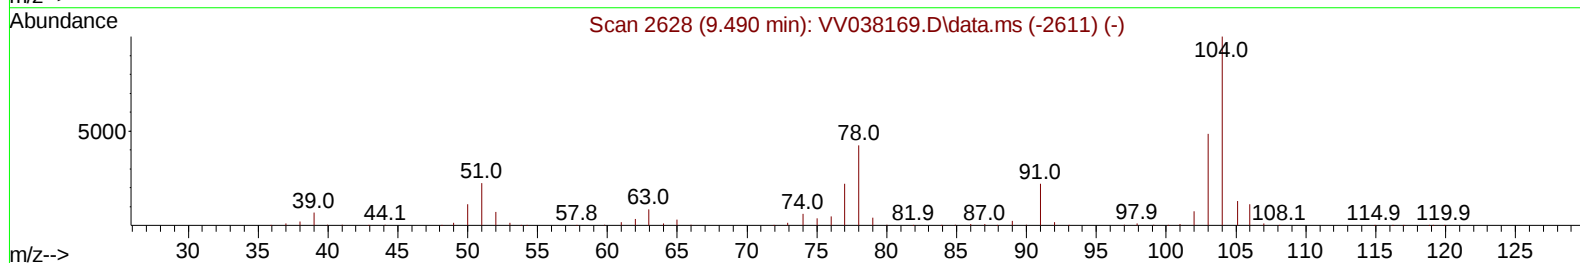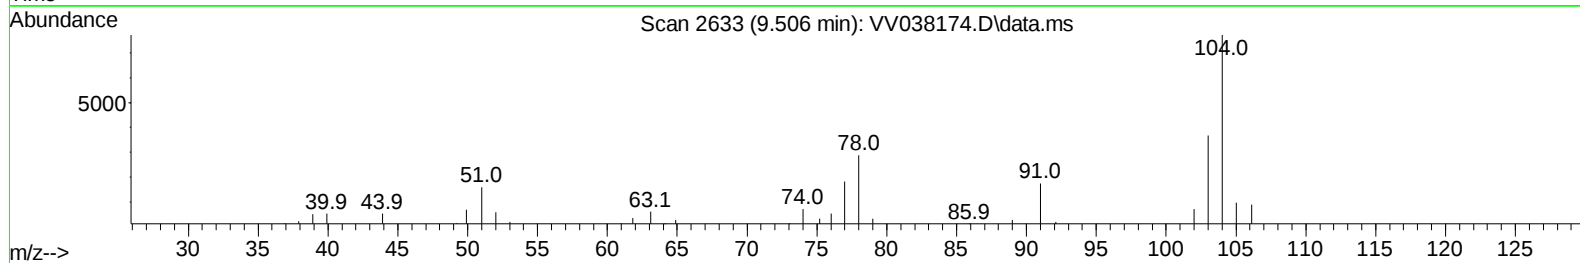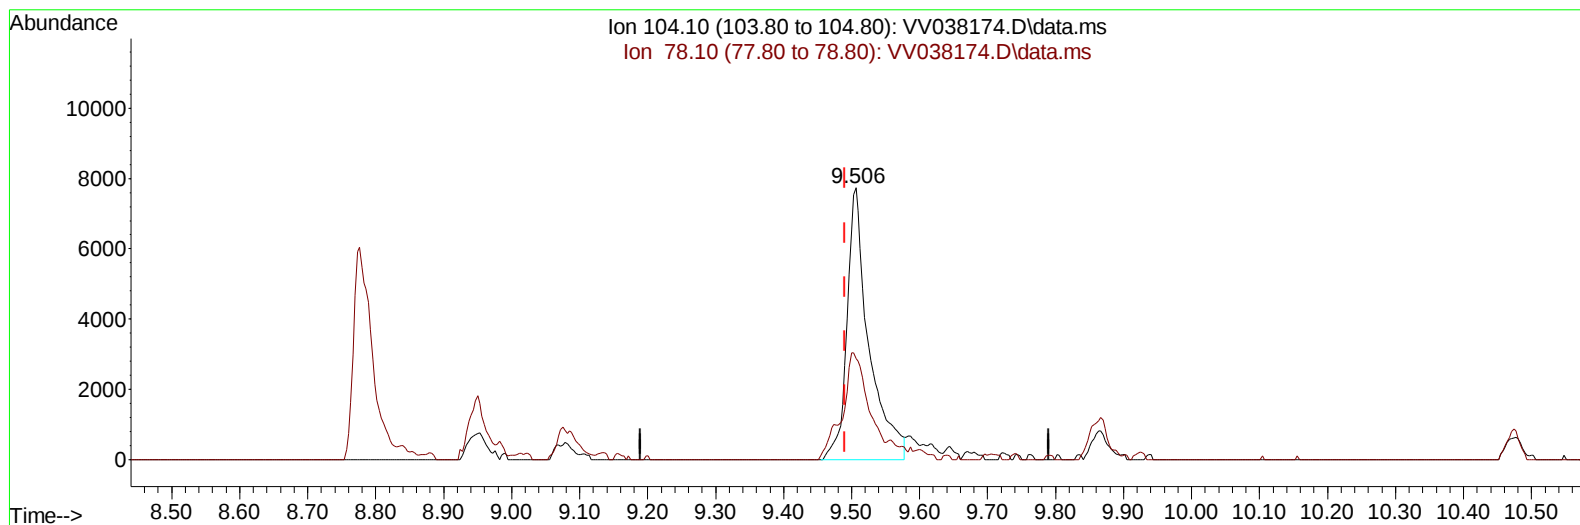

TIC: VV038174.D\data.ms

(55) Styrene (T)

9.506min (+ 0.016) 0.32 ug/L

response 17260

Ion	Exp%	Act%
104.10	100.00	100.00
78.10	42.40	37.20
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

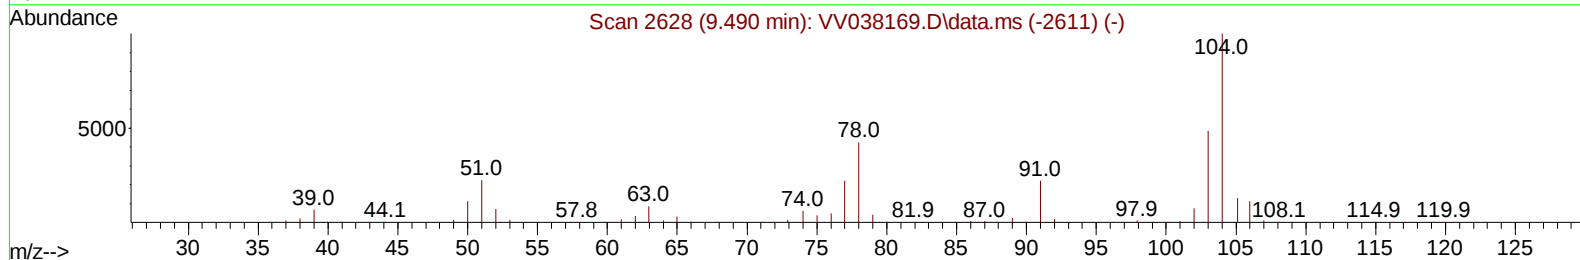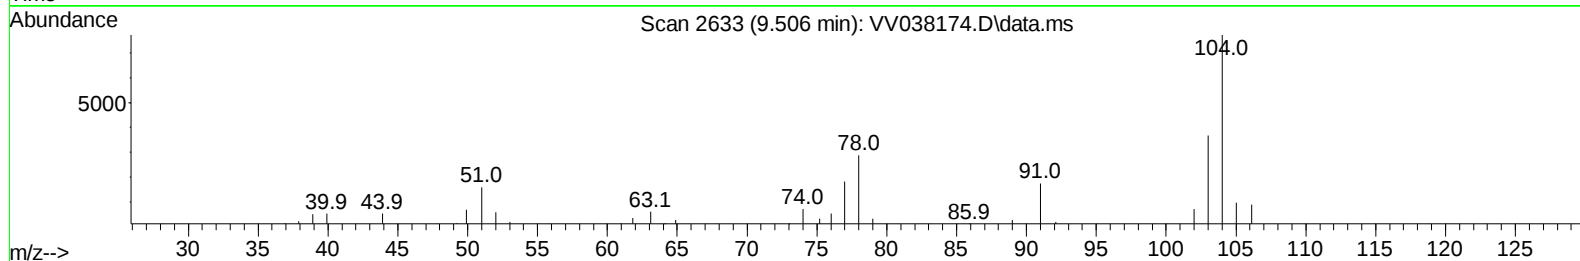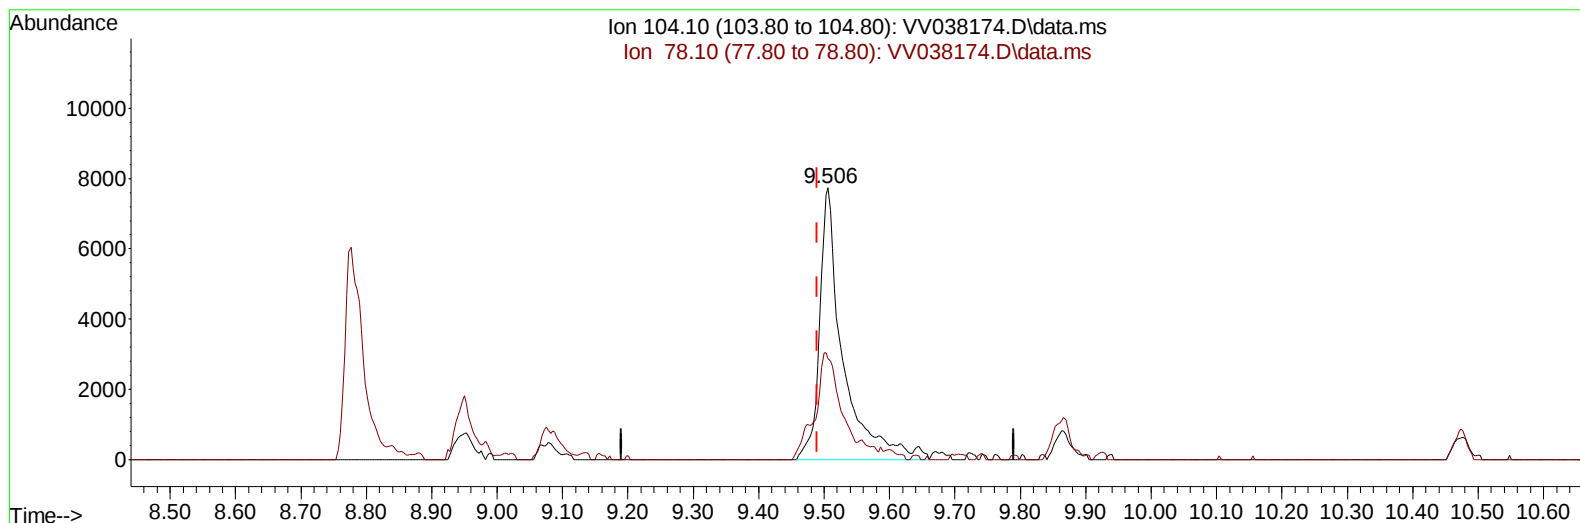

TIC: VV038174.D\data.ms

(55) Styrene (T)

9.506min (+ 0.016) 0.35 ug/L m

response 19081

Ion	Exp%	Act%
104.10	100.00	100.00
78.10	42.40	37.20
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
 Data File : VV038174.D
 Acq On : 19 Nov 2024 13:17
 Operator : SY/MD
 Sample : VSTD0.519
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 19 21:34:01 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
 Supervised By :Semsettin Yesilyurt 11/21/2024

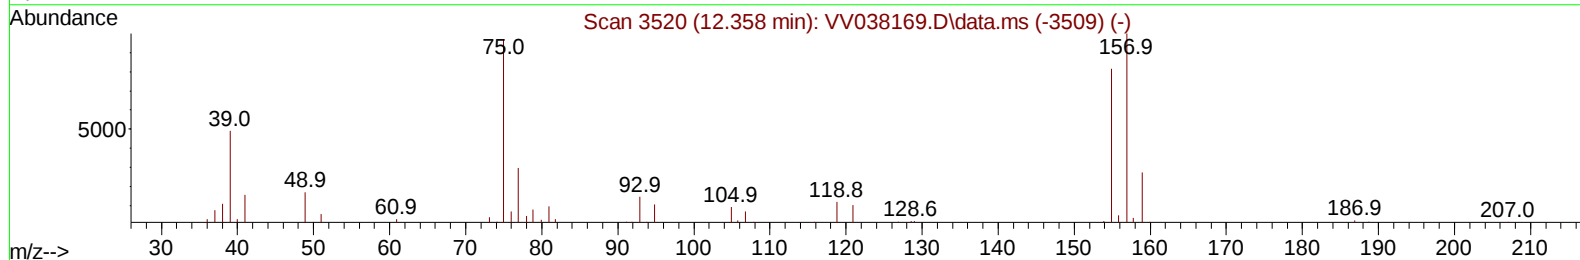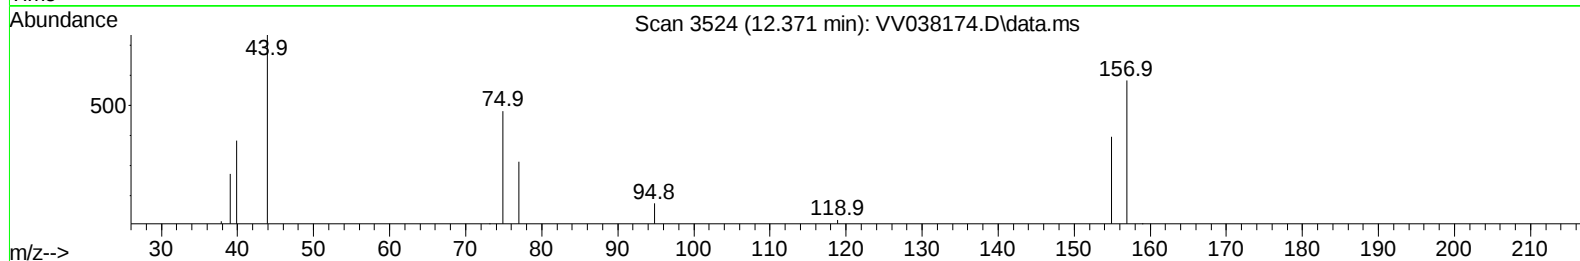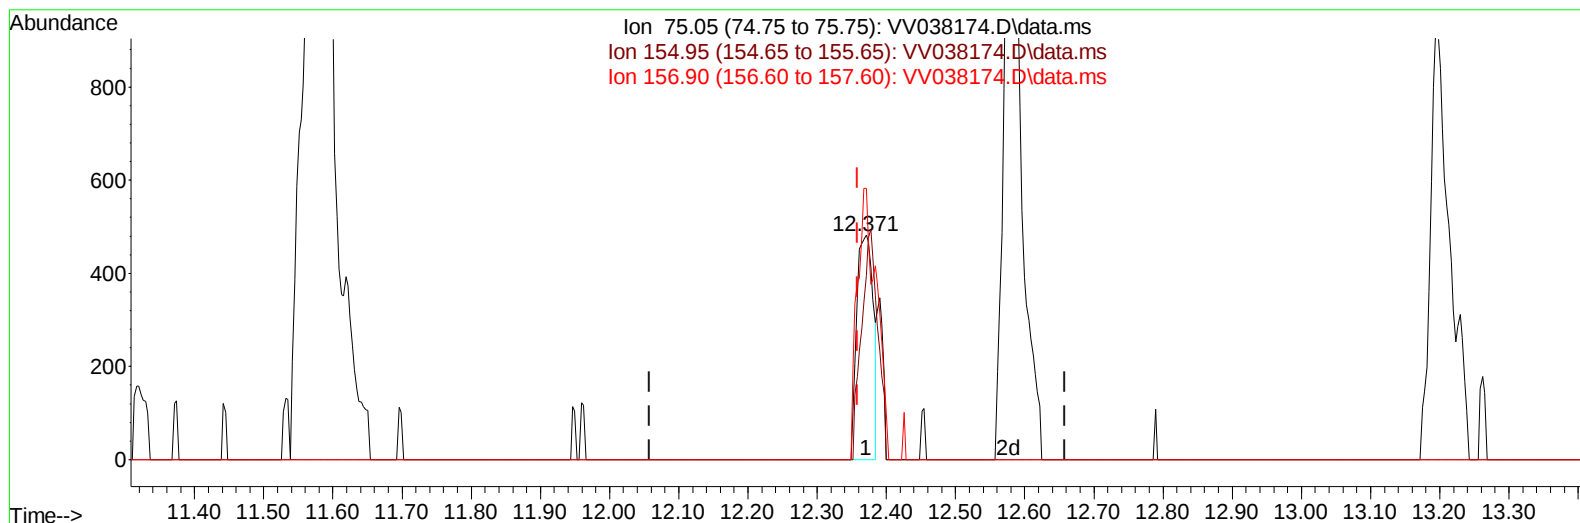

TIC: VV038174.D\data.ms

(68) 1,2-Dibromo-3-chloropropane (T)

12.371min (+ 0.013) 0.31 ug/L

response 782

Ion	Exp%	Act%
75.05	100.00	100.00
154.95	84.40	82.16
156.90	103.40	120.95
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038174.D
Acq On : 19 Nov 2024 13:17
Operator : SY/MD
Sample : VSTD0.519
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

Quant Time: Nov 19 21:38:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 19 21:34:01 2024
Response via : Initial Calibration

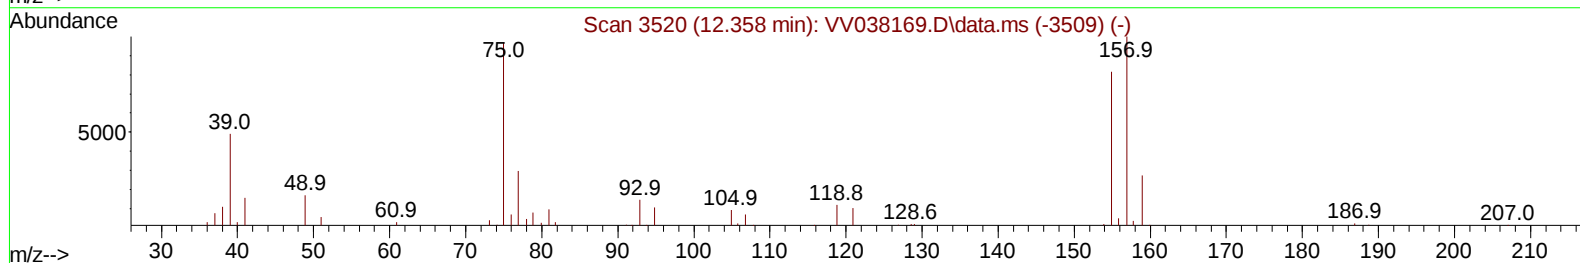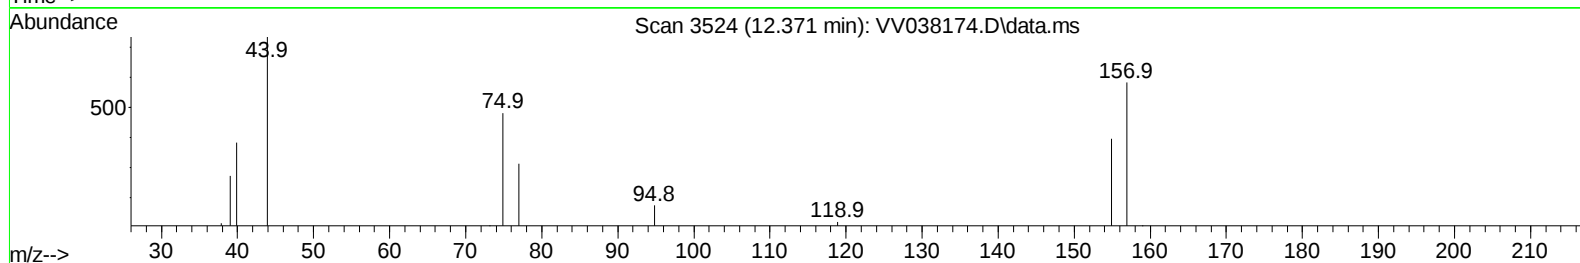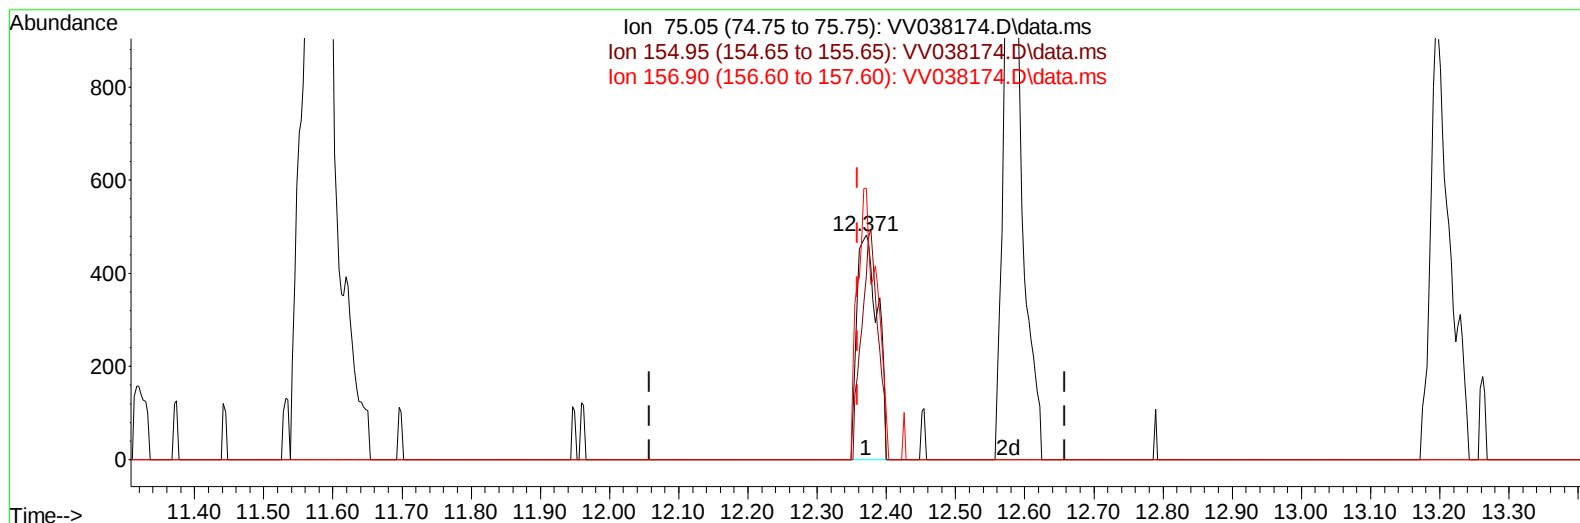

TIC: VV038174.D\data.ms

(68) 1,2-Dibromo-3-chloropropane (T)

12.371min (+ 0.013) 0.40 ug/L m

response 1001

Ion	Exp%	Act%
75.05	100.00	100.00
154.95	84.40	82.16
156.90	103.40	120.95
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
 Data File : VV038174.D
 Acq On : 19 Nov 2024 13:17
 Operator : SY/MD
 Sample : VSTD0.519
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5221

Manual IntegrationsAPPROVED

Quant Time: Nov 19 21:38:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 19 21:34:01 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2024
 Supervised By :Semsettin Yesilyurt 11/21/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	259388	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	269242	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	131394	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	9766	0.491	ug/L	0.00
7) Chloroethane-d5	1.529	69	7395	0.460	ug/L	0.00
11) 1,1-Dichloroethene-d2	2.056	65	3881	0.454	ug/L	0.00
20) 2-Butanone-d5	3.895	46	17129m	4.517	ug/L	0.10
24) Chloroform-d	4.249	84	16967	0.440	ug/L	0.00
26) 1,2-Dichloroethane-d4	4.953	65	7712m	0.442	ug/L	0.02
32) Benzene-d6	4.966	84	28623	0.411	ug/L	0.02
36) 1,2-Dichloropropane-d6	5.992	67	11098m	0.520	ug/L	0.00
41) Toluene-d8	7.246	98	24073	0.374	ug/L	0.00
43) trans-1,3-Dichloroprop...	7.574	79	2695m	0.346	ug/L	0.02
46) 2-Hexanone-d5	8.050	63	10443m	3.536	ug/L	0.03
56) 1,1,2,2-Tetrachloroeth...	10.152	84	8500	0.468	ug/L	0.00
66) 1,2-Dichlorobenzene-d4	11.561	152	10213	0.456	ug/L	0.00
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.105	85	11660	0.475	ug/L	100
3) Chloromethane	1.214	50	10274	0.486	ug/L	98
5) Vinyl chloride	1.278	62	11168	0.466	ug/L #	77
6) Bromomethane	1.484	94	4679	0.501	ug/L	87
8) Chloroethane	1.545	64	7559m	0.451	ug/L	
9) Trichlorofluoromethane	1.709	101	15791	0.463	ug/L	100
10) 1,1,2-Trichloro-1,2,2-...	2.063	101	8653	0.445	ug/L	95
12) 1,1-Dichloroethene	2.063	96	8938	0.482	ug/L	95
13) Acetone	2.133	43	14093	4.791	ug/L	97
14) Carbon disulfide	2.233	76	26927	0.451	ug/L	99
15) Methyl Acetate	2.410	43	3539	0.489	ug/L #	76
16) Methylene chloride	2.442	84	9437	0.447	ug/L	93
17) Methyl tert-butyl Ether	2.699	73	17723	0.423	ug/L	98
18) trans-1,2-Dichloroethene	2.693	96	8619	0.442	ug/L	89
19) 1,1-Dichloroethane	3.108	63	15801	0.446	ug/L	98
21) 2-Butanone	3.950	43	20103m	5.127	ug/L	
22) cis-1,2-Dichloroethene	3.818	96	8069	0.400	ug/L	92
23) Bromochloromethane	4.156	128	4216	0.428	ug/L	84
25) Chloroform	4.275	83	17415	0.459	ug/L	92
27) 1,2-Dichloroethane	5.063	62	8609	0.417	ug/L #	85
29) 1,1,1-Trichloroethane	4.506	97	14790	0.458	ug/L	95
30) Cyclohexane	4.574	56	11521	0.430	ug/L	93
31) Carbon tetrachloride	4.725	117	12707	0.446	ug/L	97
33) Benzene	5.014	78	30225	0.400	ug/L	100
34) Trichloroethene	5.844	95	9336	0.453	ug/L	98
35) Methylcyclohexane	6.046	83	12556	0.431	ug/L	93
37) 1,2-Dichloropropane	6.101	63	7818	0.413	ug/L	99
38) Bromodichloromethane	6.439	83	10186	0.400	ug/L #	87
39) cis-1,3-Dichloropropene	6.976	75	10226m	0.399	ug/L	
40) 4-Methyl-2-pentanone	7.165	43	39115m	4.012	ug/L	
42) Toluene	7.323	91	31202	0.390	ug/L	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
 Data File : VV038174.D
 Acq On : 19 Nov 2024 13:17
 Operator : SY/MD
 Sample : VSTD0.519
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5221

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/21/2024
 Supervised By :Semsettin Yesilyurt 11/21/2024

Quant Time: Nov 19 21:38:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 19 21:34:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) trans-1,3-Dichloropropene	7.603	75	7876m	0.358	ug/L	
45) 1,1,2-Trichloroethane	7.773	97	6728	0.438	ug/L	96
47) Tetrachloroethene	7.908	164	7388	0.446	ug/L	89
48) 2-Hexanone	8.095	43	26868m	3.993	ug/L	
49) Dibromochloromethane	8.178	129	6642	0.397	ug/L	98
50) 1,2-Dibromoethane	8.287	107	6094	0.428	ug/L	87
51) Chlorobenzene	8.815	112	23562	0.427	ug/L	94
52) Ethylbenzene	8.947	91	33596	0.395	ug/L	99
53) m,p-Xylene	9.075	106	11751	0.366	ug/L	95
54) o-Xylene	9.477	106	11476	0.368	ug/L	95
55) Styrene	9.506	104	19081m	0.351	ug/L	
57) 1,1,2,2-Tetrachloroethane	10.178	83	8100	0.451	ug/L	99
59) Bromoform	9.667	173	3011	0.394	ug/L #	98
60) Isopropylbenzene	9.863	105	30222	0.399	ug/L	98
61) 1,2,3-Trichloropropane	10.210	75	5696	0.506	ug/L #	86
62) 1,3,5-Trimethylbenzene	10.474	105	23963	0.399	ug/L	97
63) 1,2,4-Trimethylbenzene	10.847	105	21643	0.361	ug/L	93
64) 1,3-Dichlorobenzene	11.120	146	18276	0.450	ug/L	97
65) 1,4-Dichlorobenzene	11.207	146	18922	0.461	ug/L	97
67) 1,2-Dichlorobenzene	11.577	146	17107	0.455	ug/L	95
68) 1,2-Dibromo-3-chloropr...	12.371	75	1001m	0.396	ug/L	
69) 1,3,5-Trichlorobenzene	12.580	180	13436	0.467	ug/L	98
70) 1,2,4-trichlorobenzene	13.200	180	10417	0.438	ug/L	91
71) Naphthalene	13.445	128	16944	0.458	ug/L #	95
72) 1,2,3-Trichlorobenzene	13.680	180	9825	0.447	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5221

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

Reviewed By :Mahesh Dadoda 11/21/2024
Supervised By :Semsettin Yesilyurt 11/21/2024

