

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
 Data File : VV038189.D
 Acq On : 19 Nov 2024 20:10
 Operator : SY/MD
 Sample : P4882-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3J3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038189.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	14	21	33	rVB2	81562	103802	1.38%	0.410%
2	1.275	66	73	86	rBV	124354	132162	1.75%	0.522%
3	1.529	144	152	164	rBV	113119	134739	1.79%	0.532%
4	1.831	235	246	282	rBV	4154525	6130940	81.26%	24.228%
5	2.053	306	315	327	rVB2	230887	332369	4.41%	1.313%
6	2.699	503	516	536	rBV	62304	131433	1.74%	0.519%
7	3.783	844	853	854	rBV	129566	146988	1.95%	0.581%
8	4.243	980	996	1023	rBV	158335	439235	5.82%	1.736%
9	4.950	1202	1216	1246	rBV3	336336	898245	11.91%	3.550%
10	5.529	1386	1396	1426	rBV2	229313	508505	6.74%	2.009%
11	5.821	1473	1487	1525	rBV	3861271	7544793	100.00%	29.815%
12	5.982	1526	1537	1567	rVB	204792	454986	6.03%	1.798%
13	6.911	1817	1826	1855	rBV2	84391	182062	2.41%	0.719%
14	7.239	1915	1928	1947	rBV	356152	663549	8.79%	2.622%
15	7.554	2017	2026	2049	rBV2	50544	107277	1.42%	0.424%
16	7.895	2114	2132	2158	rBV	2453546	4165130	55.21%	16.460%
17	8.017	2161	2170	2221	rVB	469631	950574	12.60%	3.756%
18	8.779	2397	2407	2437	rBV	404035	728450	9.66%	2.879%
19	10.146	2821	2832	2852	rBV	180590	301373	3.99%	1.191%
20	11.181	3143	3154	3185	rBV	347500	600884	7.96%	2.375%
21	11.554	3259	3270	3290	rBV	371645	647625	8.58%	2.559%




Sum of corrected areas: 25305121

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038189.D
Acq On : 19 Nov 2024 20:10
Operator : SY/MD
Sample : P4882-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3J3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

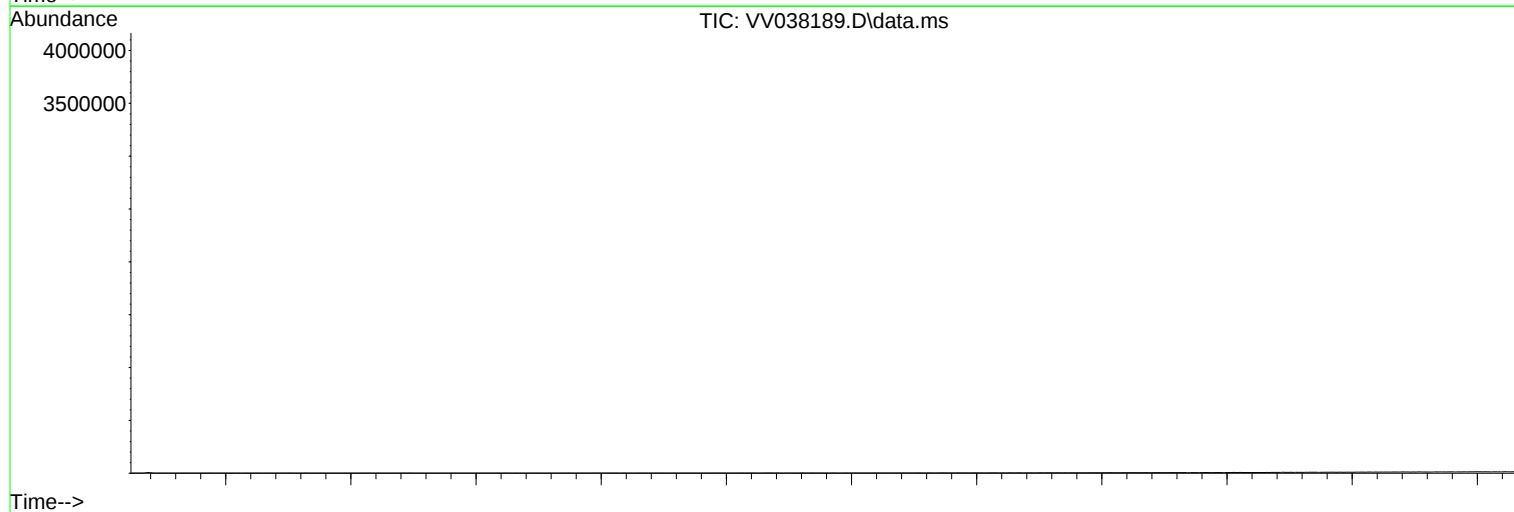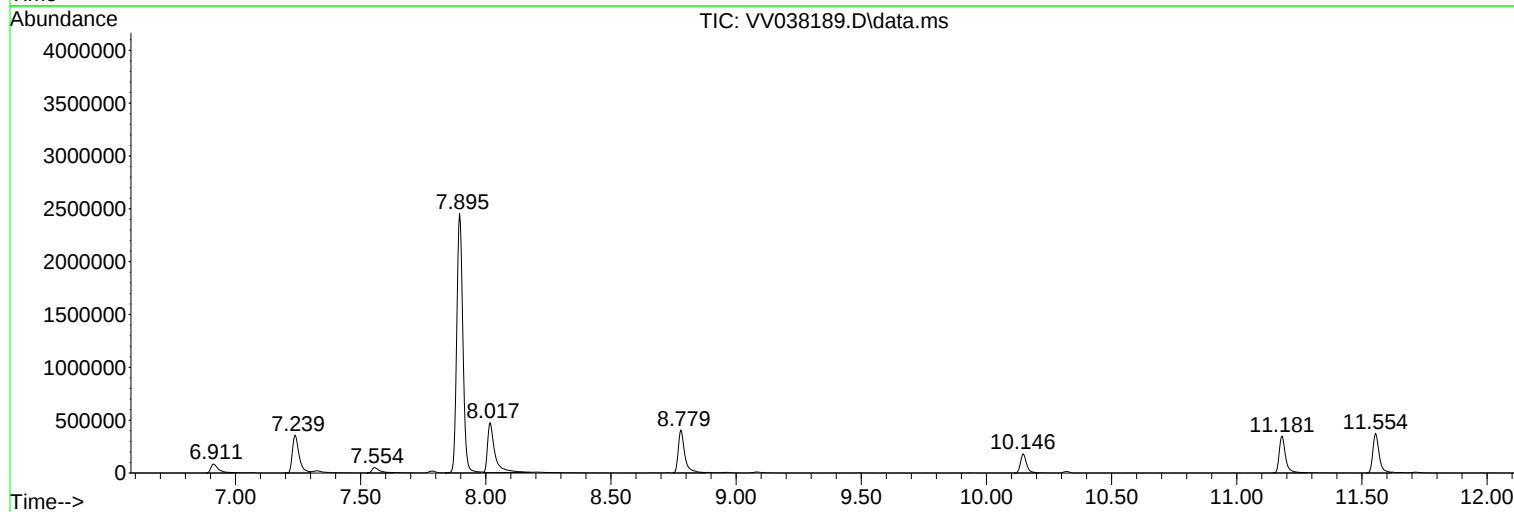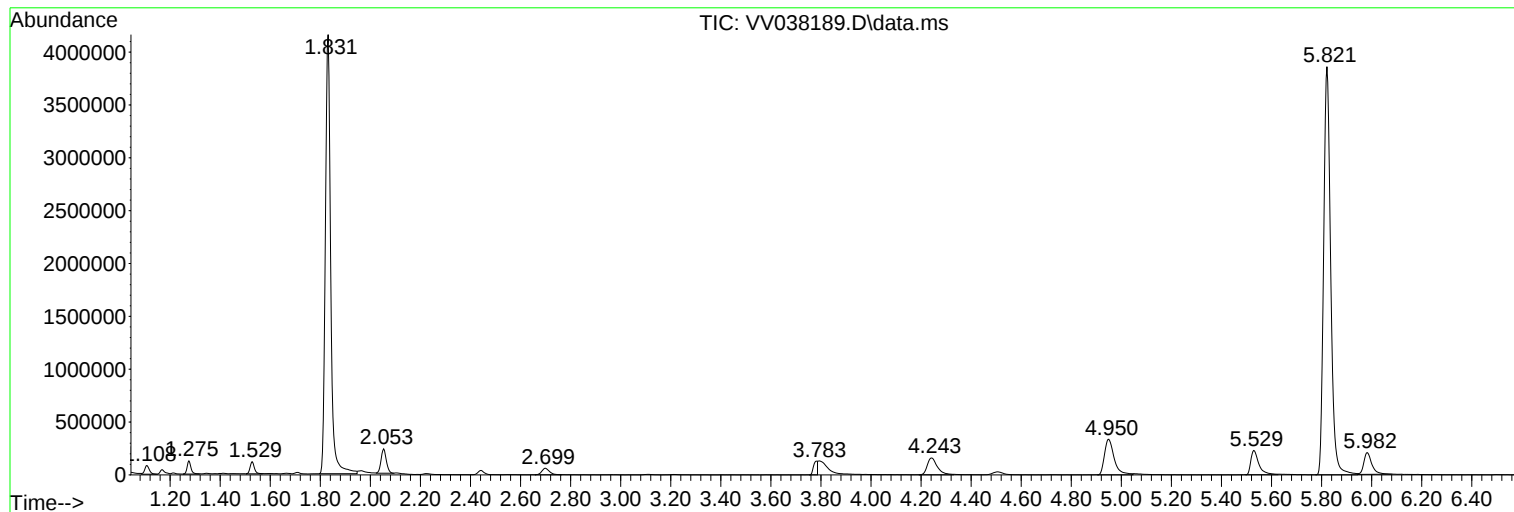

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038189.D
Acq On : 19 Nov 2024 20:10
Operator : SY/MD
Sample : P4882-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3J3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038189.D
Acq On : 19 Nov 2024 20:10
Operator : SY/MD
Sample : P4882-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3J3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc