
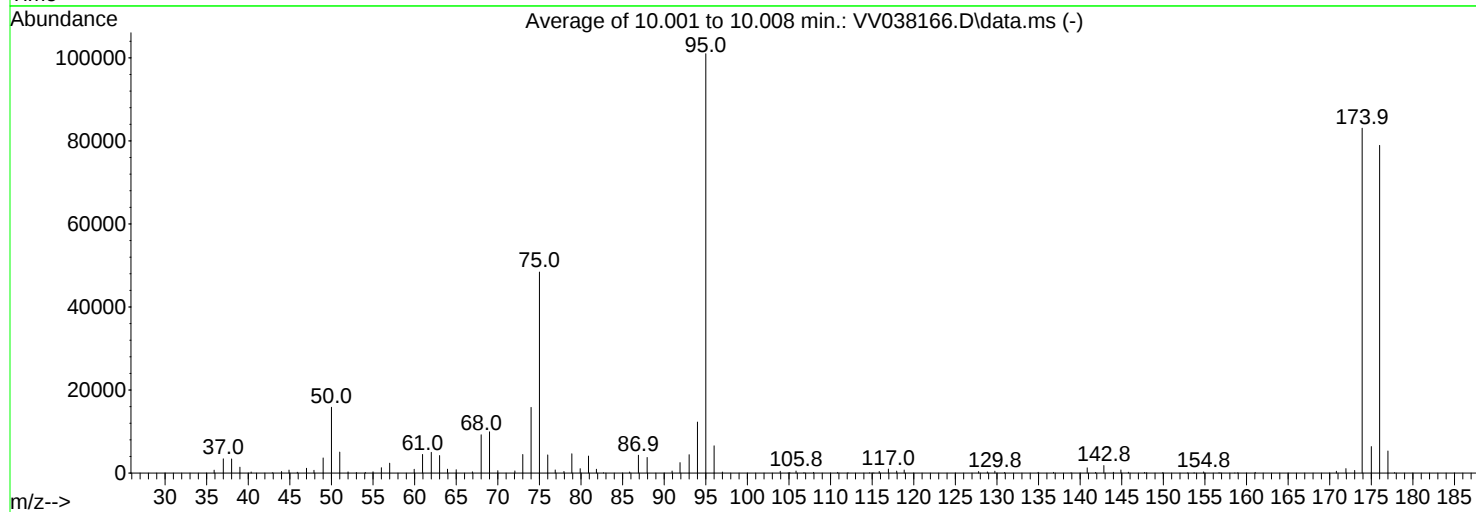


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111924\
Data File : VV038166.D
Acq On : 19 Nov 2024 08:20
Operator : SY/MD
Sample : BFB287
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB287

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Nov 21 01:41:56 2024

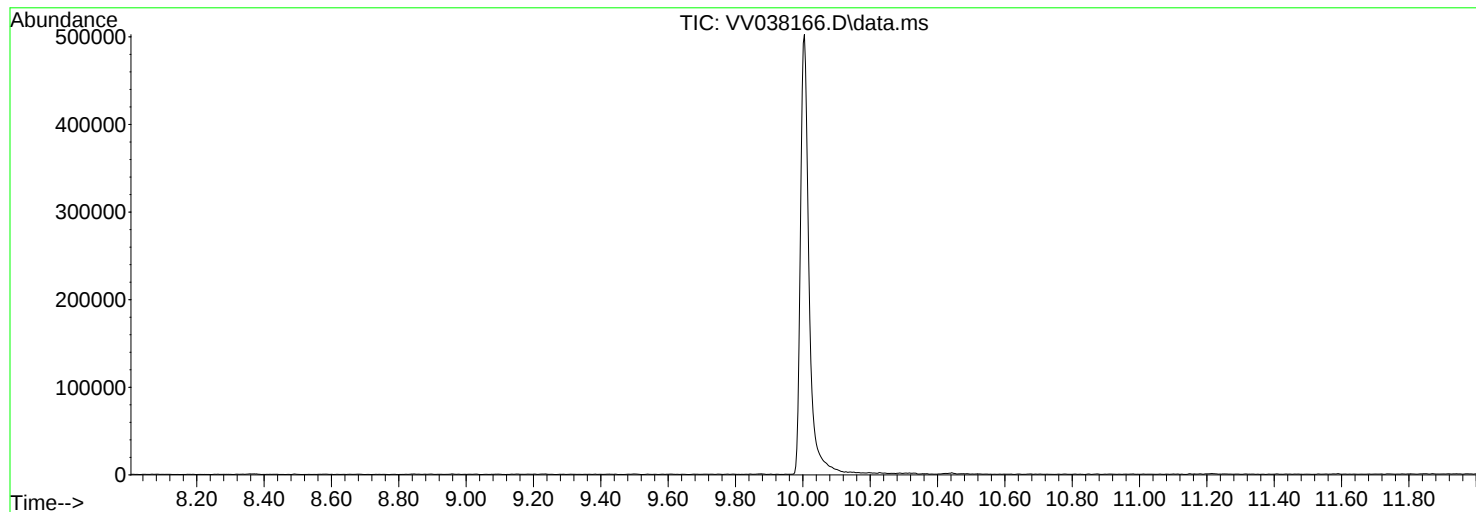

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	15848	PASS
75	95	30	80	47.9	48419	PASS
95	95	100	100	100.0	100997	PASS
96	95	5	9	6.5	6575	PASS
173	174	0.00	2	0.8	635	PASS
174	95	50	120	82.2	83061	PASS
175	174	5	9	7.7	6383	PASS
176	174	95	105	95.0	78928	PASS
177	176	5	10	6.7	5317	PASS

Scan 2775 (9.963 min): VV038166.D\data.ms
BFB287

m/z	Abundance
39.90	264.0
44.00	446.0

Instrument :
MSVOA_V
ClientSampleId :
BFB287

m/z	Abundance
35.90	790.0
37.00	3589.0
38.00	3466.0
39.00	1366.0
39.80	220.0
40.40	257.0
42.90	143.0
44.00	887.0
44.90	841.0
45.90	295.0
47.00	1091.0
47.80	697.0
49.00	3621.0
50.00	16126.0
51.00	5225.0
52.00	275.0
52.90	146.0
54.10	111.0
55.00	305.0
56.00	1412.0
57.00	2393.0
59.90	868.0
61.00	4537.0
62.00	5261.0
63.00	4327.0
64.00	948.0
65.00	831.0
66.90	309.0
68.00	9281.0
69.00	10182.0
70.00	553.0
72.10	636.0
73.00	4621.0
74.00	15947.0
75.00	49336.0
76.00	4260.0
76.90	686.0
77.90	420.0
78.90	4814.0
79.90	956.0
80.90	4211.0
81.90	825.0
85.80	257.0
86.90	4623.0
88.00	3906.0
91.00	558.0
91.90	2581.0
93.00	4516.0
94.00	12409.0
95.00	103600.0
96.00	7063.0
97.00	208.0
104.00	452.0
104.90	129.0
105.90	484.0
106.80	104.0
108.00	144.0
110.90	181.0
112.10	121.0
114.70	127.0
115.20	124.0
115.90	402.0
116.90	982.0
118.00	414.0
118.80	723.0
127.80	332.0
128.80	297.0
129.70	488.0
130.90	166.0
135.00	225.0
136.80	200.0
140.80	1211.0
141.90	114.0
142.90	1937.0
143.90	247.0
145.00	758.0
145.80	198.0
147.70	250.0
152.90	134.0
154.90	328.0
156.70	190.0
158.90	144.0
161.10	139.0
170.70	466.0
171.90	1073.0
173.90	82928.0
175.00	6709.0
176.00	77784.0
177.00	5188.0
177.80	189.0

Instrument :
MSVOA_V
ClientSampleId :
BFB287

m/z	Abundance
35.90	725.0
37.00	3494.0
38.00	3455.0
39.00	1464.0
39.90	205.0
40.40	276.0
42.90	140.0
44.00	814.0
44.90	733.0
45.90	210.0
47.00	1215.0
47.90	700.0
49.00	3791.0
50.00	16327.0
51.00	5158.0
52.00	277.0
53.00	133.0
54.10	141.0
55.00	335.0
56.00	1295.0
57.00	2456.0
60.00	908.0
61.00	4589.0
62.00	5129.0
63.00	4380.0
64.00	953.0
65.00	810.0
67.00	313.0
68.00	9581.0
69.00	10350.0
70.00	601.0
72.00	503.0
73.00	4635.0
74.00	16181.0
75.00	49968.0
76.00	4491.0
76.90	801.0
78.00	400.0
78.90	4785.0
79.90	1070.0
80.90	4214.0
81.80	981.0
82.70	130.0
85.80	318.0
86.90	4403.0
88.00	3867.0
91.00	503.0
91.90	2545.0
93.00	4508.0
94.00	12760.0
95.00	103872.0
96.00	6828.0
97.00	280.0
104.00	479.0
105.10	138.0
105.80	504.0
106.80	122.0
108.00	212.0
110.80	185.0
112.10	114.0
114.70	106.0
115.80	395.0
117.00	1011.0
117.90	492.0
118.80	779.0
127.80	377.0
128.80	289.0
129.80	476.0
130.90	155.0
135.00	191.0
136.80	174.0
138.90	106.0
140.90	1303.0
141.80	163.0
142.80	1875.0
144.00	190.0
144.90	787.0
145.80	221.0
147.80	236.0
149.90	117.0
153.70	115.0
154.90	325.0
156.70	168.0
159.00	116.0
161.10	184.0
170.80	435.0
171.90	1108.0
173.00	1007.0
173.90	85440.0
175.00	6516.0
176.00	81280.0
177.00	5539.0

Instrument :
MSVOA_V
ClientSampleId :
BFB287

177.80

151.0

Instrument :

MSVOA_V

ClientSampleId :

BFB287

m/z	Abundance
35.90	619.0
37.00	3232.0
38.00	3297.0
39.00	1434.0
39.90	202.0
40.30	265.0
44.00	753.0
44.90	609.0
45.90	125.0
47.00	1156.0
48.00	612.0
49.00	3525.0
50.00	15092.0
51.00	4775.0
52.00	331.0
53.10	127.0
54.10	123.0
55.00	312.0
56.00	1175.0
57.00	2308.0
60.00	950.0
60.90	4328.0
62.00	4597.0
63.00	3954.0
63.90	910.0
65.00	783.0
67.00	287.0
68.00	8799.0
69.00	9300.0
70.00	602.0
72.00	424.0
73.00	4183.0
74.00	15312.0
75.00	45952.0
76.00	4359.0
76.90	764.0
78.00	346.0
78.90	4362.0
79.90	1176.0
80.90	3896.0
81.80	988.0
82.70	108.0
85.90	233.0
86.90	3887.0
87.90	3494.0
90.90	448.0
91.90	2429.0
93.00	4255.0
94.00	11703.0
95.00	95520.0
96.00	5834.0
97.00	273.0
103.90	402.0
105.10	172.0
105.80	488.0
106.80	123.0
107.90	176.0
110.80	138.0
115.80	389.0
117.00	907.0
117.90	527.0
118.90	739.0
127.80	414.0
128.90	276.0
129.80	438.0
130.90	121.0
134.90	149.0
136.80	136.0
138.90	105.0
140.90	1257.0
141.80	190.0
142.80	1649.0
144.10	164.0
144.80	728.0
145.80	203.0
148.00	262.0
149.90	125.0
153.70	133.0
154.80	224.0
156.90	125.0
158.60	110.0
161.00	160.0
170.90	407.0
172.00	1037.0
173.00	898.0
173.90	80816.0
175.00	5924.0
176.00	77720.0
177.00	5224.0

Instrument :
MSVOA_V
ClientSampleId :
BFB287