
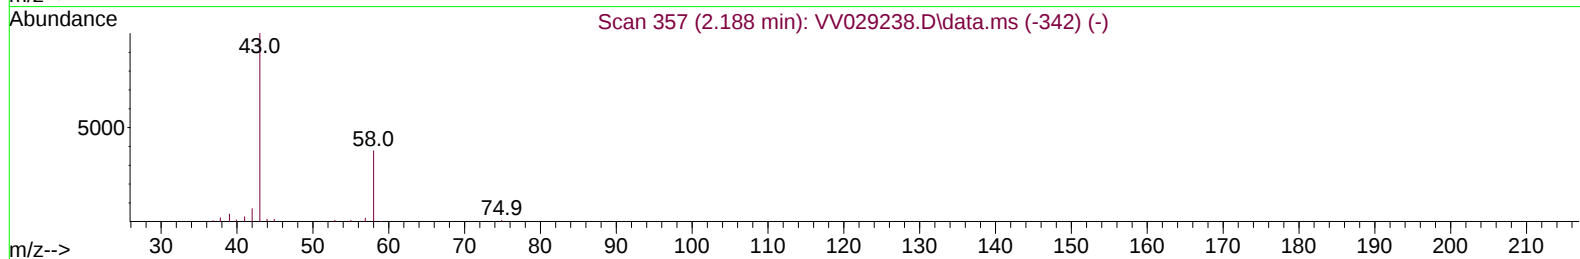
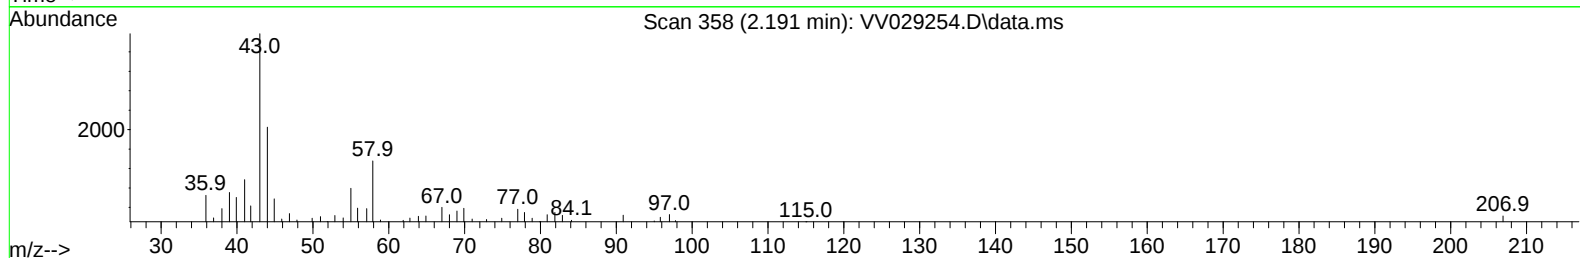


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029254.D
 Acq On : 21 Nov 2022 03:49
 Operator : SY/MD
 Sample : N5725-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Quant Time: Nov 21 05:12:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 21 03:37:08 2022
 Response via : Initial Calibration

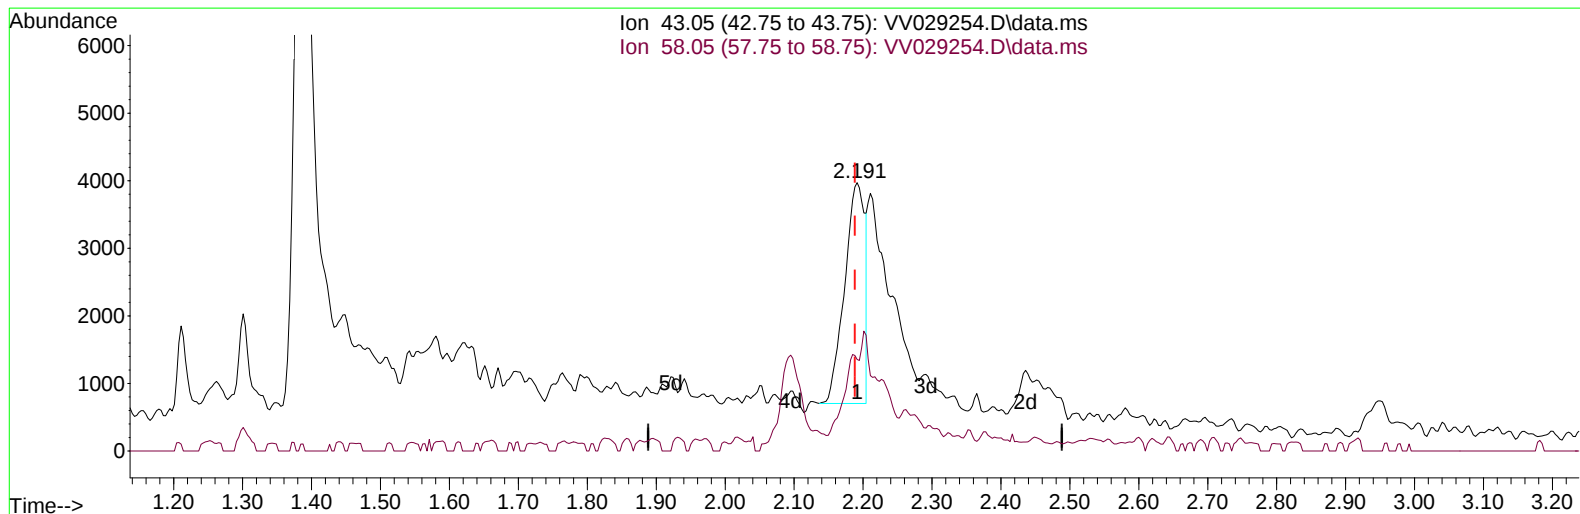

TIC: VV029254.D\data.ms

(13) Acetone (T)

2.191min (+ 0.003) 2.18 ug/L

response 6672

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	28.30	28.40
0.00	0.00	0.00
0.00	0.00	0.00