




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029253.D
Acq On : 21 Nov 2022 03:24
Operator : SY/MD
Sample : N5725-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB58

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 11/21/2022
Supervised By :Mahesh Dadoda 11/21/2022

Quant Time: Nov 21 03:58:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 21 03:37:08 2022
Response via : Initial Calibration

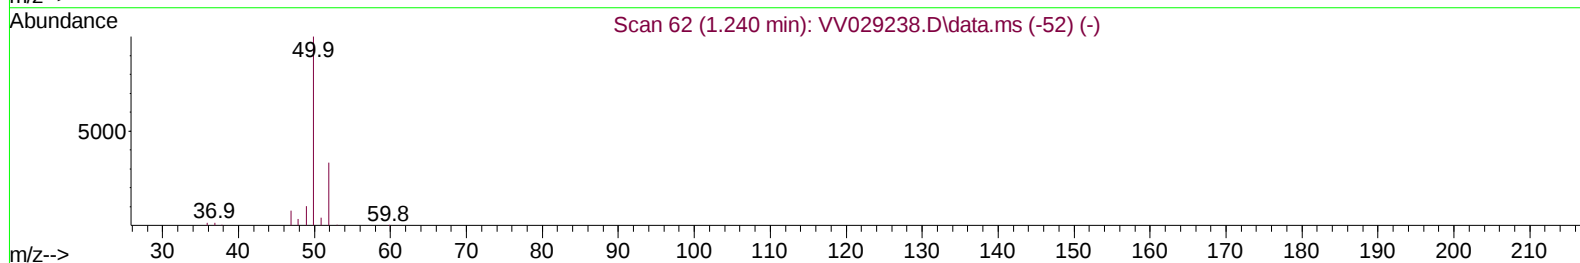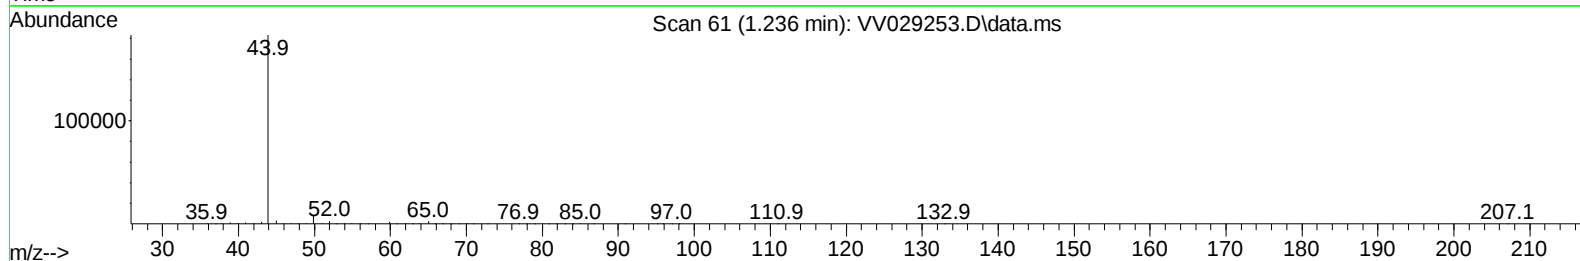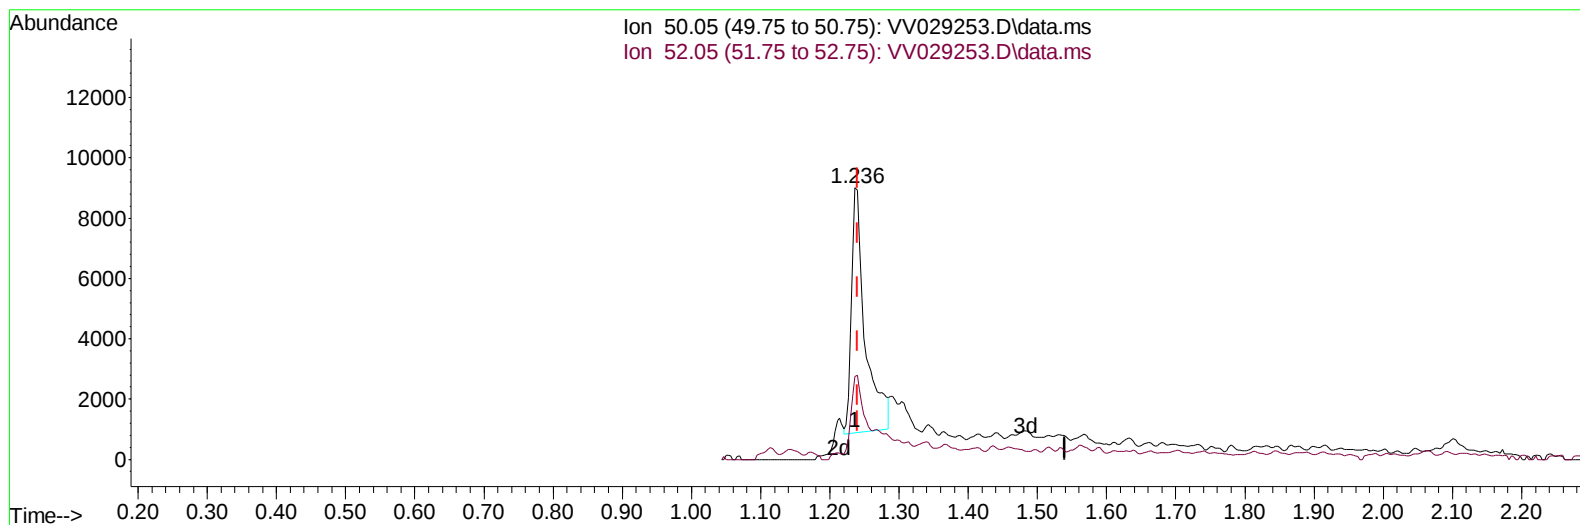

TIC: VV029253.D\data.ms

(3) Chloromethane (T)

1.236min (-0.003) 0.34 ug/L

response 11187

Ion	Exp%	Act%
50.05	100.00	100.00
52.05	33.80	30.62
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029253.D
 Acq On : 21 Nov 2022 03:24
 Operator : SY/MD
 Sample : N5725-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB58

Manual IntegrationsAPPROVED

Quant Time: Nov 21 03:58:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 21 03:37:08 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/21/2022
 Supervised By :Mahesh Dadoda 11/21/2022

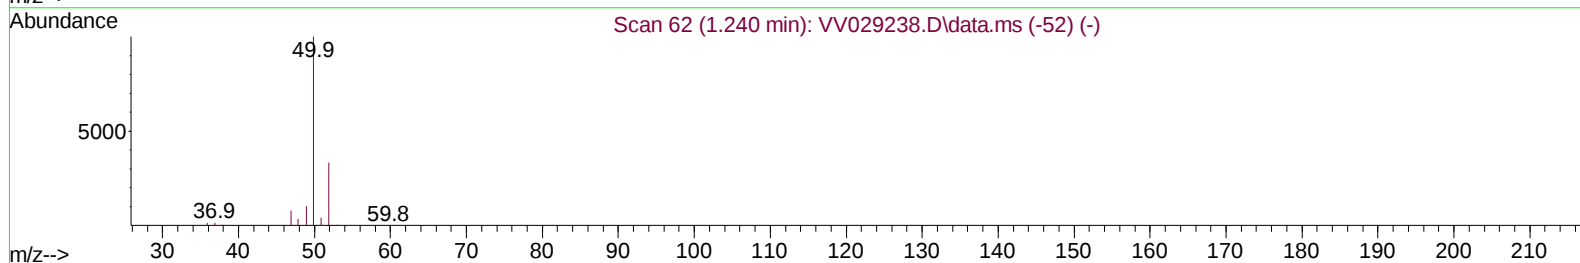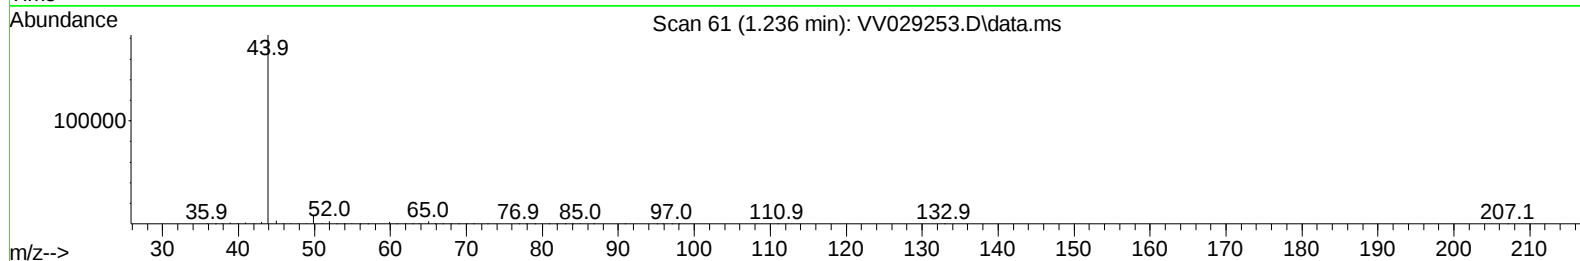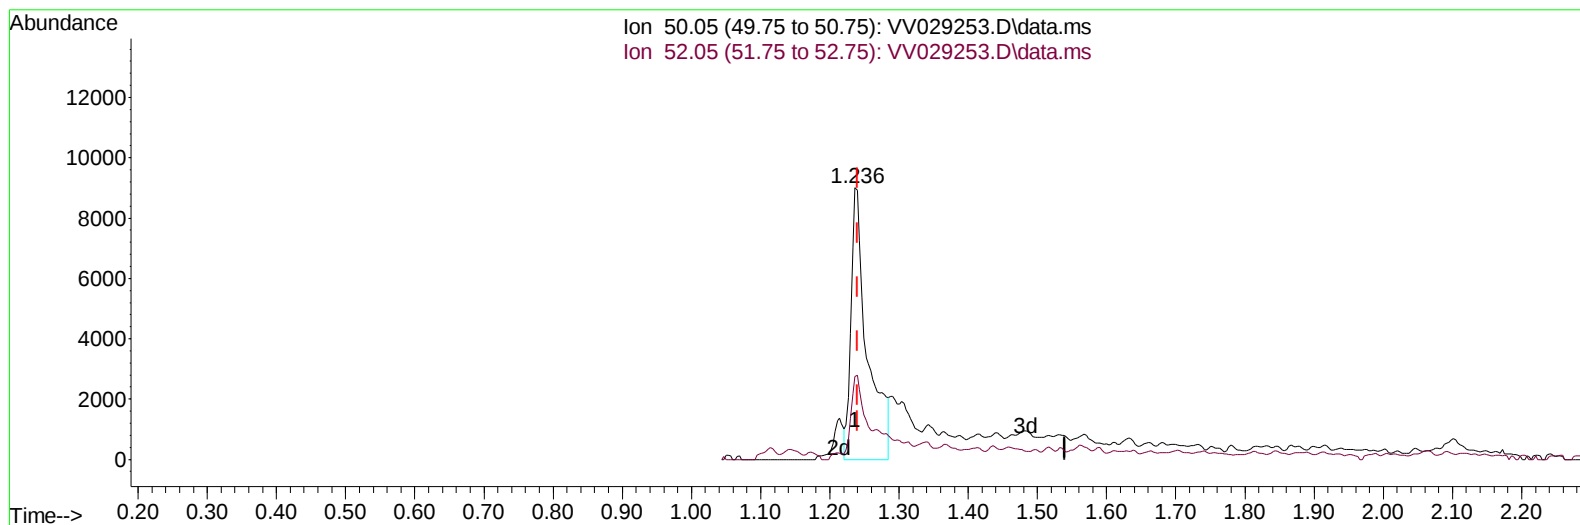

TIC: VV029253.D\data.ms

(3) Chloromethane (T)

1.236min (-0.003) 0.45 ug/L m

response 14744

Ion	Exp%	Act%
50.05	100.00	100.00
52.05	33.80	30.62
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029253.D
 Acq On : 21 Nov 2022 03:24
 Operator : SY/MD
 Sample : N5725-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB58

Manual IntegrationsAPPROVED

Quant Time: Nov 21 03:58:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 21 03:37:08 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/21/2022
 Supervised By :Mahesh Dadoda 11/21/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	470183	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	414759	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	207255	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	123529	4.309	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	86.200%	
7) Chloroethane-d5	1.564	69	107406	4.262	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	85.200%	
11) 1,1-Dichloroethene-d2	2.101	63	164130	3.142	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	62.800%	
20) 2-Butanone-d5	3.889	46	301708	62.878	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	125.760%	
24) Chloroform-d	4.336	84	238286	4.049	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	81.000%	
26) 1,2-Dichloroethane-d4	5.024	65	107472	4.059	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	81.200%	
32) Benzene-d6	5.040	84	506322	4.090	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	81.800%	
36) 1,2-Dichloropropane-d6	6.059	67	157724	4.562	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	91.200%	
41) Toluene-d8	7.307	98	438094	3.931	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	78.600%	
43) trans-1,3-Dichloroprop...	7.612	79	54180	4.805	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	96.200%	
46) 2-Hexanone-d5	8.082	63	246571	51.234	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	102.460%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	111250	4.642	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	92.800%	
66) 1,2-Dichlorobenzene-d4	11.615	152	164626	4.440	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	88.800%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.236	50	14744m	0.453	ug/L	
5) Vinyl chloride	1.304	62	89519	2.413	ug/L	99
12) 1,1-Dichloroethene	2.114	96	16316	0.573	ug/L #	1
13) Acetone	2.198	43	15715	5.091	ug/L	84
14) Carbon disulfide	2.291	76	33584	0.332	ug/L	98
18) trans-1,2-Dichloroethene	2.757	96	1574	0.048	ug/L	96
19) 1,1-Dichloroethane	3.182	63	239657	4.441	ug/L	99
22) cis-1,2-Dichloroethene	3.899	96	216461	6.450	ug/L	97
27) 1,2-Dichloroethane	5.127	62	5852	0.201	ug/L	97
29) 1,1,1-Trichloroethane	4.603	97	8328	0.171	ug/L	97
33) Benzene	5.092	78	140881	1.112	ug/L	100
34) Trichloroethene	5.905	95	34270	1.056	ug/L	94
51) Chlorobenzene	8.876	112	3734	0.044	ug/L #	84
53) m,p-Xylene	9.133	106	2782	0.049	ug/L	88
54) o-Xylene	9.535	106	3260	0.060	ug/L	96
60) Isopropylbenzene	9.924	105	74861	0.556	ug/L	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029253.D
 Acq On : 21 Nov 2022 03:24
 Operator : SY/MD
 Sample : N5725-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 BHB58

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 11/21/2022
 Supervised By :Mahesh Dadoda 11/21/2022

Quant Time: Nov 21 03:58:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 21 03:37:08 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev	(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed								

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029253.D
Acq On : 21 Nov 2022 03:24
Operator : SY/MD
Sample : N5725-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB58

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 11/21/2022
Supervised By :Mahesh Dadoda 11/21/2022

Quant Time: Nov 21 03:58:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 21 03:37:08 2022
Response via : Initial Calibration

