




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029254.D
Acq On : 21 Nov 2022 03:49
Operator : SY/MD
Sample : N5725-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB59

Manual IntegrationsAPPROVED

Quant Time: Nov 21 05:12:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR11122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 21 03:37:08 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 11/21/2022
Supervised By :Mahesh Dadoda 11/21/2022

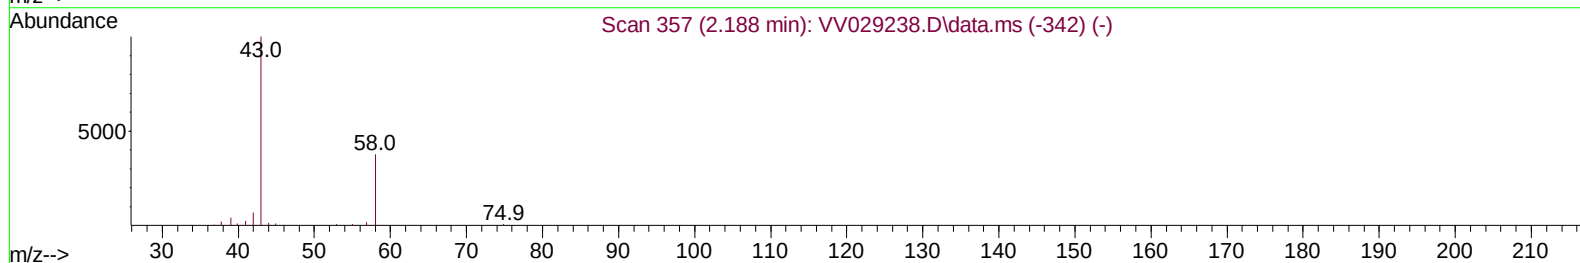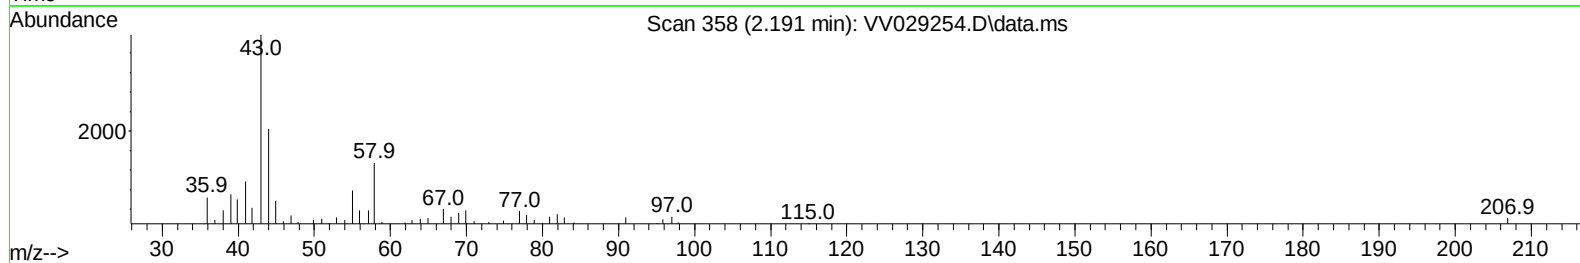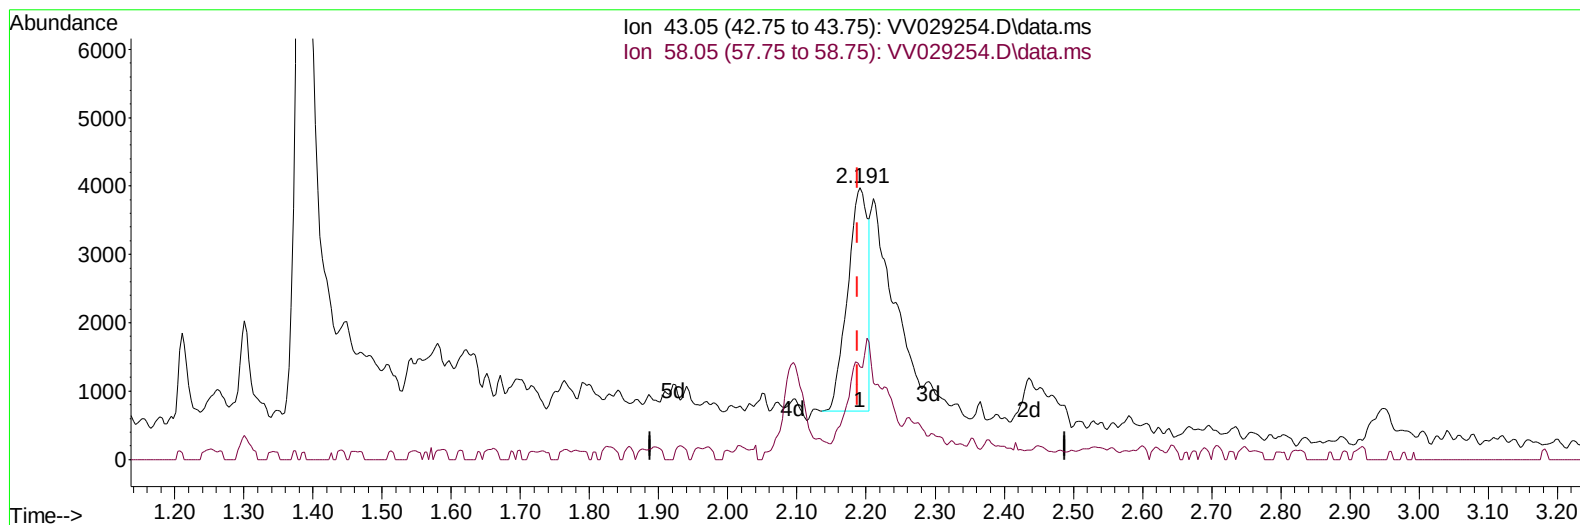

TIC: VV029254.D\data.ms

(13) Acetone (T)

2.191min (+ 0.003) 2.18 ug/L

response 6672

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	28.30	28.40
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029254.D
 Acq On : 21 Nov 2022 03:49
 Operator : SY/MD
 Sample : N5725-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB59

Manual IntegrationsAPPROVED

Quant Time: Nov 21 05:12:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 21 03:37:08 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/21/2022
 Supervised By :Mahesh Dadoda 11/21/2022

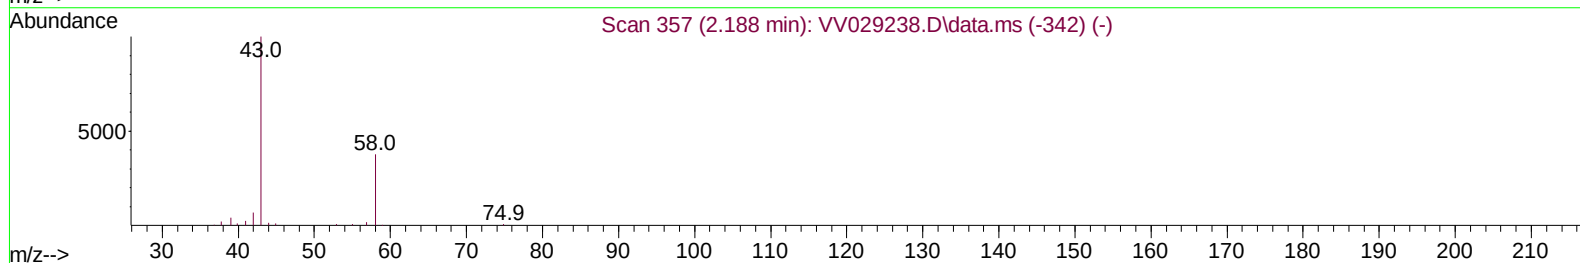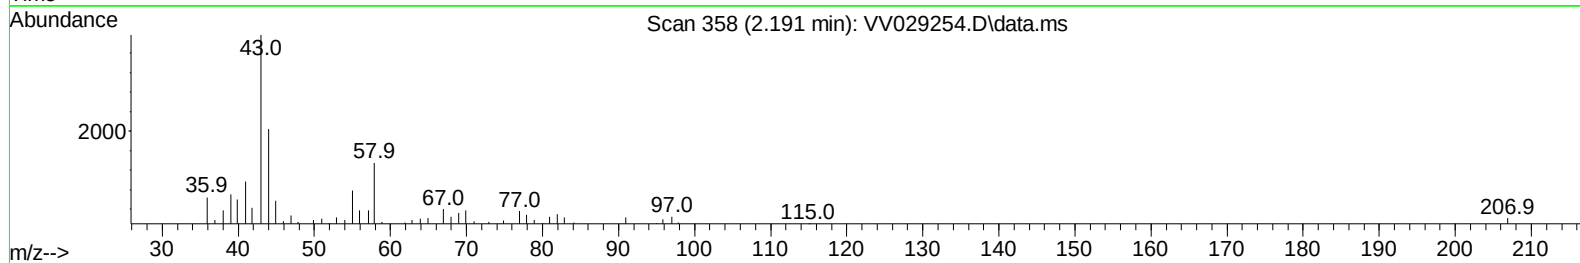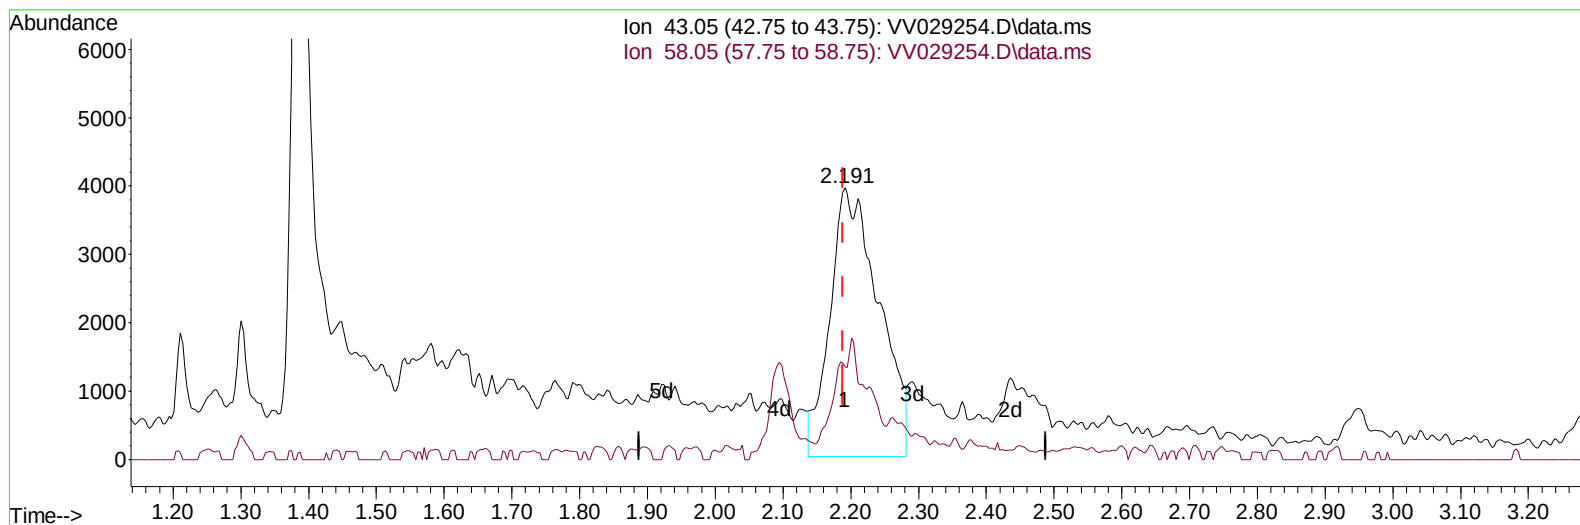

TIC: VV029254.D\data.ms

(13) Acetone (T)

2.191min (+ 0.003) 6.44 ug/L m

response 19713

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	28.30	9.61
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029254.D
 Acq On : 21 Nov 2022 03:49
 Operator : SY/MD
 Sample : N5725-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB59

Manual IntegrationsAPPROVED

Quant Time: Nov 21 05:12:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 21 03:37:08 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/21/2022
 Supervised By :Mahesh Dadoda 11/21/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	466339	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	403370	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	197912	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	121398	4.270	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	85.400%		
7) Chloroethane-d5	1.564	69	106511	4.262	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	85.200%		
11) 1,1-Dichloroethene-d2	2.101	63	151349	2.921	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	58.400%#		
20) 2-Butanone-d5	3.892	46	290699	61.083	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	122.160%		
24) Chloroform-d	4.339	84	233345	3.998	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	80.000%		
26) 1,2-Dichloroethane-d4	5.024	65	105574	4.020	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	80.400%		
32) Benzene-d6	5.040	84	485509	4.032	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	80.600%		
36) 1,2-Dichloropropane-d6	6.059	67	152678	4.541	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	90.800%		
41) Toluene-d8	7.307	98	418355	3.860	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	77.200%		
43) trans-1,3-Dichloroprop...	7.616	79	51495	4.696	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	94.000%		
46) 2-Hexanone-d5	8.082	63	247904	52.965	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	105.940%		
56) 1,1,2,2-Tetrachloroeth...	10.207	84	106987	4.590	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	91.800%		
66) 1,2-Dichlorobenzene-d4	11.612	152	153884	4.346	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	87.000%		
Target Compounds						
						Qvalue
3) Chloromethane	1.236	50	11521	0.357	ug/L	98
13) Acetone	2.191	43	19713m	6.439	ug/L	
14) Carbon disulfide	2.294	76	83903	0.837	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029254.D
Acq On : 21 Nov 2022 03:49
Operator : SY/MD
Sample : N5725-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB59

Manual IntegrationsAPPROVED

Quant Time: Nov 21 05:12:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 21 03:37:08 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 11/21/2022
Supervised By :Mahesh Dadoda 11/21/2022

