




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029259.D
 Acq On : 21 Nov 2022 05:51
 Operator : SY/MD
 Sample : N5725-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB66

Manual IntegrationsAPPROVED

Quant Time: Nov 21 06:11:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 21 03:37:08 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/21/2022
 Supervised By :Mahesh Dadoda 11/21/2022

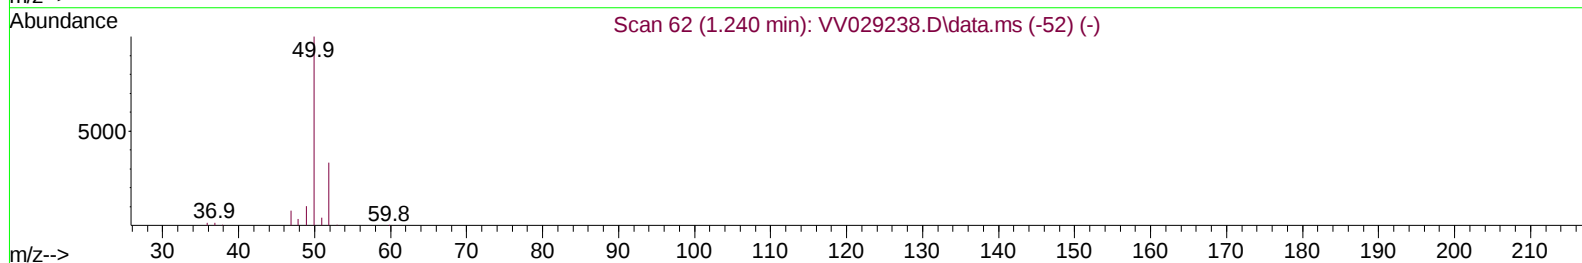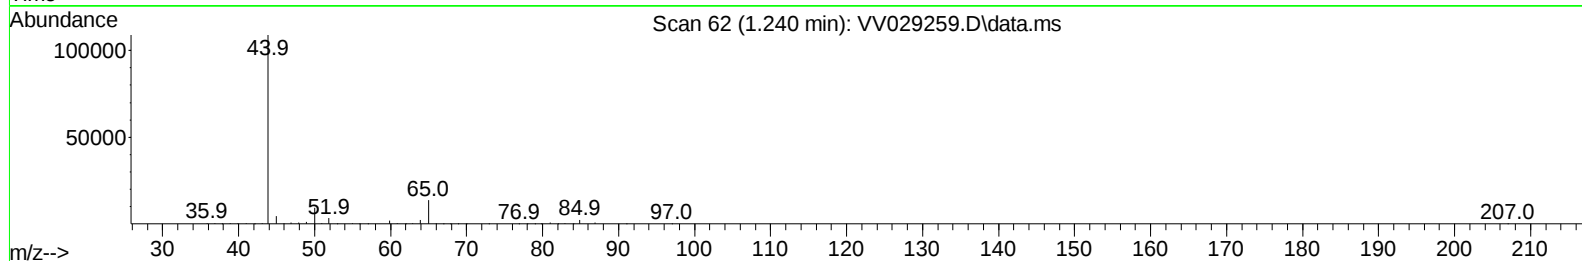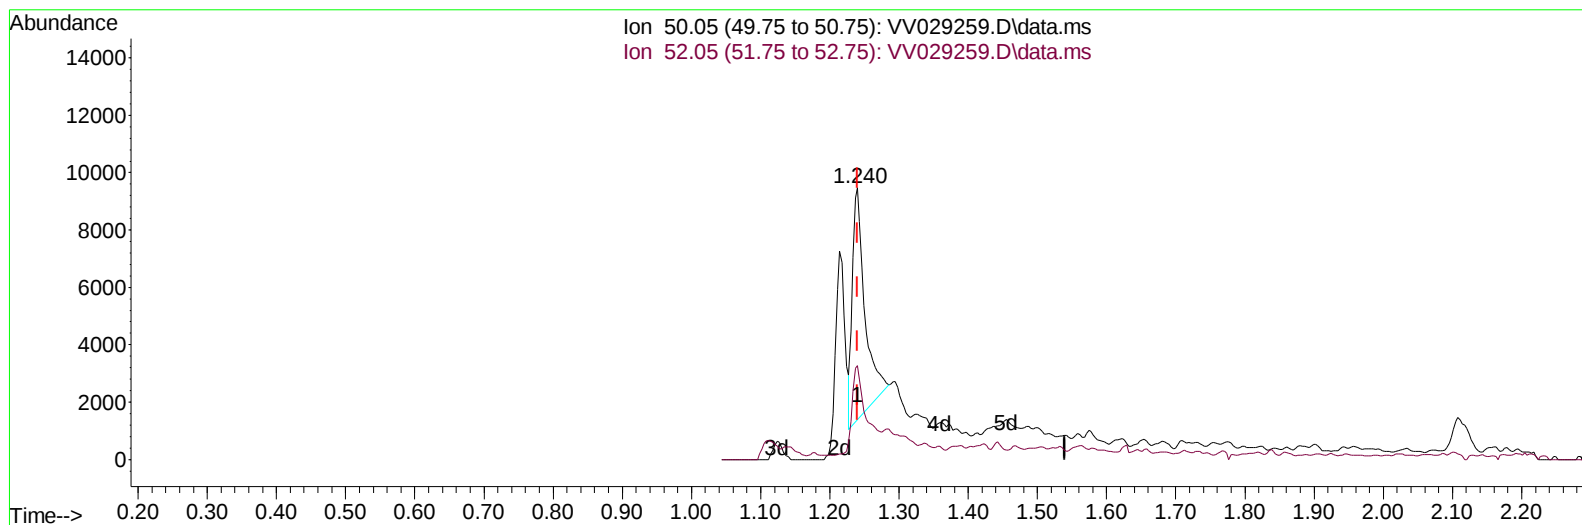

TIC: VV029259.D\data.ms

(3) Chloromethane (T)

1.240min (+ 0.000) 0.31 ug/L

response 10284

Ion	Exp%	Act%
50.05	100.00	100.00
52.05	33.80	34.49
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029259.D
 Acq On : 21 Nov 2022 05:51
 Operator : SY/MD
 Sample : N5725-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB66

Manual IntegrationsAPPROVED

Quant Time: Nov 21 06:11:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 21 03:37:08 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/21/2022
 Supervised By :Mahesh Dadoda 11/21/2022

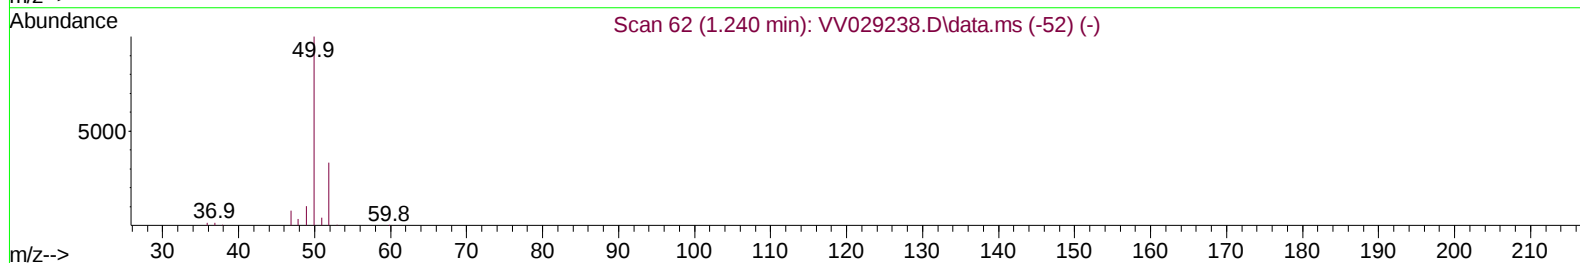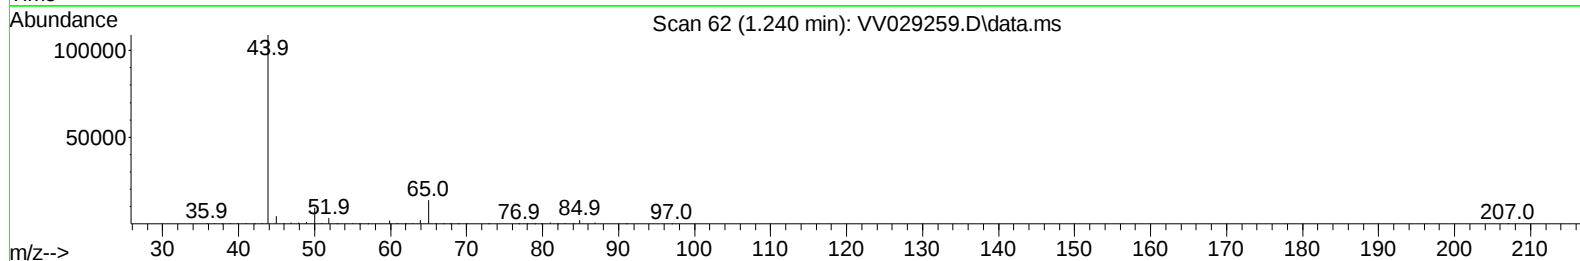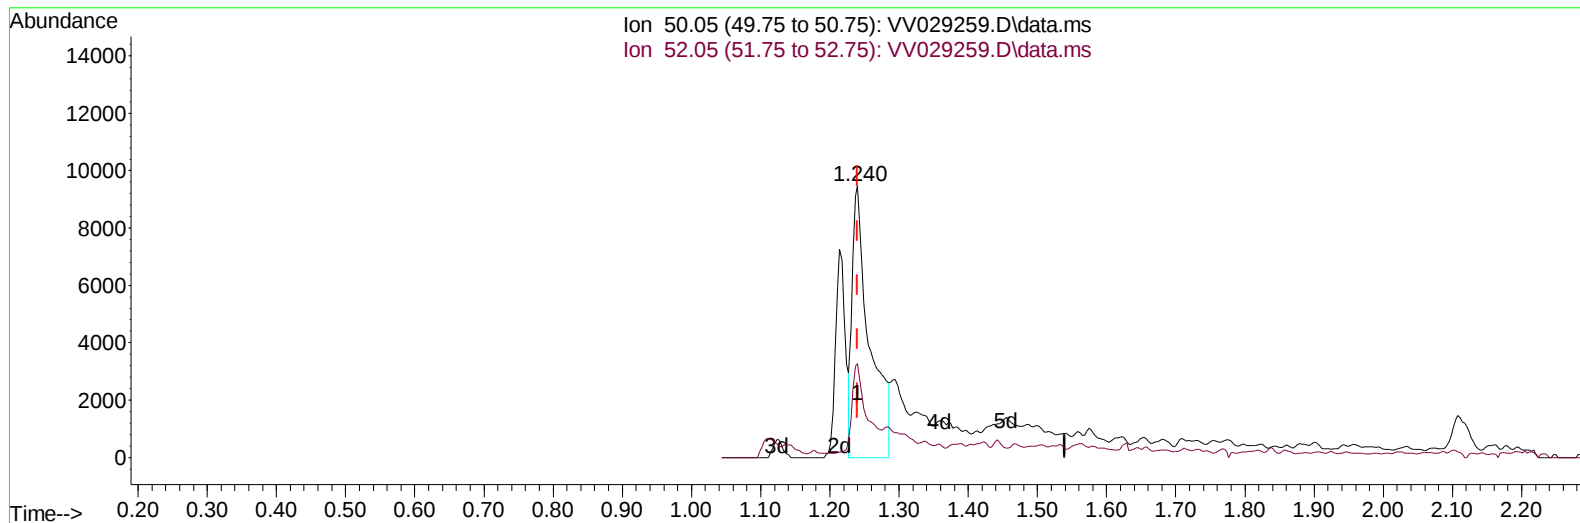

TIC: VV029259.D\data.ms

(3) Chloromethane (T)

1.240min (+ 0.000) 0.49 ug/L m

response 16623

Ion	Exp%	Act%
50.05	100.00	100.00
52.05	33.80	34.49
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029259.D
 Acq On : 21 Nov 2022 05:51
 Operator : SY/MD
 Sample : N5725-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB66

Manual IntegrationsAPPROVED

Quant Time: Nov 21 06:11:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 21 03:37:08 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/21/2022
 Supervised By :Mahesh Dadoda 11/21/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	487115	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	433485	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	218296	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	137929	4.645	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	92.800%	
7) Chloroethane-d5	1.565	69	115896	4.439	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	88.800%	
11) 1,1-Dichloroethene-d2	2.108	63	362613	6.700	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	134.000%#	
20) 2-Butanone-d5	3.880	46	318606	64.091	ug/L	-0.02
Spiked Amount 50.000	Range 40	- 130	Recovery	=	128.180%	
24) Chloroform-d	4.336	84	244200	4.005	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	80.200%	
26) 1,2-Dichloroethane-d4	5.024	65	111581	4.068	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	81.400%	
32) Benzene-d6	5.040	84	519229	4.013	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	80.200%	
36) 1,2-Dichloropropane-d6	6.063	67	161841	4.479	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	89.600%	
41) Toluene-d8	7.307	98	459470	3.945	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	78.800%	
43) trans-1,3-Dichloroprop...	7.613	79	57115	4.847	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	97.000%	
46) 2-Hexanone-d5	8.082	63	277298	55.130	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	110.260%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	114046	4.553	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	91.000%	
66) 1,2-Dichlorobenzene-d4	11.616	152	171619	4.394	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	87.800%	
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.127	85	4802	0.118	ug/L	96
3) Chloromethane	1.240	50	16623m	0.493	ug/L	
12) 1,1-Dichloroethene	2.114	96	403696	13.690	ug/L #	83
14) Carbon disulfide	2.291	76	53060	0.507	ug/L	100
18) trans-1,2-Dichloroethene	2.757	96	8225	0.240	ug/L	96
19) 1,1-Dichloroethane	3.179	63	1525847	27.291	ug/L	99
22) cis-1,2-Dichloroethene	3.899	96	5465127	157.181	ug/L	97
25) Chloroform	4.365	83	20274	0.346	ug/L	99
27) 1,2-Dichloroethane	5.124	62	53040	1.757	ug/L	98
29) 1,1,1-Trichloroethane	4.597	97	1693058	33.284	ug/L	98
34) Trichloroethene	5.905	95	1142367	33.686	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029259.D
Acq On : 21 Nov 2022 05:51
Operator : SY/MD
Sample : N5725-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB66

Manual IntegrationsAPPROVED

Quant Time: Nov 21 06:11:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 21 03:37:08 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 11/21/2022
Supervised By :Mahesh Dadoda 11/21/2022

