

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029215.D
 Acq On : 20 Nov 2022 11:02
 Operator : SY/MD
 Sample : VV1120WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK272

Quant Time: Nov 21 00:55:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 21 00:54:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	399700	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	361272	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	166097	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	133662	5.485	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.800%
7) Chloroethane-d5	1.564	69	107038	4.997	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.000%
11) 1,1-Dichloroethene-d2	2.101	63	168505	3.795	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.800%
20) 2-Butanone-d5	3.896	46	172592	42.312	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.620%
24) Chloroform-d	4.336	84	233738	4.672	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%
26) 1,2-Dichloroethane-d4	5.024	65	107258	4.765	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.400%
32) Benzene-d6	5.040	84	500990	4.646	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.000%
36) 1,2-Dichloropropane-d6	6.059	67	146515	4.866	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.400%
41) Toluene-d8	7.307	98	442792	4.562	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.200%
43) trans-1,3-Dichloroprop...	7.616	79	44793	4.561	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.200%
46) 2-Hexanone-d5	8.085	63	203468	48.537	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.080%
56) 1,1,2,2-Tetrachloroeth...	10.207	84	102762	4.922	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.400%
66) 1,2-Dichlorobenzene-d4	11.616	152	149107	5.018	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.400%
Target Compounds						Qvalue
16) Methylene chloride	2.500	84	8305	0.265	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029215.D
Acq On : 20 Nov 2022 11:02
Operator : SY/MD
Sample : VV1120WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272


Quant Time: Nov 21 00:55:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 21 00:54:18 2022
Response via : Initial Calibration

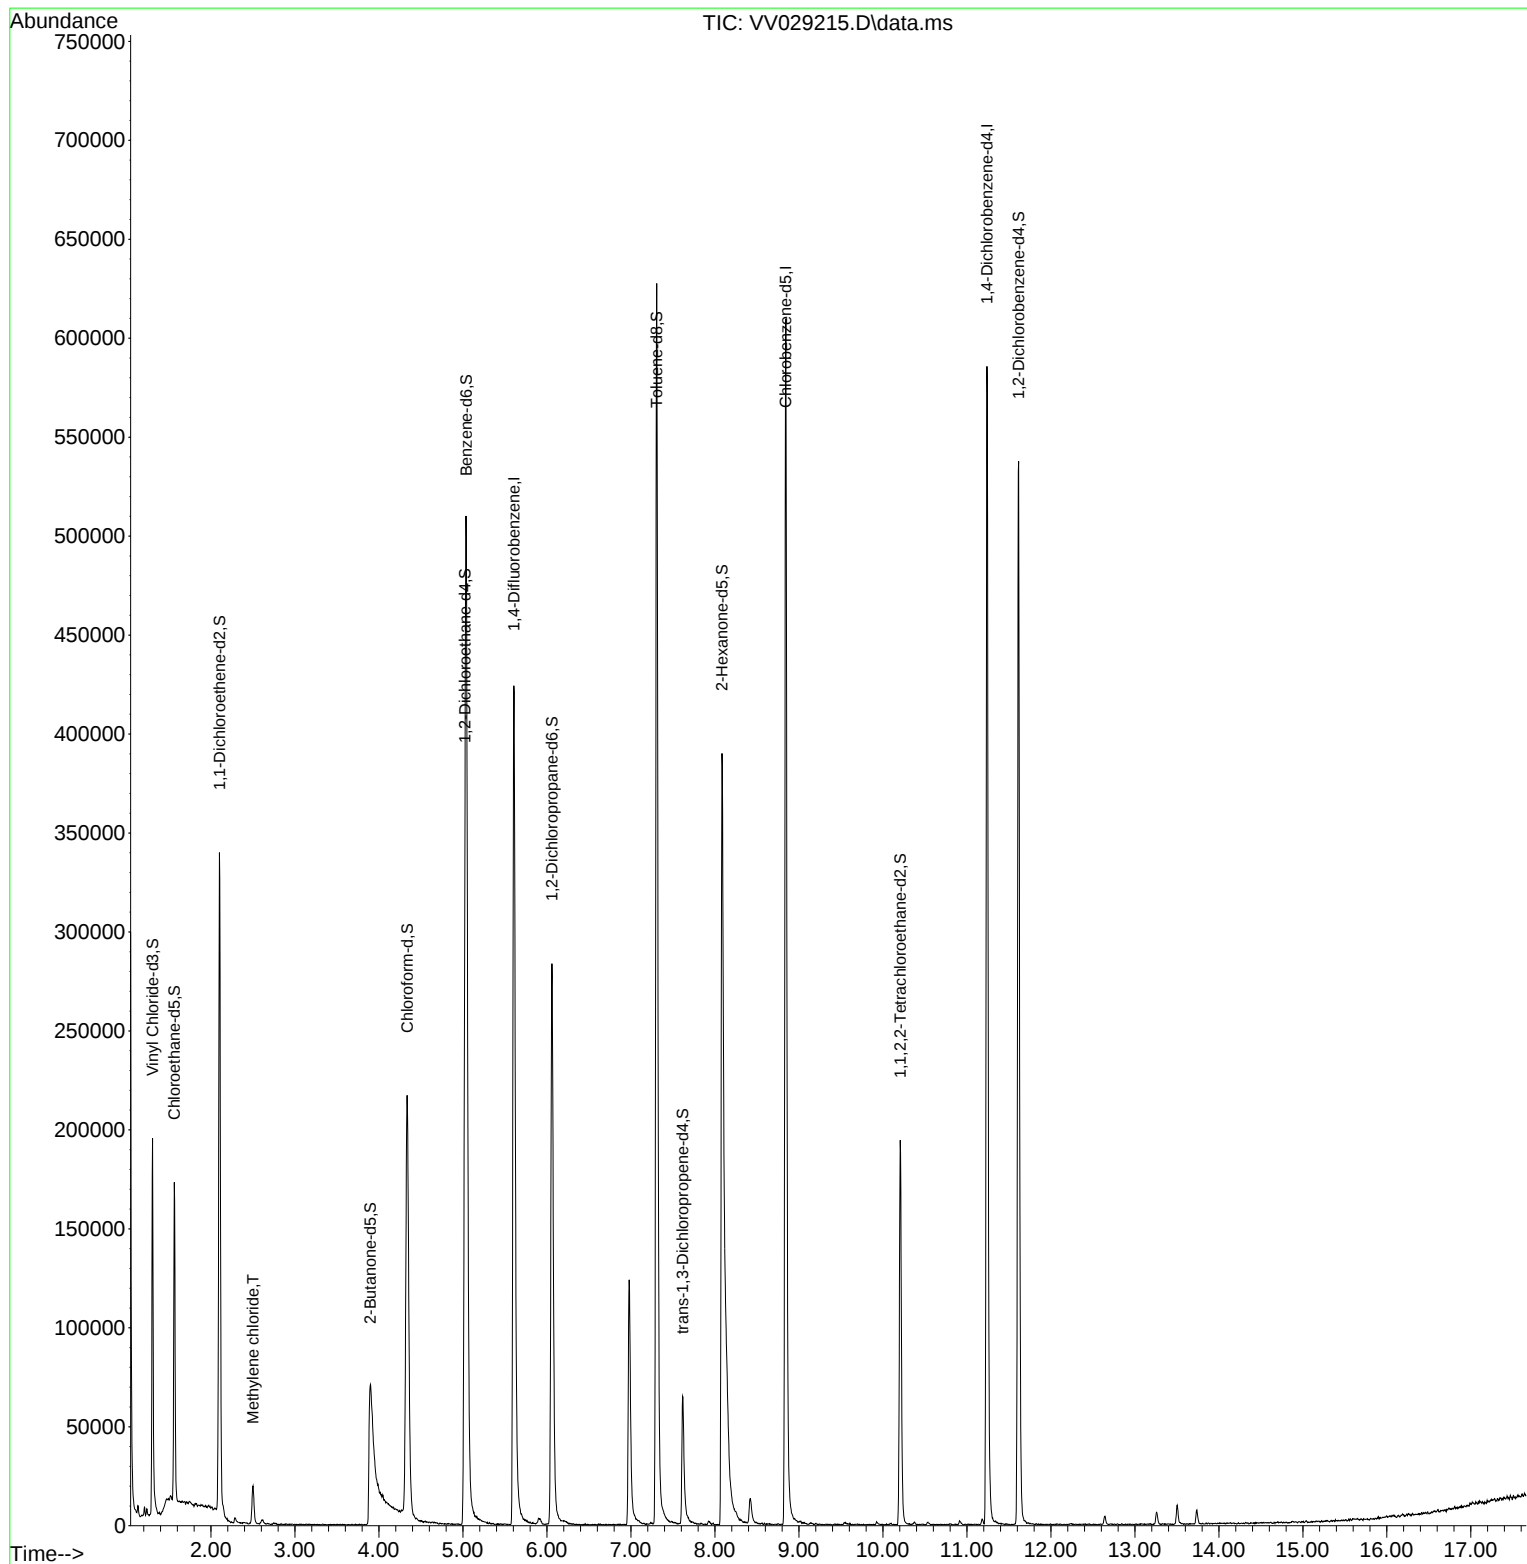

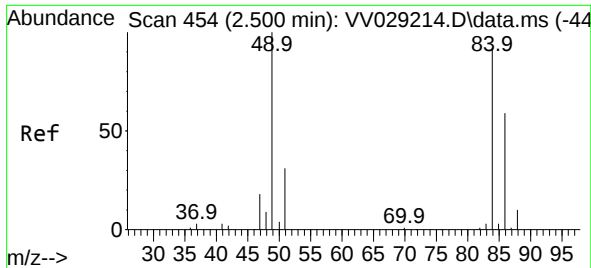

#16
Methylene chloride
Concen: 0.265 ug/L
RT: 2.500 min Scan# 4
Delta R.T. -0.000 min
Lab File: VV029215.D
Acq: 20 Nov 2022 11:02

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

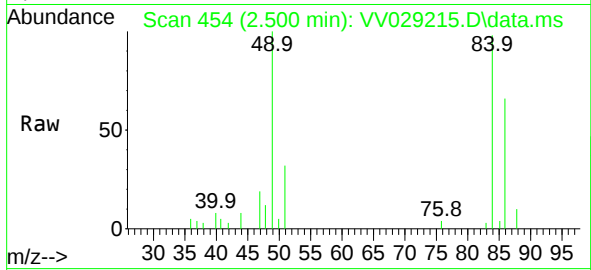

Tgt Ion: 84 Resp: 8305
Ion Ratio Lower Upper
84 100
86 67.2 45.8 85.0
49 101.7 75.5 140.1

