

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112022\
 Data File : VW029222.D
 Acq On : 20 Nov 2022 14:00
 Operator : SY/MD
 Sample : N5651-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1M7

Quant Time: Nov 21 00:57:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 21 00:54:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	291843	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	273987	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	119306	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	99373	5.585	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	111.800%	
7) Chloroethane-d5	1.568	69	82498	5.274	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	105.400%	
11) 1,1-Dichloroethene-d2	2.105	63	126613	3.905	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	78.000%	
20) 2-Butanone-d5	3.889	46	206066	69.188	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	138.380%#	
24) Chloroform-d	4.342	84	186439	5.104	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.000%	
26) 1,2-Dichloroethane-d4	5.027	65	85742	5.217	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	104.400%	
32) Benzene-d6	5.043	84	387405	4.737	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.800%	
36) 1,2-Dichloropropane-d6	6.066	67	116049	5.082	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	101.600%	
41) Toluene-d8	7.310	98	341447	4.638	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.800%	
43) trans-1,3-Dichloroprop...	7.622	79	35347	4.746	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	95.000%	
46) 2-Hexanone-d5	8.088	63	160534	50.495	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	101.000%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	82618	5.218	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	104.400%	
66) 1,2-Dichlorobenzene-d4	11.616	152	123165	5.770	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	115.400%	
Target Compounds						
3) Chloromethane	1.240	50	7587	0.376	ug/L	97
13) Acetone	2.185	43	41750	21.792	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029222.D
Acq On : 20 Nov 2022 14:00
Operator : SY/MD
Sample : N5651-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1M7

Quant Time: Nov 21 00:57:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 21 00:54:18 2022
Response via : Initial Calibration




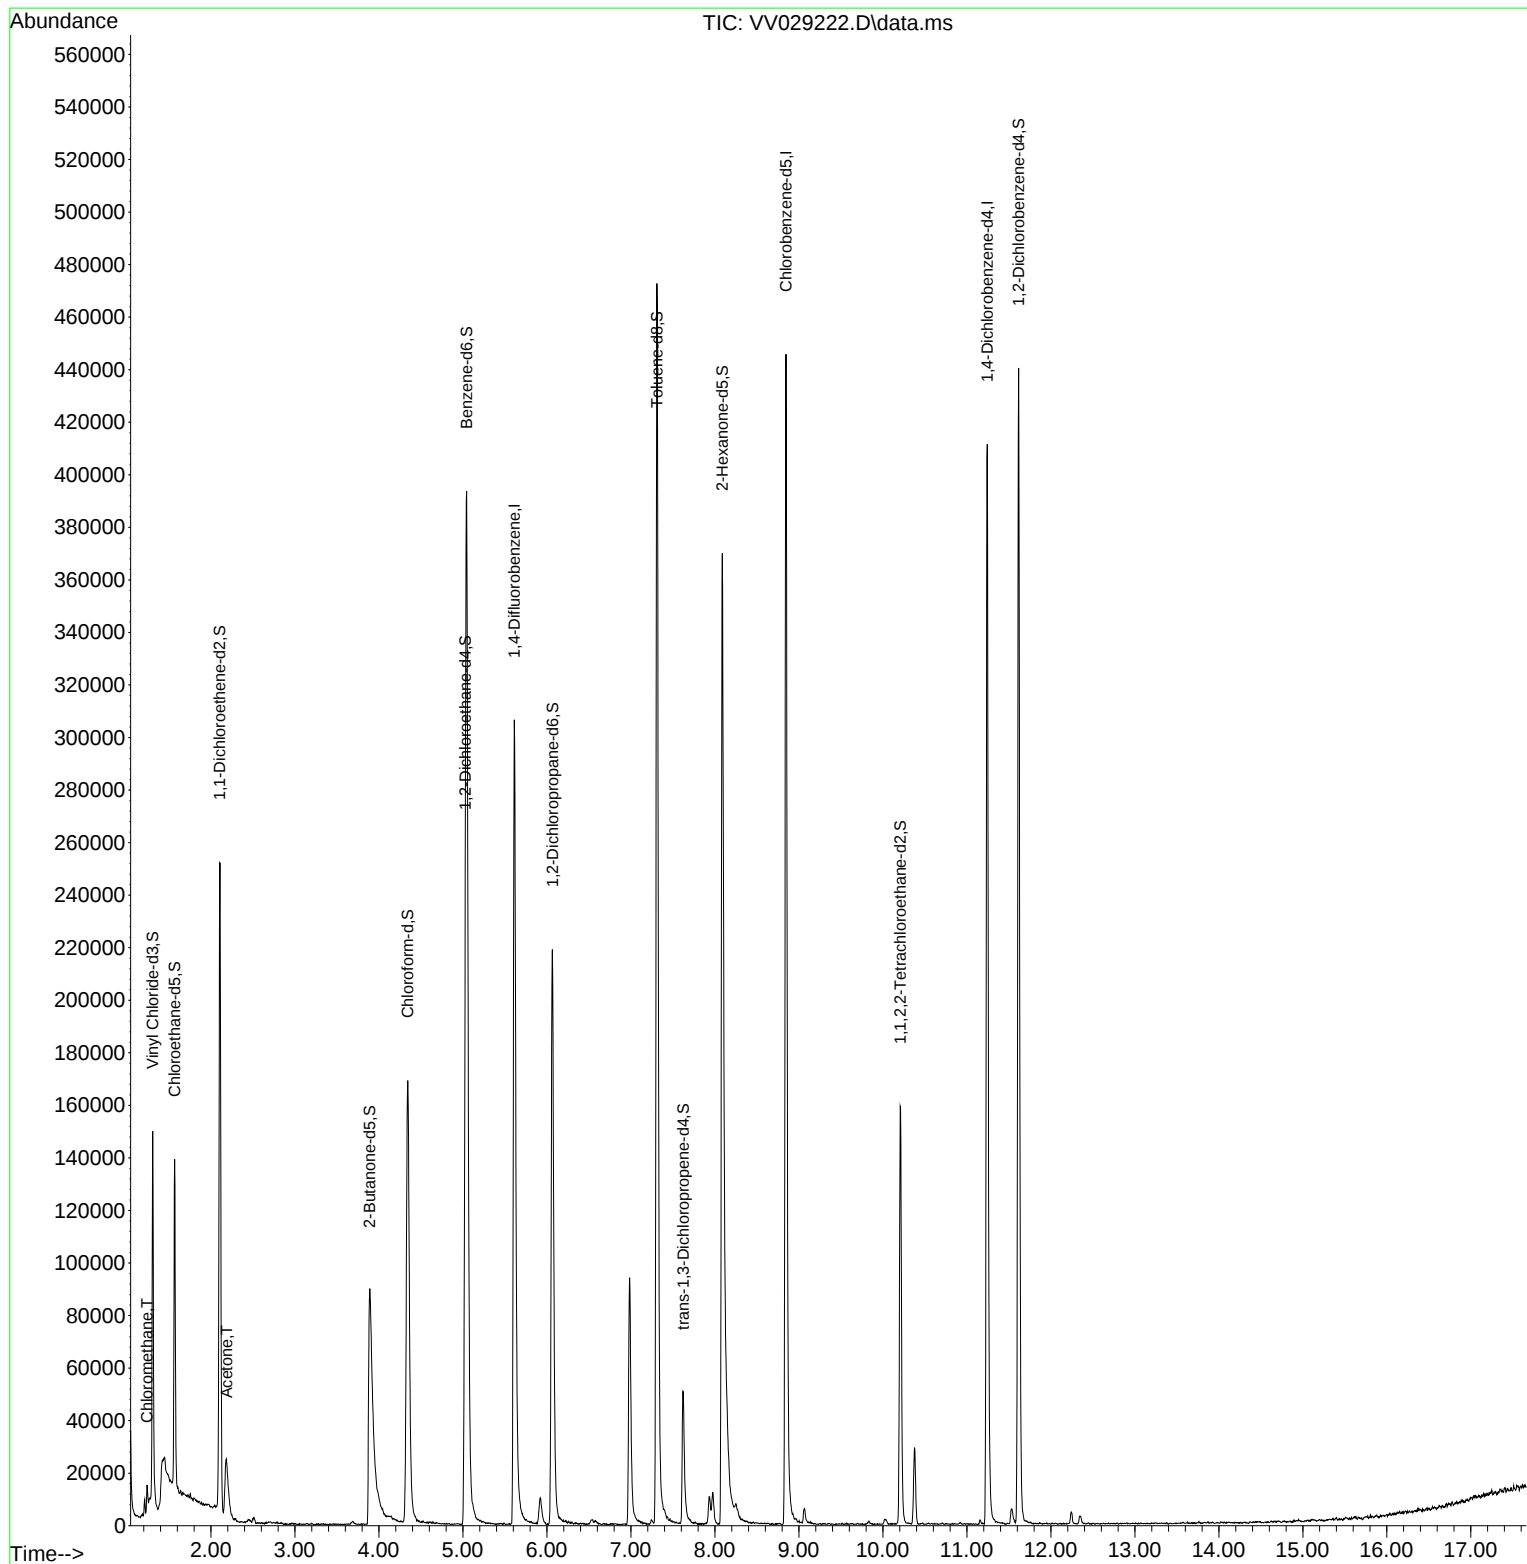


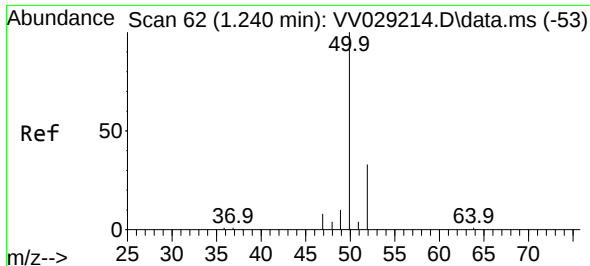

#3
Chloromethane
Concen: 0.376 ug/L
RT: 1.240 min Scan# 61
Delta R.T. -0.000 min
Lab File: VV029222.D
Acq: 20 Nov 2022 14:00

Instrument :
MSVOA_V
ClientSampleId :
BH1M7

Tgt Ion: 50 Resp: 7587
Ion Ratio Lower Upper
50 100
52 35.4 23.7 43.9

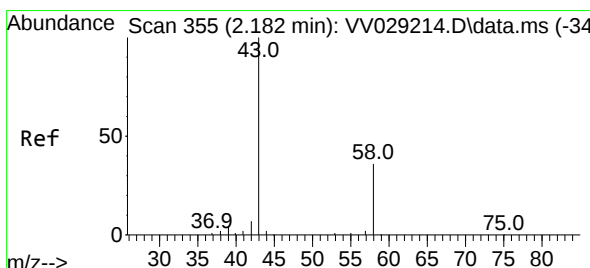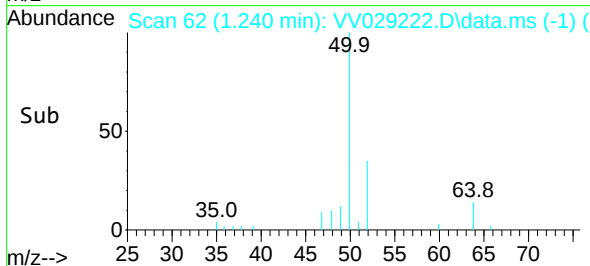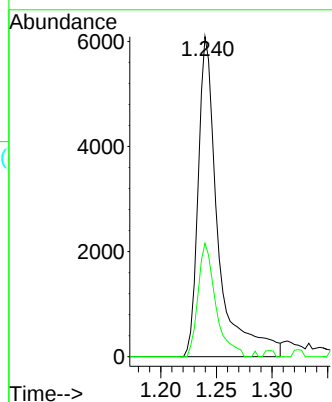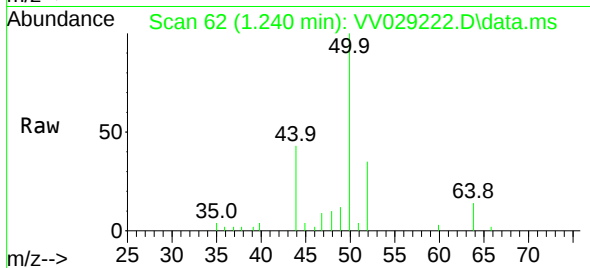

#13
Acetone
Concen: 21.792 ug/L
RT: 2.185 min Scan# 356
Delta R.T. 0.003 min
Lab File: VV029222.D
Acq: 20 Nov 2022 14:00

Tgt Ion: 43 Resp: 41750
Ion Ratio Lower Upper
43 100
58 37.5 0.0 56.6

