

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112022\
 Data File : VW029223.D
 Acq On : 20 Nov 2022 14:24
 Operator : SY/MD
 Sample : N5651-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 21 00:57:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 21 00:54:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	308793	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	283436	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	129918	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	93946	4.990	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.800%
7) Chloroethane-d5	1.568	69	79177	4.784	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.600%
11) 1,1-Dichloroethene-d2	2.105	63	121069	3.529	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.600%
20) 2-Butanone-d5	3.902	46	120541	38.251	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	76.500%
24) Chloroform-d	4.342	84	178268	4.612	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.200%
26) 1,2-Dichloroethane-d4	5.027	65	83313	4.791	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.800%
32) Benzene-d6	5.043	84	369557	4.368	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.400%
36) 1,2-Dichloropropane-d6	6.066	67	112003	4.741	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.800%
41) Toluene-d8	7.310	98	320214	4.205	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.000%
43) trans-1,3-Dichloroprop...	7.622	79	32669	4.240	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.800%
46) 2-Hexanone-d5	8.088	63	151191	45.971	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.940%
56) 1,1,2,2-Tetrachloroeth...	10.210	84	77469	4.730	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.600%
66) 1,2-Dichlorobenzene-d4	11.615	152	115581	4.973	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.400%
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	5747	0.238	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029223.D
Acq On : 20 Nov 2022 14:24
Operator : SY/MD
Sample : N5651-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Nov 21 00:57:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 21 00:54:18 2022
Response via : Initial Calibration

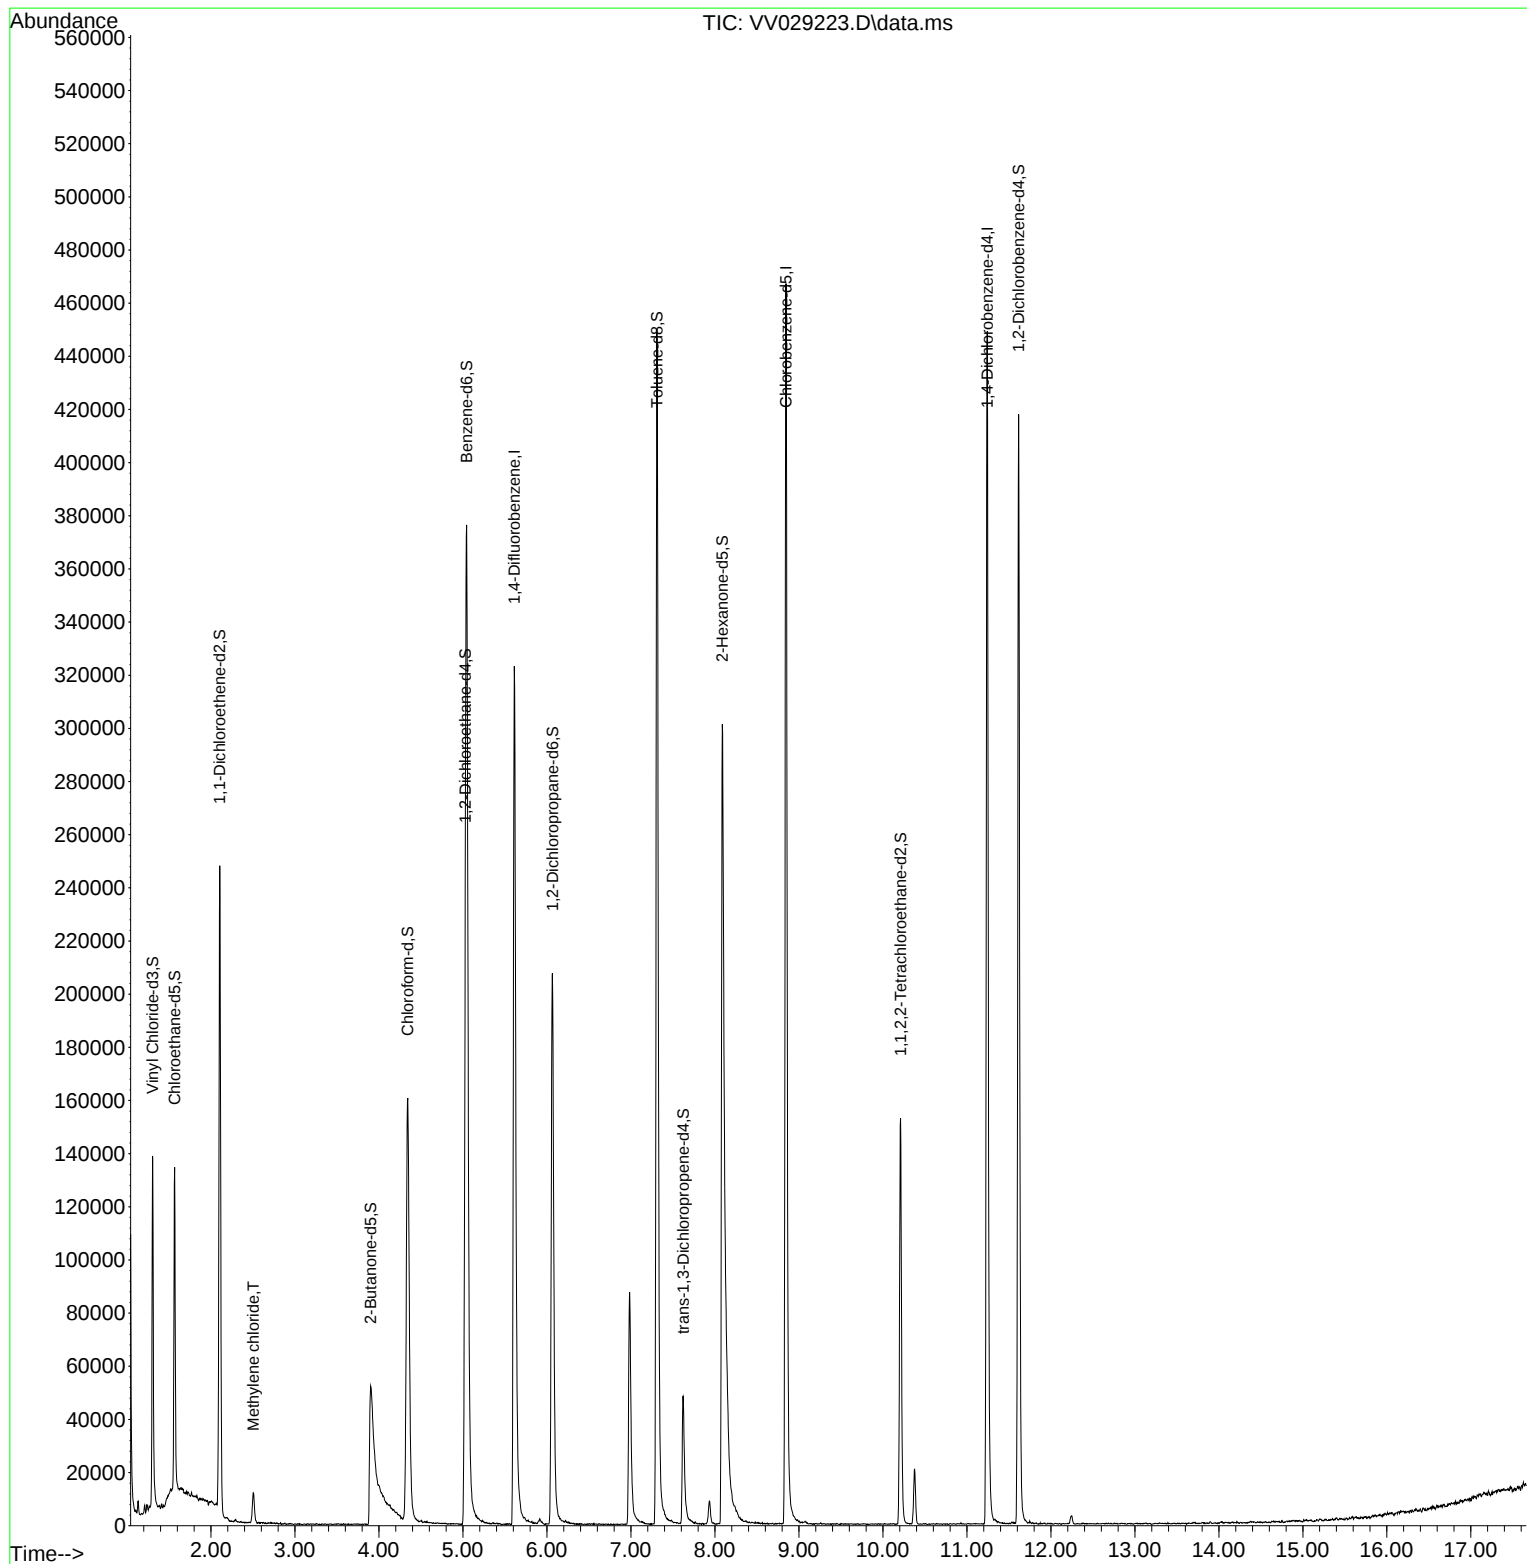

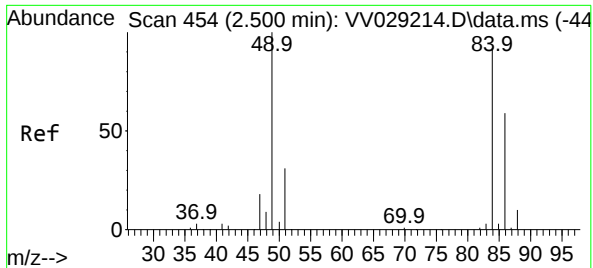

#16
Methylene chloride
Concen: 0.238 ug/L
RT: 2.503 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV029223.D
Acq: 20 Nov 2022 14:24

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 5747
Ion Ratio Lower Upper
84 100
86 50.7 45.8 85.0
49 91.9 75.5 140.1

