

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112022\
 Data File : VW029237.D
 Acq On : 20 Nov 2022 20:06
 Operator : SY/MD
 Sample : N5652-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1M3

Quant Time: Nov 21 01:00:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 21 00:54:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	308638	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	285759	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	129843	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	88430	4.700	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.000%
7) Chloroethane-d5	1.567	69	74525	4.505	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.200%
11) 1,1-Dichloroethene-d2	2.108	63	116089	3.386	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.800%
20) 2-Butanone-d5	3.895	46	192846	61.226	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	122.460%
24) Chloroform-d	4.342	84	175115	4.533	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.600%
26) 1,2-Dichloroethane-d4	5.030	65	80796	4.648	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.000%
32) Benzene-d6	5.046	84	353974	4.150	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.000%
36) 1,2-Dichloropropane-d6	6.066	67	107863	4.529	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.600%
41) Toluene-d8	7.310	98	308506	4.018	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.400%
43) trans-1,3-Dichloroprop...	7.622	79	33270	4.283	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.600%
46) 2-Hexanone-d5	8.088	63	153778	46.377	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.760%
56) 1,1,2,2-Tetrachloroeth...	10.210	84	77742	4.708	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.200%
66) 1,2-Dichlorobenzene-d4	11.615	152	112605	4.847	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.000%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.130	85	2662	0.103	ug/L #	86
3) Chloromethane	1.240	50	3368	0.158	ug/L	98
9) Trichlorofluoromethane	1.754	101	3977	0.121	ug/L	94
12) 1,1-Dichloroethene	2.114	96	3668	0.196	ug/L #	1
17) Methyl tert-butyl Ether	2.764	73	4402	0.110	ug/L #	95
18) trans-1,2-Dichloroethene	2.760	96	60532	2.793	ug/L	98
19) 1,1-Dichloroethane	3.198	63	2916	0.082	ug/L	92
22) cis-1,2-Dichloroethene	3.905	96	164700	7.476	ug/L	98
25) Chloroform	4.371	83	26057	0.702	ug/L	91
29) 1,1,1-Trichloroethane	4.606	97	1604	0.048	ug/L	96
33) Benzene	5.104	78	6778	0.078	ug/L	100
34) Trichloroethene	5.908	95	1368332	61.208	ug/L	98
38) Bromodichloromethane	6.509	83	3070	0.120	ug/L #	98
47) Tetrachloroethene	7.969	164	62573	3.496	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029237.D
Acq On : 20 Nov 2022 20:06
Operator : SY/MD
Sample : N5652-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1M3

Quant Time: Nov 21 01:00:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 21 00:54:18 2022
Response via : Initial Calibration




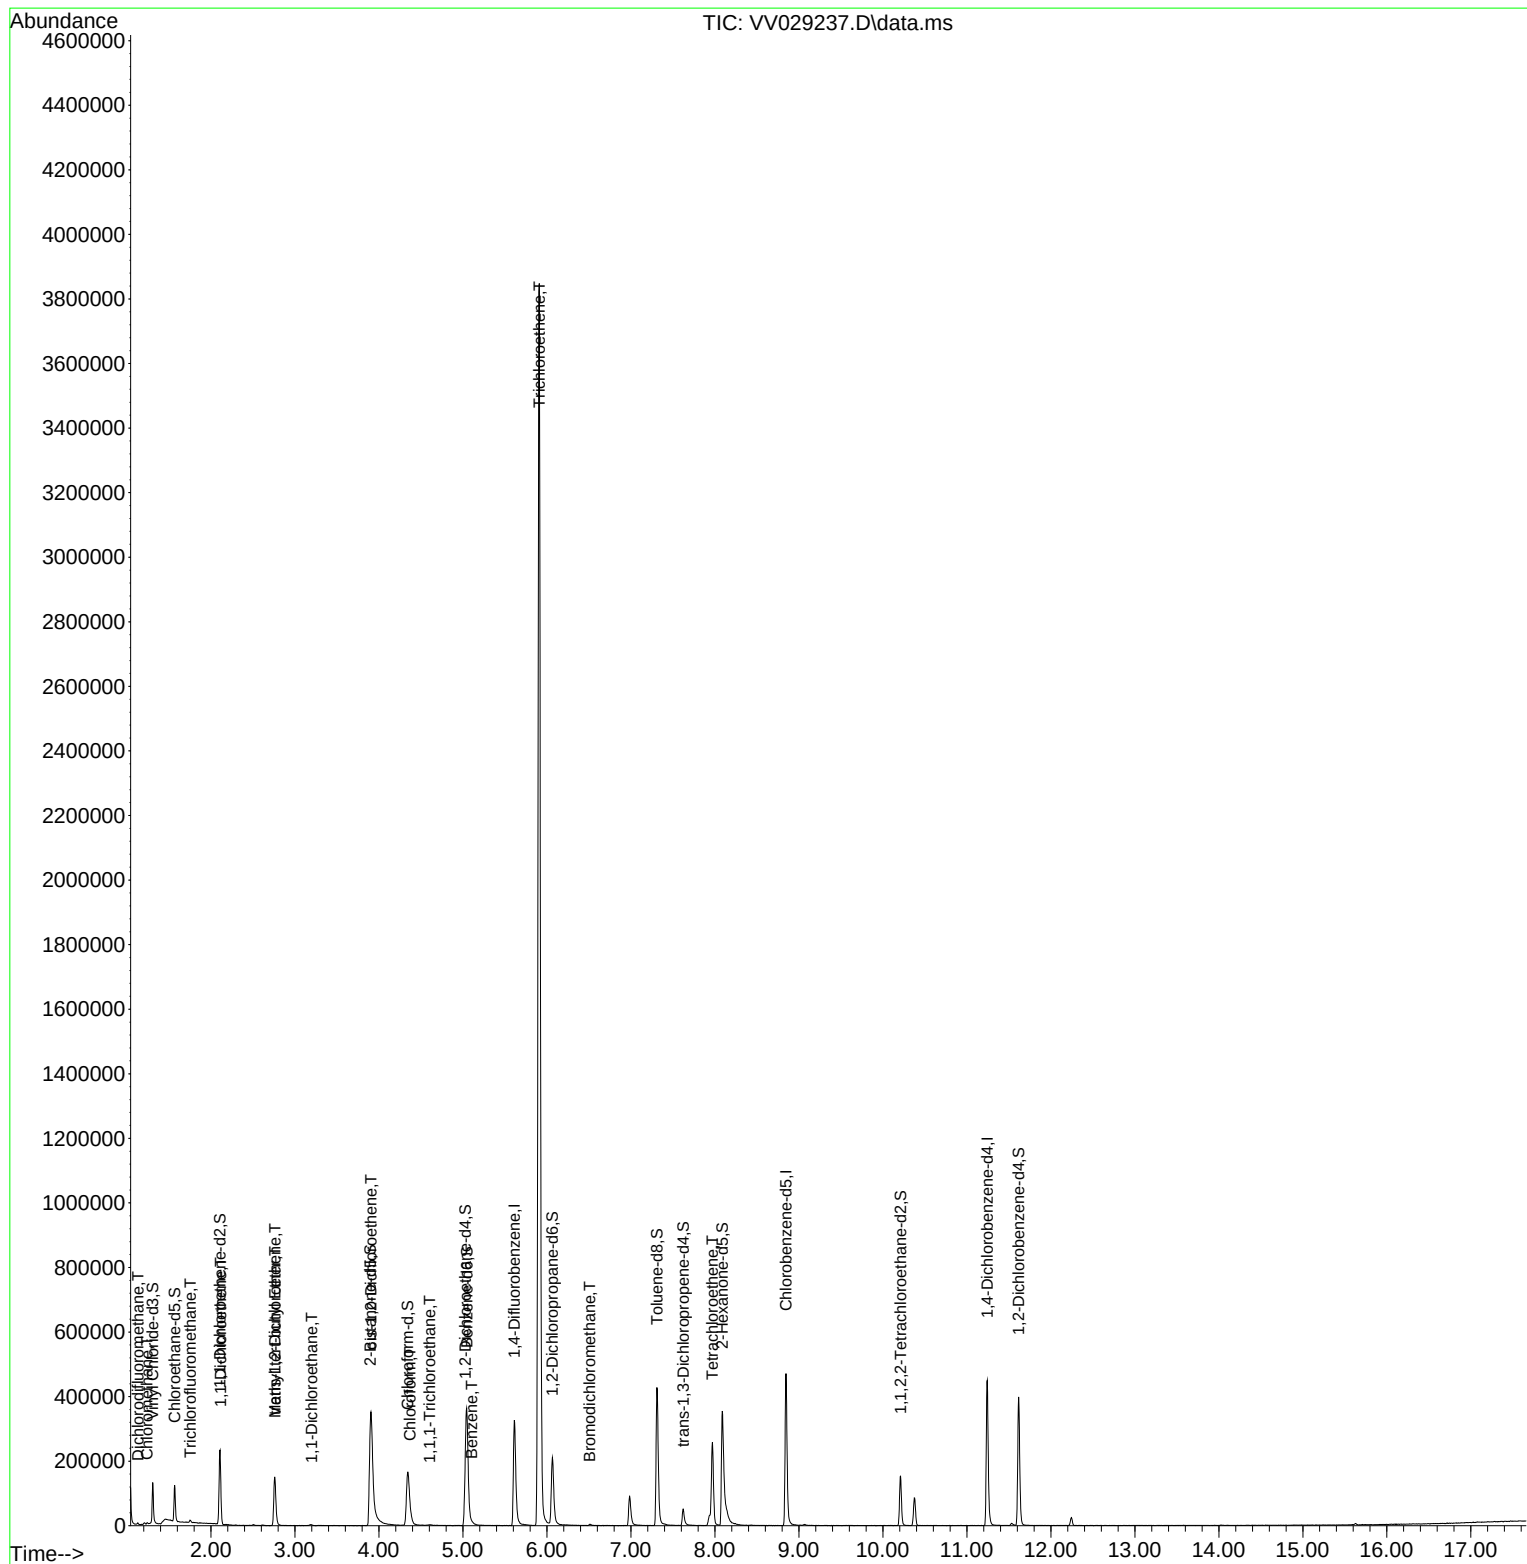


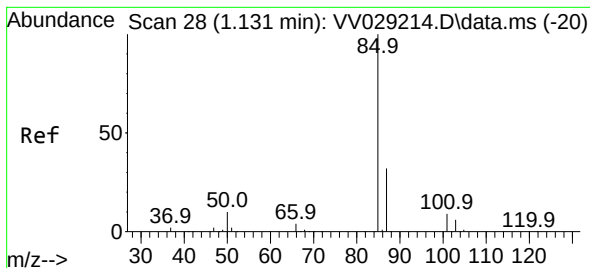

#2
 Dichlorodifluoromethane
 Concen: 0.103 ug/L
 RT: 1.130 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VV029237.D
 Acq: 20 Nov 2022 20:06




Instrument :
 MSVOA_V
 ClientSampleId :
 BH1M3


Tgt Ion: 85 Resp: 2662
 Ion Ratio Lower Upper
 85 100
 87 23.5 25.0 37.4#

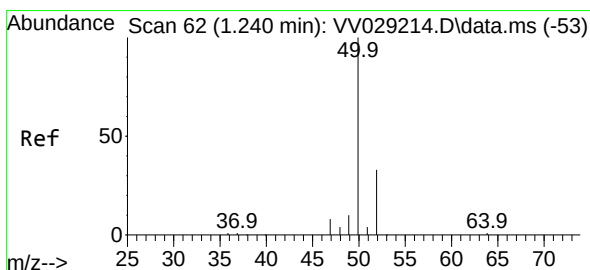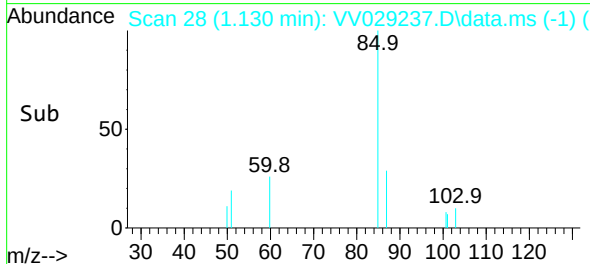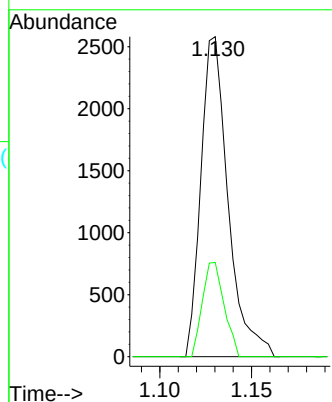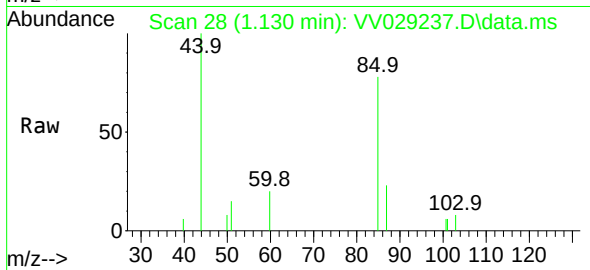

#3
 Chloromethane
 Concen: 0.158 ug/L
 RT: 1.240 min Scan# 62
 Delta R.T. -0.000 min
 Lab File: VV029237.D
 Acq: 20 Nov 2022 20:06

Tgt Ion: 50 Resp: 3368
 Ion Ratio Lower Upper
 50 100
 52 32.9 23.7 43.9


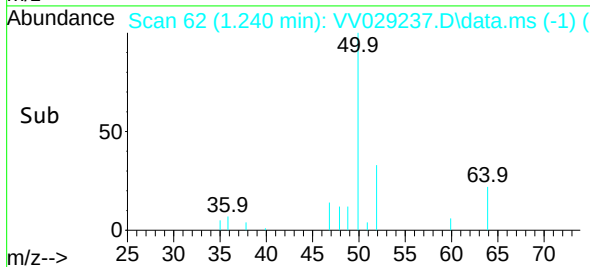
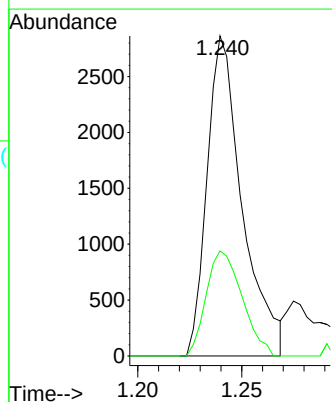
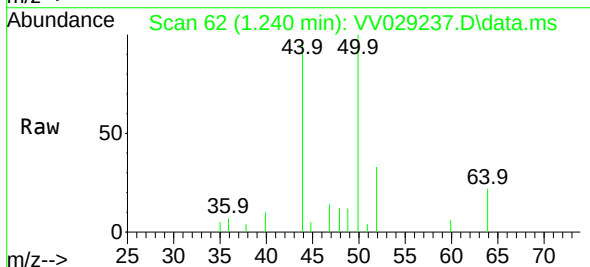


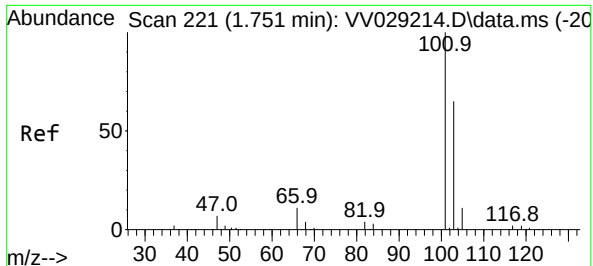

#9
 Trichlorofluoromethane
 Concen: 0.121 ug/L
 RT: 1.754 min Scan# 21
 Delta R.T. 0.003 min
 Lab File: VV029237.D
 Acq: 20 Nov 2022 20:06




Instrument :
 MSVOA_V
 ClientSampleId :
 BH1M3


Tgt Ion:101 Resp: 3977
 Ion Ratio Lower Upper
 101 100
 103 69.0 51.3 76.9

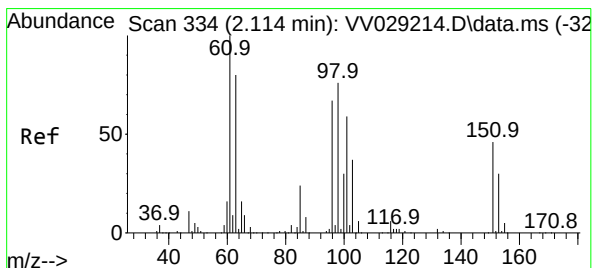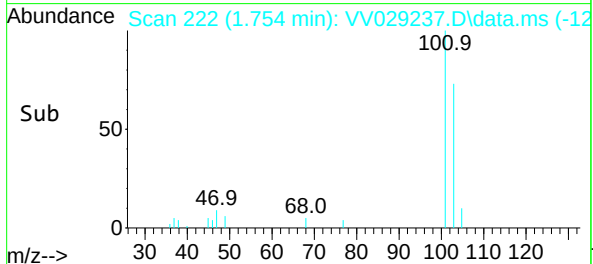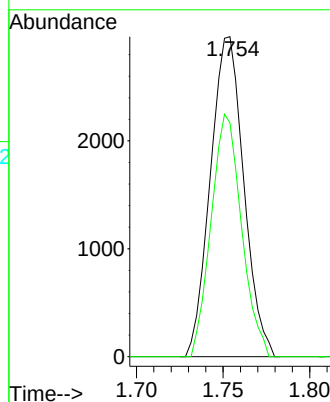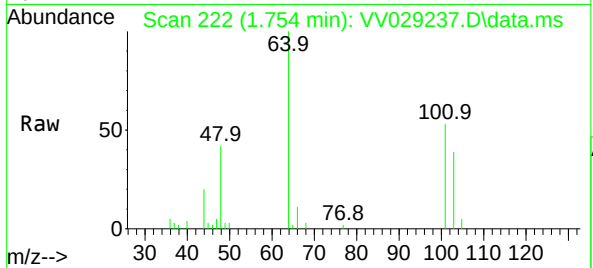

#12
 1,1-Dichloroethene
 Concen: 0.196 ug/L
 RT: 2.114 min Scan# 334
 Delta R.T. -0.000 min
 Lab File: VV029237.D
 Acq: 20 Nov 2022 20:06

Tgt Ion: 96 Resp: 3668
 Ion Ratio Lower Upper
 96 100
 61 398.4 104.2 193.4#
 63 2556.8 75.9 140.9#


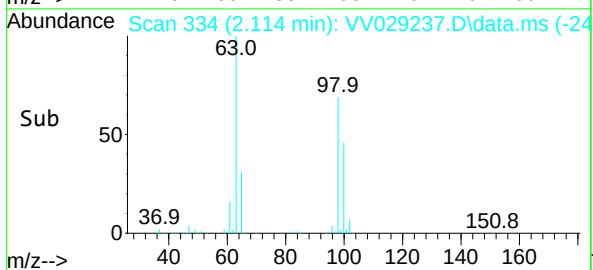
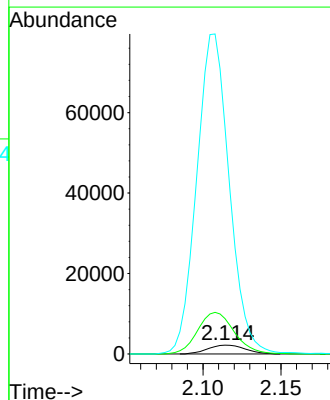
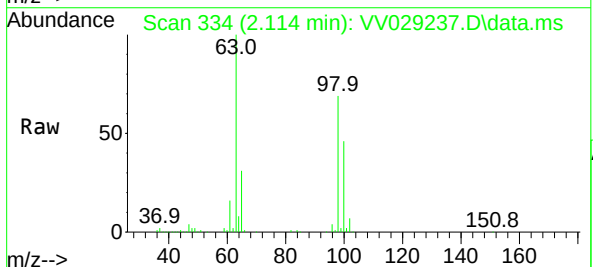


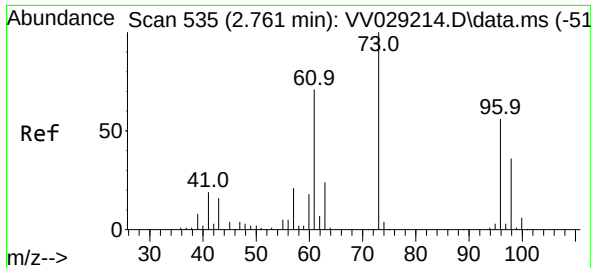

#17
Methyl tert-butyl Ether
Concen: 0.110 ug/L
RT: 2.764 min Scan# 51
Delta R.T. 0.003 min
Lab File: VV029237.D
Acq: 20 Nov 2022 20:06




Instrument :
MSVOA_V
ClientSampleId :
BH1M3


Tgt Ion: 73 Resp: 4402
Ion Ratio Lower Upper
73 100
43 11.9 13.0 19.4#
57 20.6 16.6 24.8

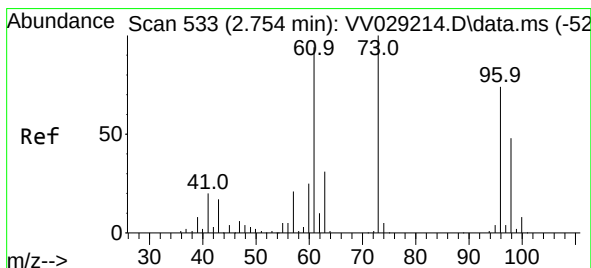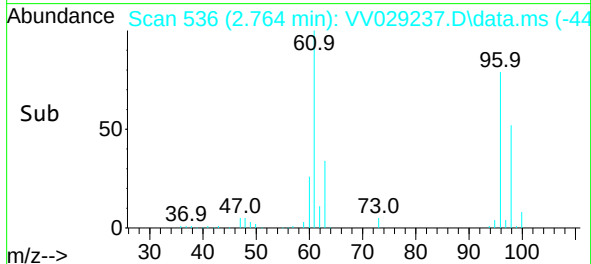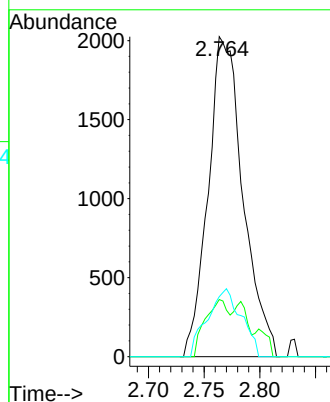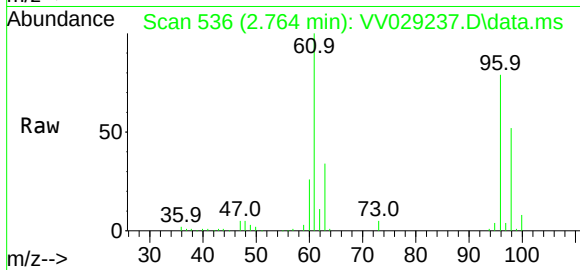

#18
trans-1,2-Dichloroethene
Concen: 2.793 ug/L
RT: 2.760 min Scan# 535
Delta R.T. 0.006 min
Lab File: VV029237.D
Acq: 20 Nov 2022 20:06

Tgt Ion: 96 Resp: 60532
Ion Ratio Lower Upper
96 100
61 129.5 91.8 170.6
98 68.3 46.4 86.2

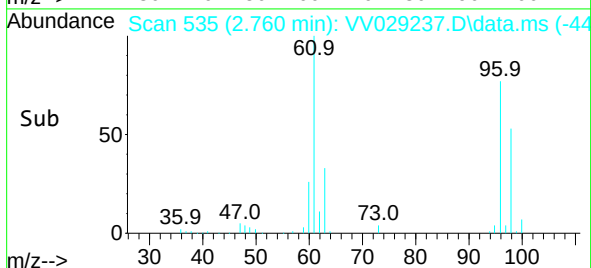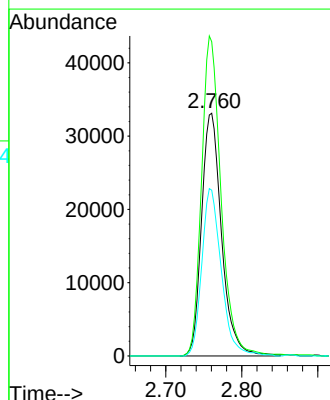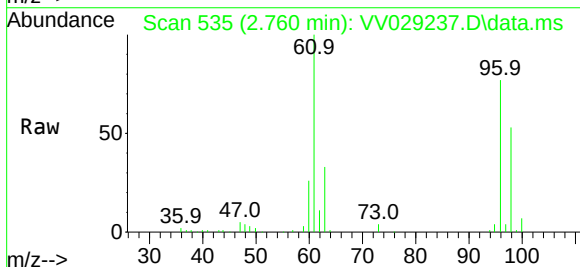

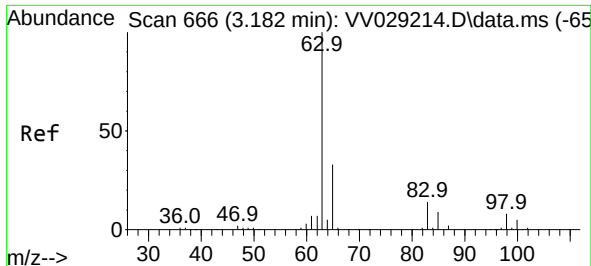

#19

1,1-Dichloroethane

Concen: 0.082 ug/L

RT: 3.198 min Scan# 6

Delta R.T. 0.016 min

Lab File: VV029237.D

Acq: 20 Nov 2022 20:06

Instrument :

MSVOA_V

ClientSampleId :

BH1M3





Tgt Ion: 63 Resp: 2916

Ion Ratio Lower Upper

63 100

65 38.5 23.0 42.6

83 15.1 9.4 17.6

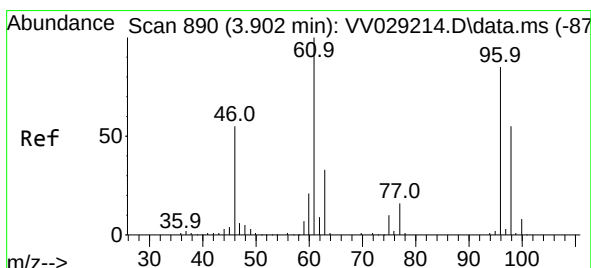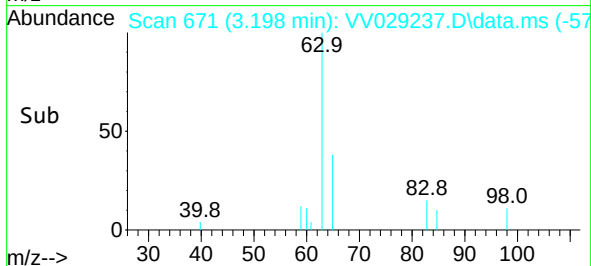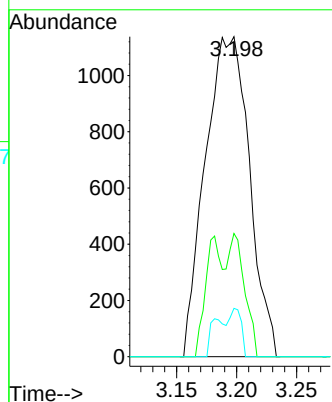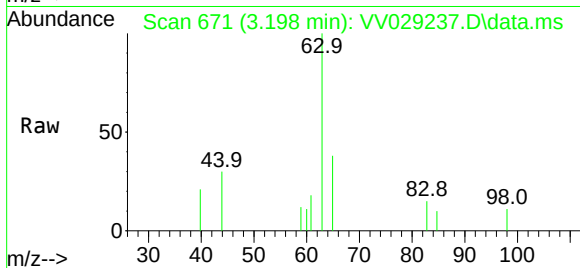

#22

cis-1,2-Dichloroethene

Concen: 7.476 ug/L

RT: 3.905 min Scan# 891

Delta R.T. 0.003 min

Lab File: VV029237.D

Acq: 20 Nov 2022 20:06




Tgt Ion: 96 Resp: 164700


Ion Ratio Lower Upper

96 100

61 114.9 82.3 152.9

68 0.0 0.0 0.0

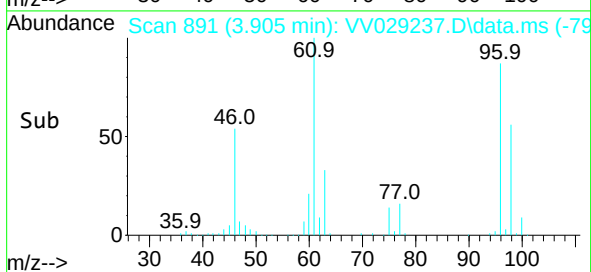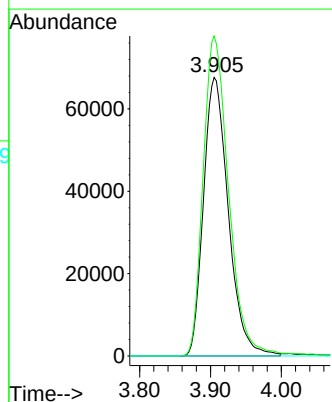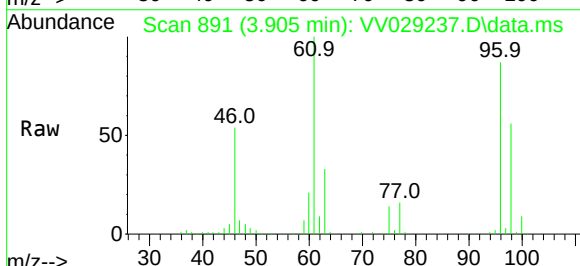

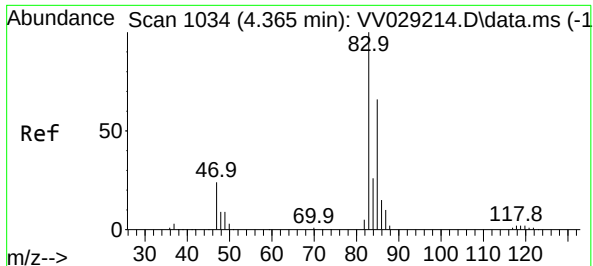

#25

Chloroform

Concen: 0.702 ug/L

RT: 4.371 min Scan# 1109

Delta R.T. 0.006 min

Lab File: VV029237.D

Acq: 20 Nov 2022 20:06

Instrument :

MSVOA_V

ClientSampleId :





BH1M3

Tgt Ion: 83 Resp: 26057

Ion Ratio Lower Upper

83 100

85 69.1 43.7 81.1

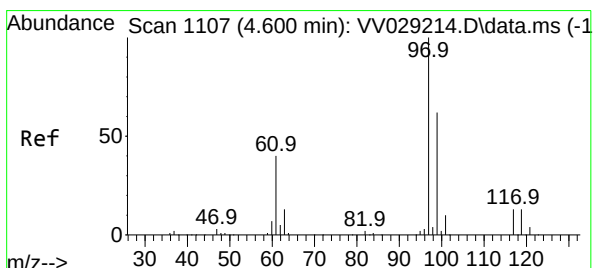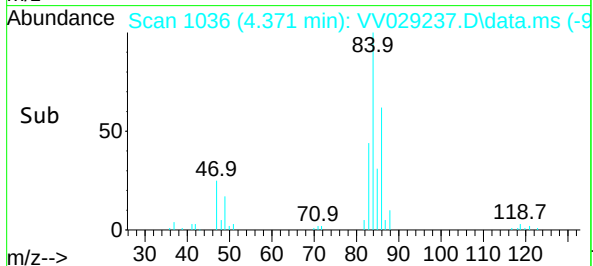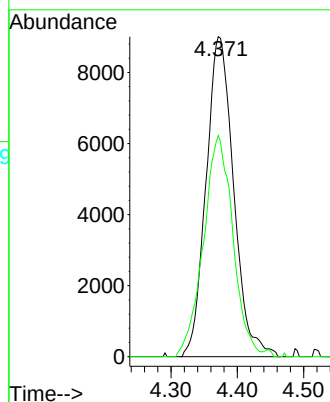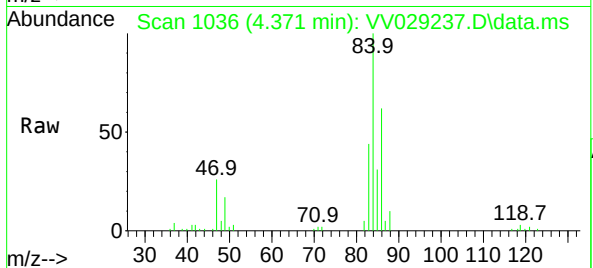

#29

1,1,1-Trichloroethane

Concen: 0.048 ug/L

RT: 4.606 min Scan# 1109

Delta R.T. 0.006 min

Lab File: VV029237.D

Acq: 20 Nov 2022 20:06




Tgt Ion: 97 Resp: 1604


Ion Ratio Lower Upper

97 100

99 64.2 52.7 79.1

61 37.0 33.8 50.6


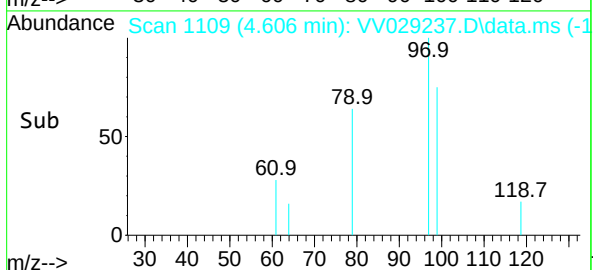
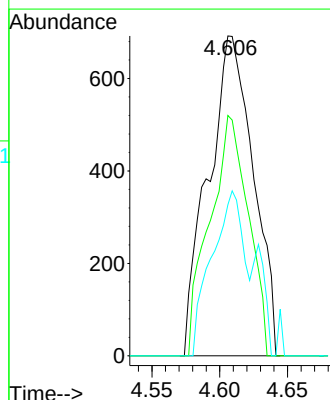
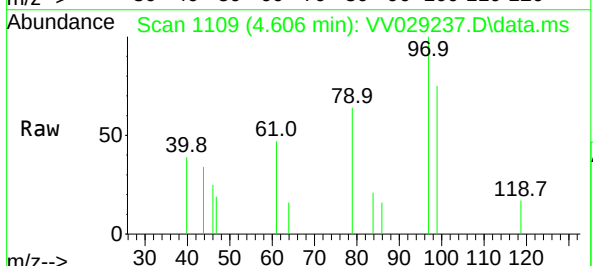


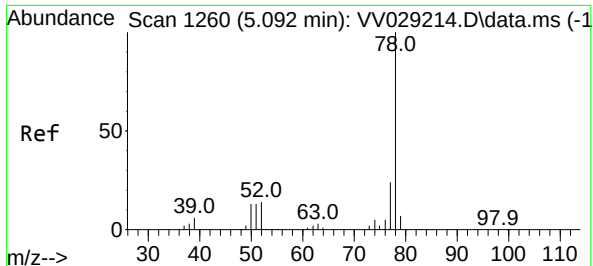

#33
Benzene
Concen: 0.078 ug/L
RT: 5.104 min Scan# 11
Delta R.T. 0.013 min
Lab File: VV029237.D
Acq: 20 Nov 2022 20:06

Instrument :
MSVOA_V
ClientSampleId :
BH1M3




Tgt Ion: 78 Resp: 6778

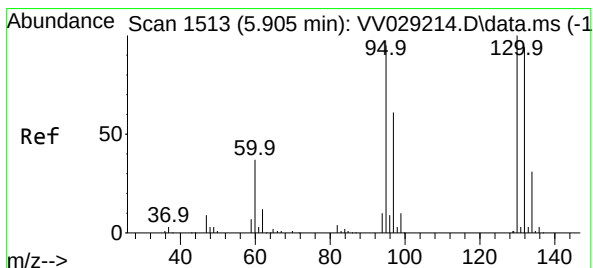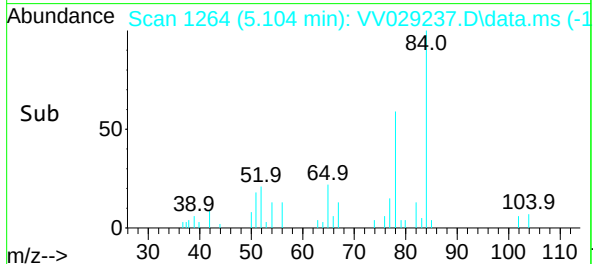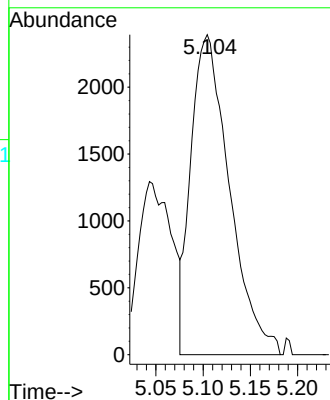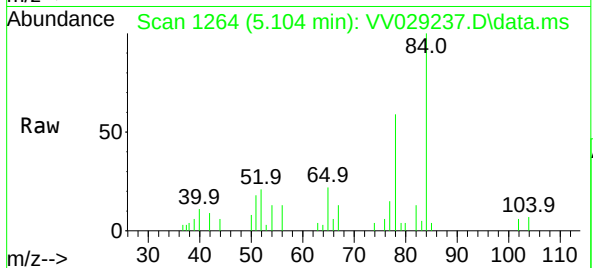


#34
Trichloroethene
Concen: 61.208 ug/L
RT: 5.908 min Scan# 1514
Delta R.T. 0.003 min
Lab File: VV029237.D
Acq: 20 Nov 2022 20:06

Tgt Ion: 95 Resp: 1368332

Ion	Ratio	Lower	Upper
95	100		
97	64.4	45.6	84.8
132	101.5	69.1	128.3
130	105.1	74.9	139.1


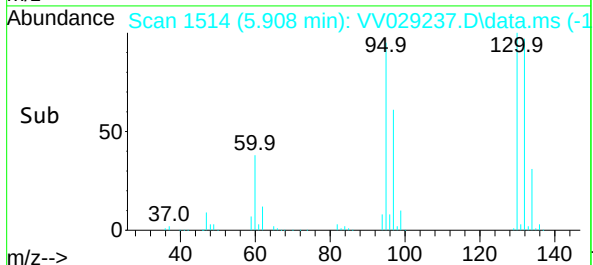
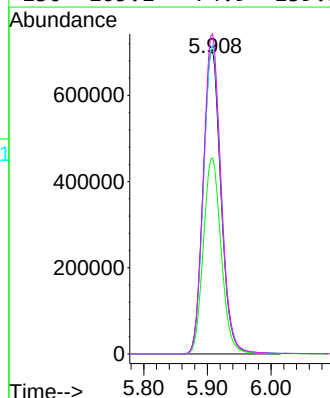
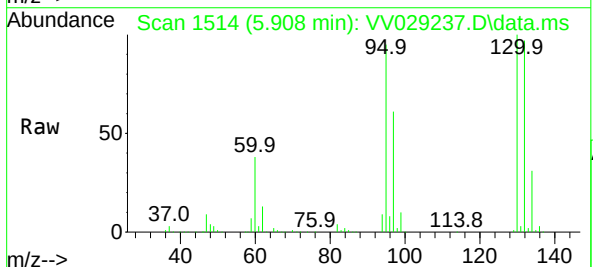


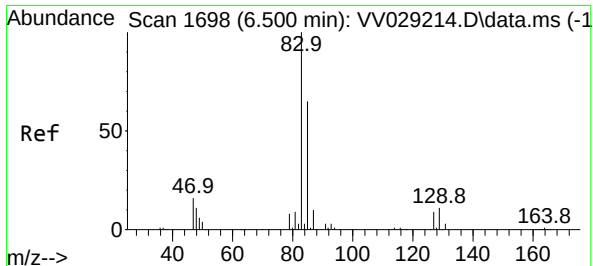

#38
Bromodichloromethane
Concen: 0.120 ug/L
RT: 6.509 min Scan# 11
Delta R.T. 0.009 min
Lab File: VV029237.D
Acq: 20 Nov 2022 20:06

Instrument :
MSVOA_V
ClientSampleId :
BH1M3

Tgt Ion: 83 Resp: 3070
Ion Ratio Lower Upper
83 100
85 64.6 46.1 85.5
127 12.1 6.7 10.1#

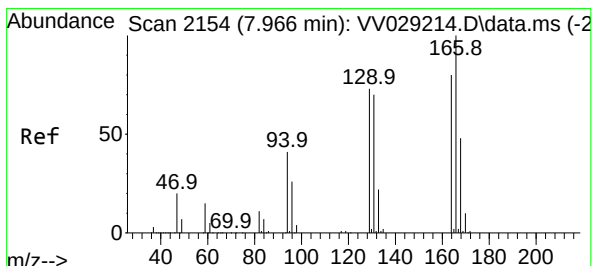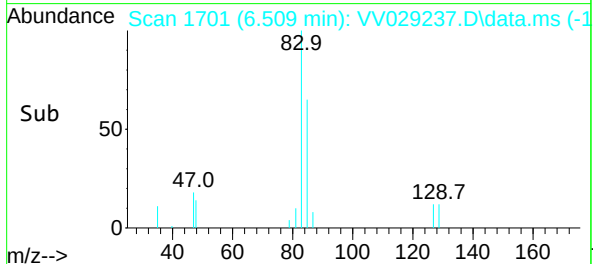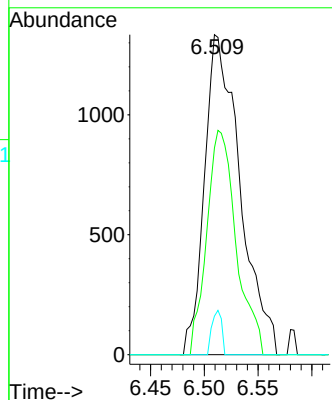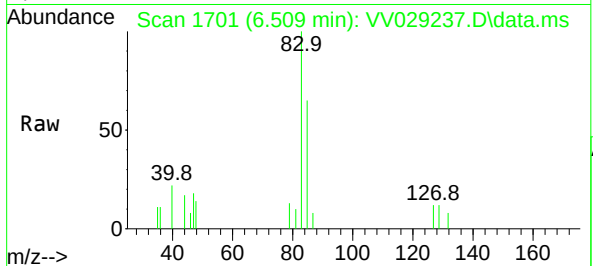

#47
Tetrachloroethene
Concen: 3.496 ug/L
RT: 7.969 min Scan# 2155
Delta R.T. 0.003 min
Lab File: VV029237.D
Acq: 20 Nov 2022 20:06

Tgt Ion: 164 Resp: 62573
Ion Ratio Lower Upper
164 100
129 94.0 63.9 118.7
131 91.2 61.8 114.8
166 132.9 90.2 167.4

