

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029215.D
 Acq On : 20 Nov 2022 11:02
 Operator : SY/MD
 Sample : VV1120WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK272

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029215.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	102	rBV	189920	207482	16.34%	2.023%
2	1.564	155	163	179	rVB	161395	184900	14.57%	1.803%
3	2.101	320	330	357	rVB	336795	501048	39.47%	4.885%
4	2.500	444	454	470	rVB2	19082	32319	2.55%	0.315%
5	3.899	874	889	916	rBV2	70874	291419	22.96%	2.841%
6	4.336	1010	1025	1048	rVB	211941	528774	41.65%	5.156%
7	5.037	1227	1243	1271	rBV2	509520	1269466	100.00%	12.378%
8	5.606	1407	1420	1447	rBV	423798	875731	68.98%	8.539%
9	6.059	1547	1561	1594	rBV	283165	589598	46.44%	5.749%
10	6.979	1836	1847	1872	rBV	123704	240611	18.95%	2.346%
11	7.307	1935	1949	1984	rBV	626861	1111164	87.53%	10.834%
12	7.616	2036	2045	2072	rBV	64262	126966	10.00%	1.238%
13	8.085	2180	2191	2255	rBV	389766	1107228	87.22%	10.796%
14	8.419	2285	2295	2314	rBV2	12363	26295	2.07%	0.256%
15	8.844	2415	2427	2457	rBV	609224	1021225	80.45%	9.958%
16	10.207	2840	2851	2876	rBV	194210	326813	25.74%	3.187%
17	11.239	3161	3172	3201	rBV	584817	929659	73.23%	9.065%
18	11.616	3275	3289	3310	rBV	537063	869326	68.48%	8.476%
19	13.503	3861	3876	3885	rBV	9856	15812	1.25%	0.154%




Sum of corrected areas: 10255836

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029215.D
Acq On : 20 Nov 2022 11:02
Operator : SY/MD
Sample : VV1120WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

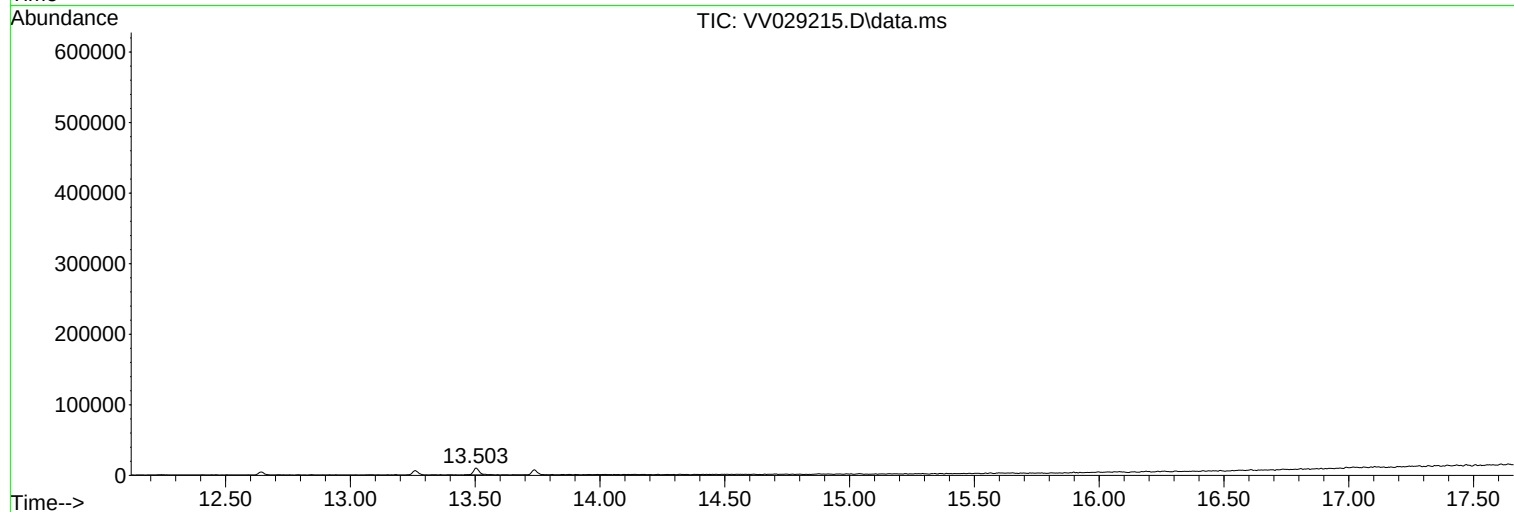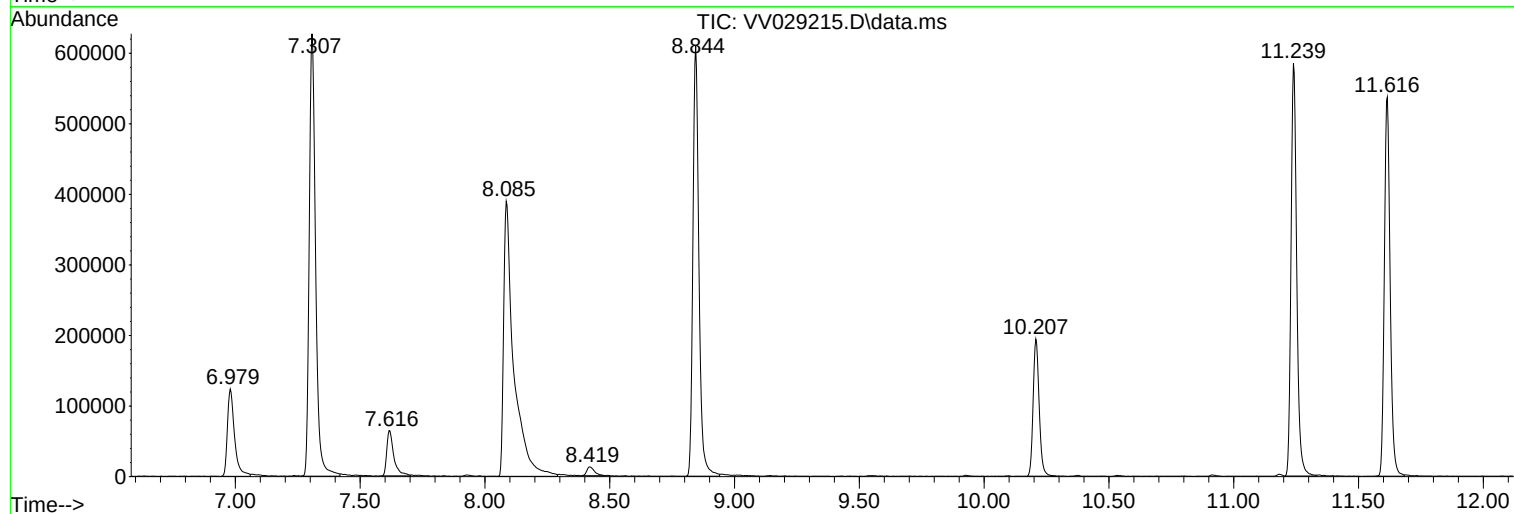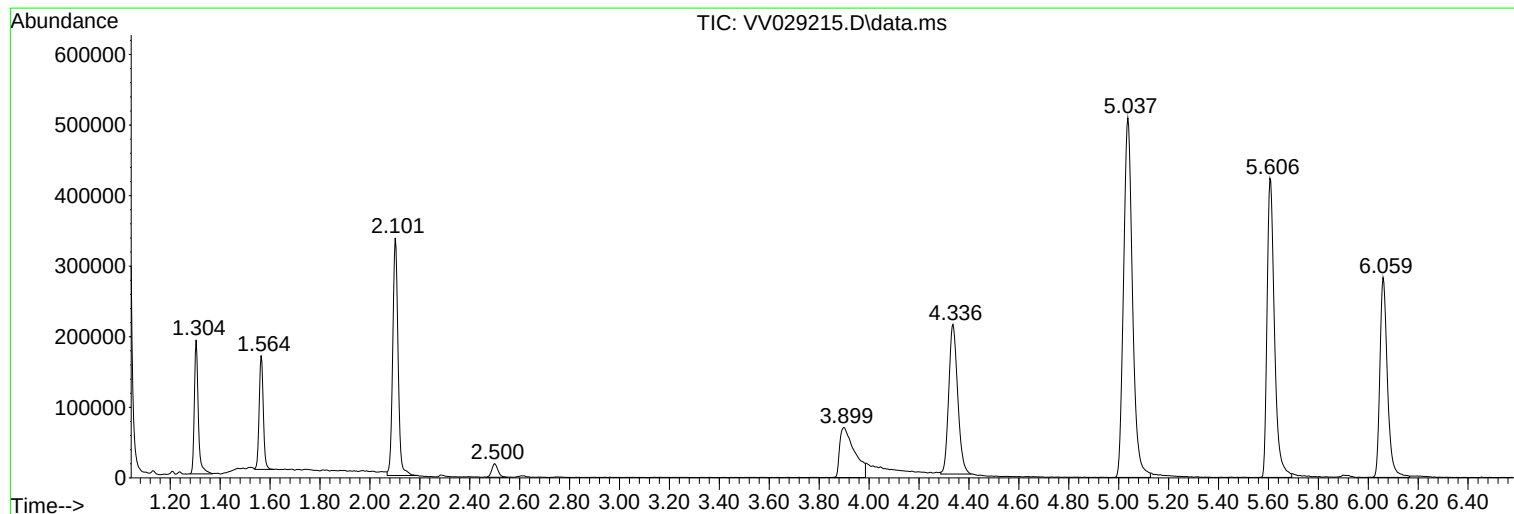

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029215.D
Acq On : 20 Nov 2022 11:02
Operator : SY/MD
Sample : VV1120WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029215.D
Acq On : 20 Nov 2022 11:02
Operator : SY/MD
Sample : VV1120WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------