

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029217.D
 Acq On : 20 Nov 2022 11:57
 Operator : SY/MD
 Sample : N5651-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1K9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029217.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	103	rVB	136926	154338	4.38%	1.148%
2	1.426	107	120	124	rBV2	17213	38316	1.09%	0.285%
3	1.568	157	164	177	rVB	113553	135432	3.85%	1.007%
4	2.105	321	331	349	rVB	235091	350741	9.96%	2.608%
5	2.767	524	537	552	rBV	19679	41559	1.18%	0.309%
6	3.902	876	890	935	rBV2	109312	418268	11.88%	3.111%
7	4.343	1011	1027	1061	rBV	151810	393725	11.18%	2.928%
8	5.043	1229	1245	1294	rBV2	351893	912420	25.91%	6.786%
9	5.613	1410	1422	1447	rBV	329705	690964	19.62%	5.139%
10	5.908	1500	1514	1548	rBV	1014619	2013836	57.19%	14.977%
11	6.066	1551	1563	1591	rVB	197939	415288	11.79%	3.088%
12	6.982	1837	1848	1878	rBV	86778	174219	4.95%	1.296%
13	7.310	1937	1950	1976	rBV	423125	769558	21.86%	5.723%
14	7.622	2037	2047	2073	rBV2	47259	91932	2.61%	0.684%
15	7.969	2131	2155	2182	rBV	2055761	3521188	100.00%	26.187%
16	8.088	2182	2192	2241	rVB	320888	763289	21.68%	5.677%
17	8.847	2415	2428	2458	rBV	482536	816993	23.20%	6.076%
18	10.210	2841	2852	2874	rBV	144262	230399	6.54%	1.713%
19	10.378	2891	2904	2919	rBV	76727	133026	3.78%	0.989%
20	11.243	3161	3173	3194	rBV	474995	773000	21.95%	5.749%
21	11.616	3278	3289	3306	rBV	374003	607909	17.26%	4.521%




Sum of corrected areas: 13446400

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029217.D
Acq On : 20 Nov 2022 11:57
Operator : SY/MD
Sample : N5651-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1K9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

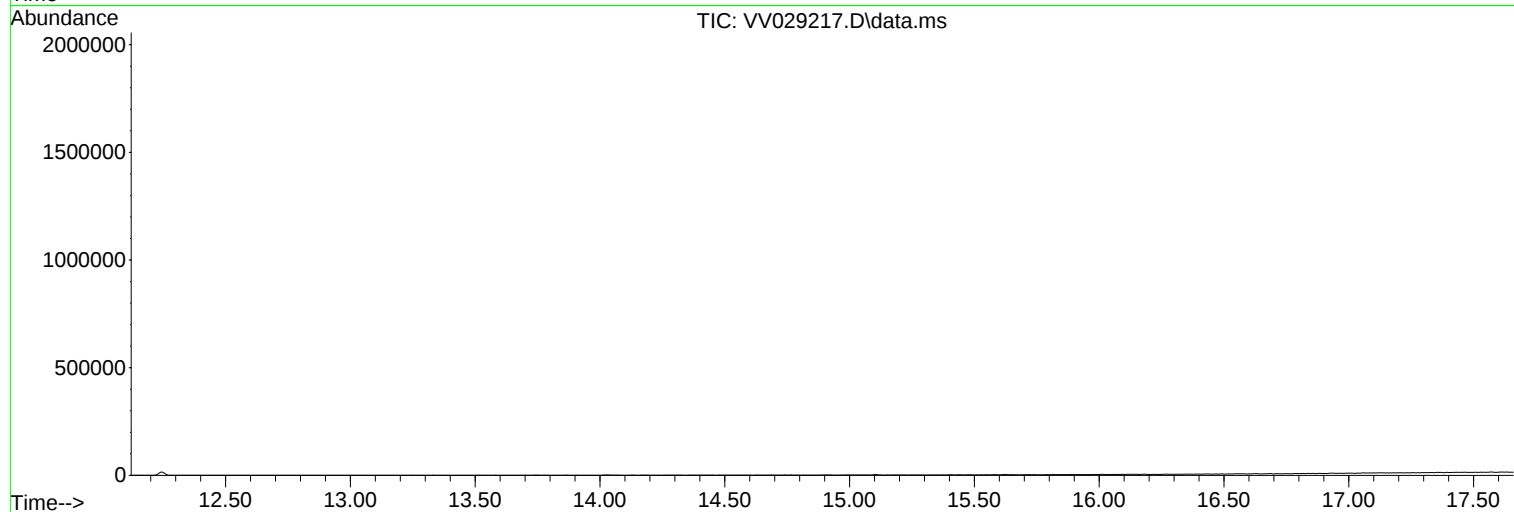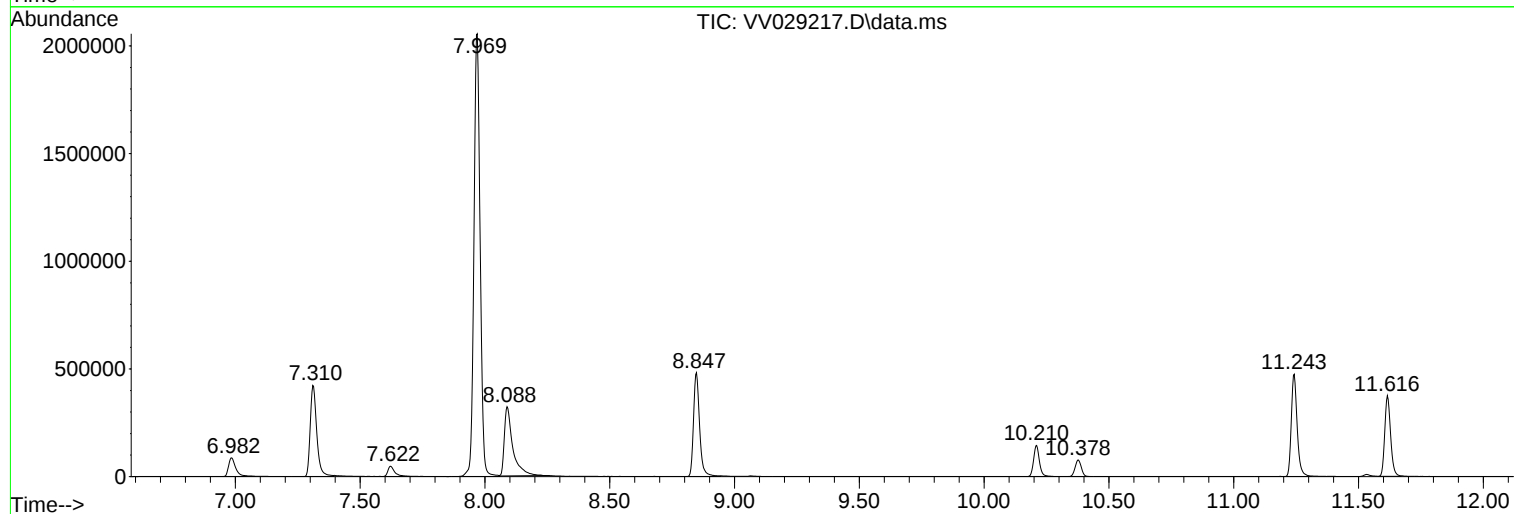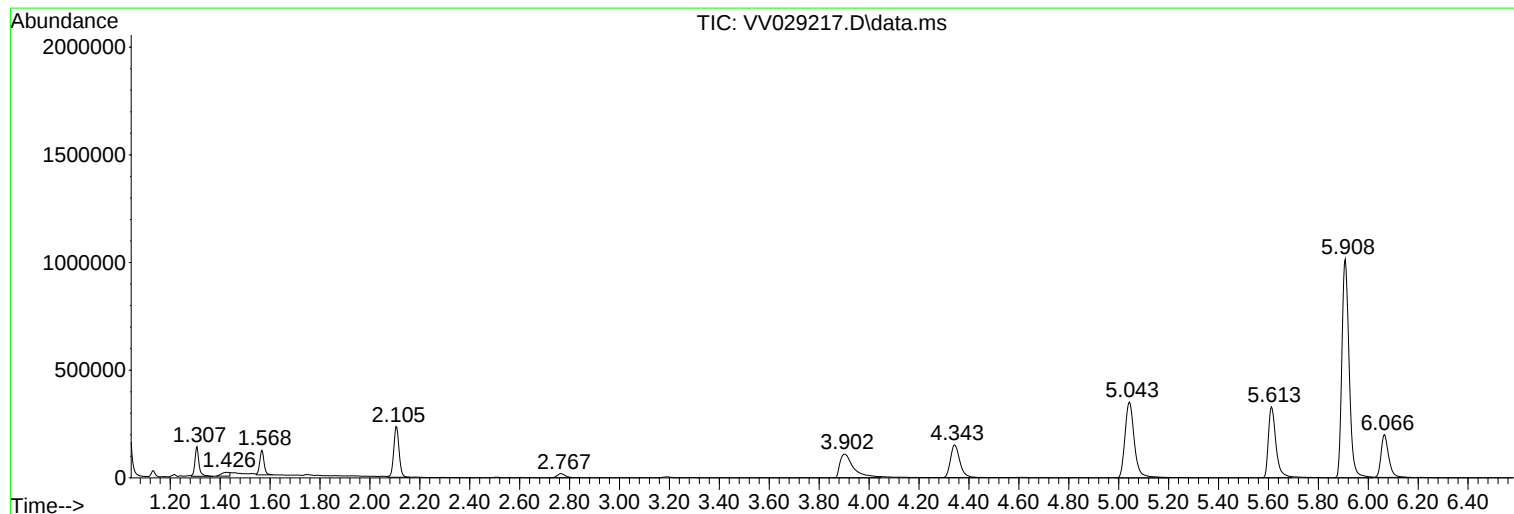

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029217.D
Acq On : 20 Nov 2022 11:57
Operator : SY/MD
Sample : N5651-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1K9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029217.D
Acq On : 20 Nov 2022 11:57
Operator : SY/MD
Sample : N5651-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1K9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc