

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029223.D
 Acq On : 20 Nov 2022 14:24
 Operator : SY/MD
 Sample : N5651-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029223.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rVB	132001	147794	15.47%	1.892%
2	1.568	156	164	177	rBV	120978	136551	14.29%	1.748%
3	2.105	321	331	351	rVB	245512	357716	37.43%	4.579%
4	2.507	443	456	469	rVB2	11532	21060	2.20%	0.270%
5	3.902	879	890	935	rBV	52144	252860	26.46%	3.237%
6	4.342	1009	1027	1058	rBV2	158452	398707	41.72%	5.104%
7	5.043	1229	1245	1282	rBV2	376074	955658	100.00%	12.234%
8	5.613	1410	1422	1457	rBV	322970	677603	70.90%	8.674%
9	6.066	1549	1563	1586	rBV	207274	438775	45.91%	5.617%
10	6.985	1837	1849	1880	rBV	87289	176648	18.48%	2.261%
11	7.310	1939	1950	1987	rBV	449701	812991	85.07%	10.407%
12	7.622	2037	2047	2072	rBV	47844	94339	9.87%	1.208%
13	7.934	2132	2144	2156	rBV2	8528	15216	1.59%	0.195%
14	8.088	2182	2192	2243	rBV	300781	843795	88.29%	10.802%
15	8.847	2417	2428	2466	rBV	466562	798659	83.57%	10.224%
16	10.210	2841	2852	2872	rBV	152619	249318	26.09%	3.192%
17	10.378	2893	2904	2918	rVB2	20583	33681	3.52%	0.431%
18	11.243	3161	3173	3197	rBV	448748	726231	75.99%	9.297%
19	11.615	3278	3289	3317	rBV	417283	674067	70.53%	8.629%




Sum of corrected areas: 7811669

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029223.D
Acq On : 20 Nov 2022 14:24
Operator : SY/MD
Sample : N5651-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

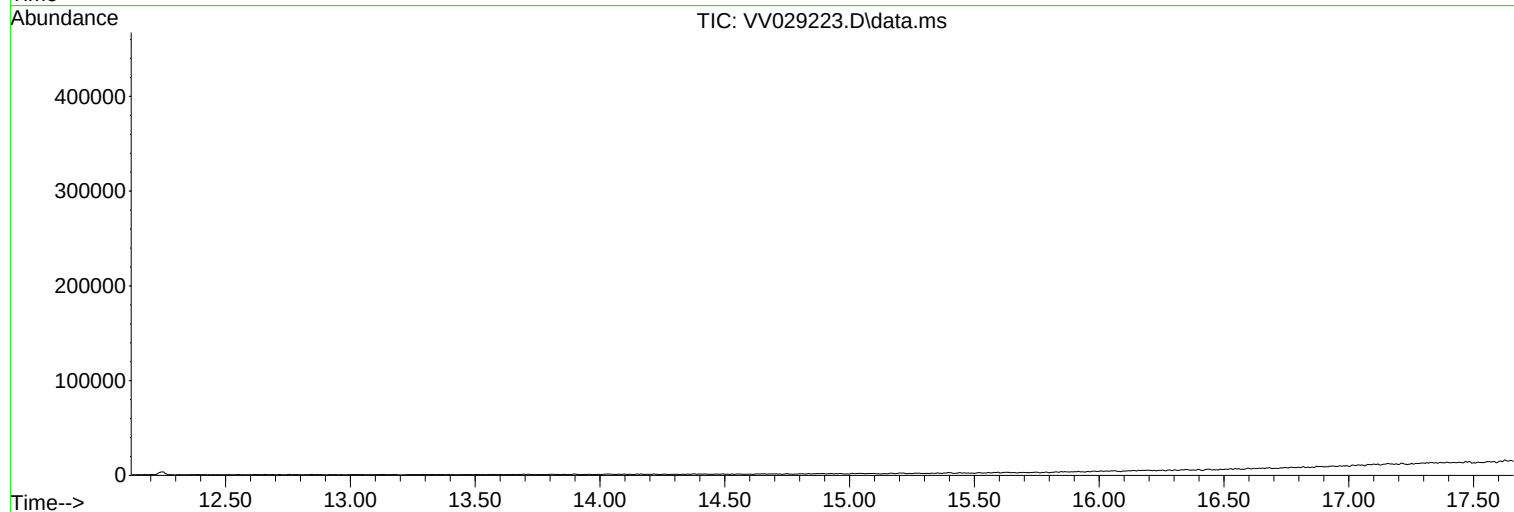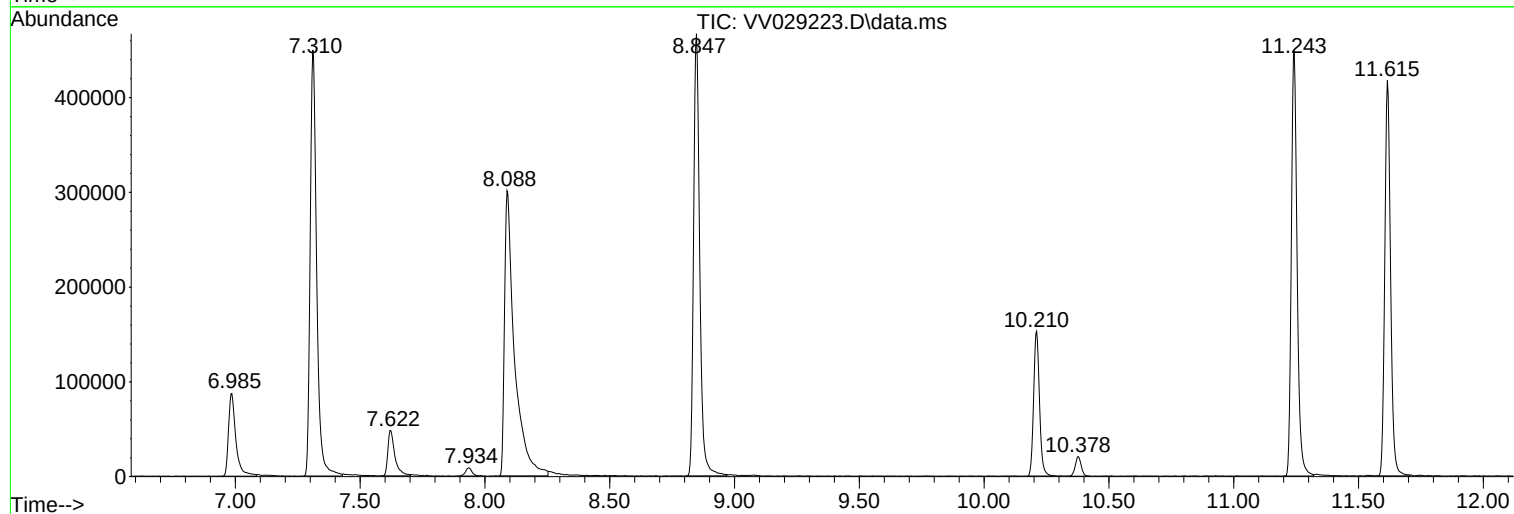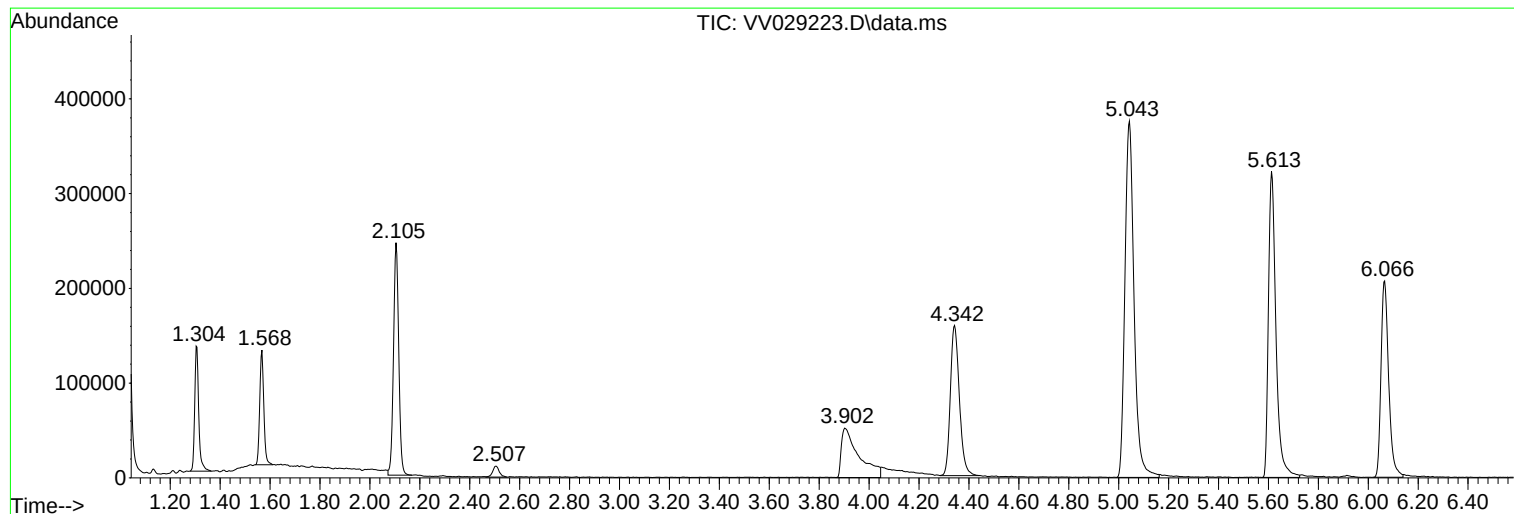

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029223.D
Acq On : 20 Nov 2022 14:24
Operator : SY/MD
Sample : N5651-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029223.D
Acq On : 20 Nov 2022 14:24
Operator : SY/MD
Sample : N5651-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
