

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029225.D
 Acq On : 20 Nov 2022 15:13
 Operator : SY/MD
 Sample : N5652-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1K5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029225.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	105	rVB	138790	158977	7.36%	1.456%
2	1.452	111	128	133	rBV2	15160	44153	2.04%	0.404%
3	1.568	157	164	175	rVB	122352	138628	6.42%	1.269%
4	1.751	211	221	241	rVB	1656108	2160216	100.00%	19.778%
5	2.108	321	332	350	rVB2	285987	459684	21.28%	4.209%
6	2.764	521	536	565	rBV2	39915	90237	4.18%	0.826%
7	3.188	654	668	685	rBV2	29324	62192	2.88%	0.569%
8	3.892	877	887	929	rBV2	86915	337806	15.64%	3.093%
9	4.343	1010	1027	1059	rBV2	173179	480141	22.23%	4.396%
10	4.603	1092	1108	1127	rBV4	11179	27533	1.27%	0.252%
11	5.044	1229	1245	1281	rBV2	383598	977486	45.25%	8.949%
12	5.613	1410	1422	1462	rBV	364290	767469	35.53%	7.027%
13	5.918	1504	1517	1543	rBV3	35287	79063	3.66%	0.724%
14	6.066	1550	1563	1596	rBV	214297	455125	21.07%	4.167%
15	6.982	1838	1848	1872	rBV	93072	183357	8.49%	1.679%
16	7.310	1939	1950	1979	rBV	463039	834323	38.62%	7.639%
17	7.622	2036	2047	2073	rBV	49767	97902	4.53%	0.896%
18	7.934	2134	2144	2151	rBV2	13081	23060	1.07%	0.211%
19	8.088	2182	2192	2239	rBV	352103	855556	39.61%	7.833%
20	8.847	2414	2428	2456	rBV	529049	888417	41.13%	8.134%
21	10.207	2840	2851	2873	rBV	158270	259198	12.00%	2.373%
22	10.378	2894	2904	2919	rVB2	33793	56211	2.60%	0.515%
23	11.243	3160	3173	3196	rBV	492203	793847	36.75%	7.268%
24	11.616	3277	3289	3314	rBV	430564	691760	32.02%	6.333%




Sum of corrected areas: 10922341

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029225.D
Acq On : 20 Nov 2022 15:13
Operator : SY/MD
Sample : N5652-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1K5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

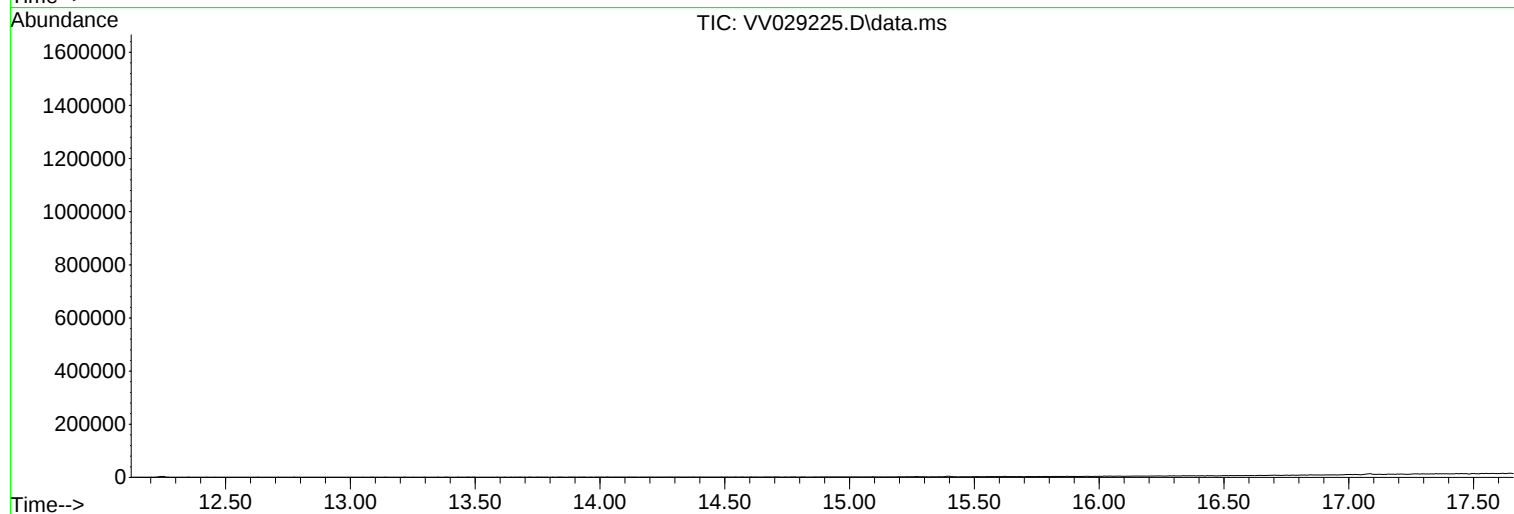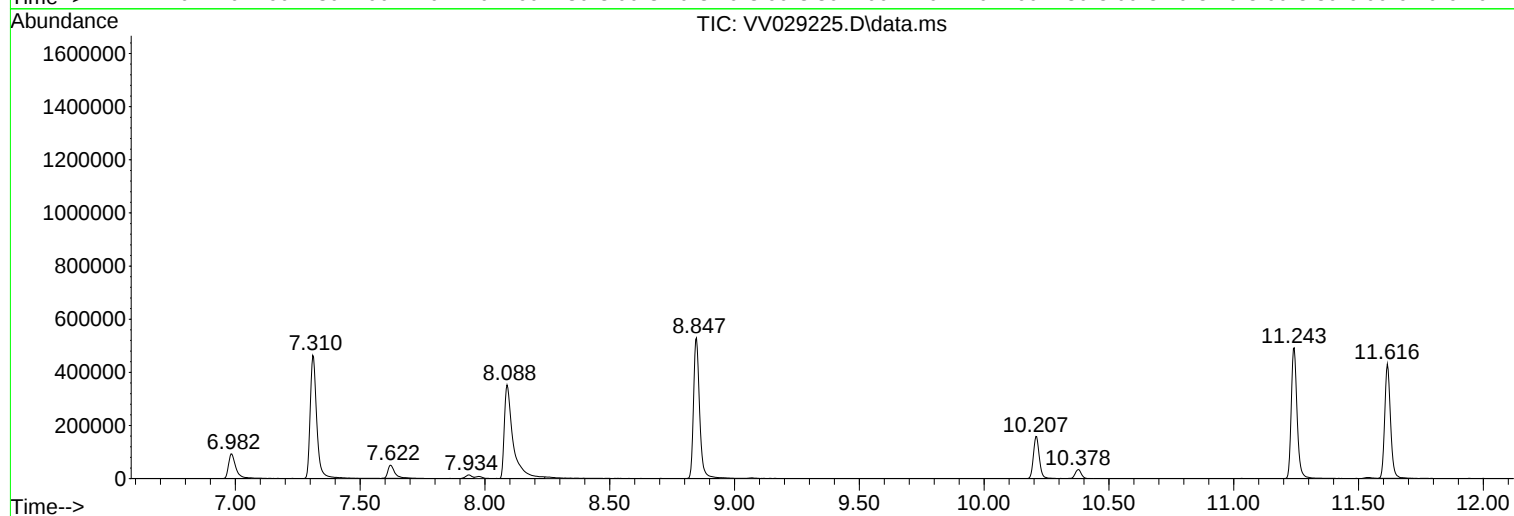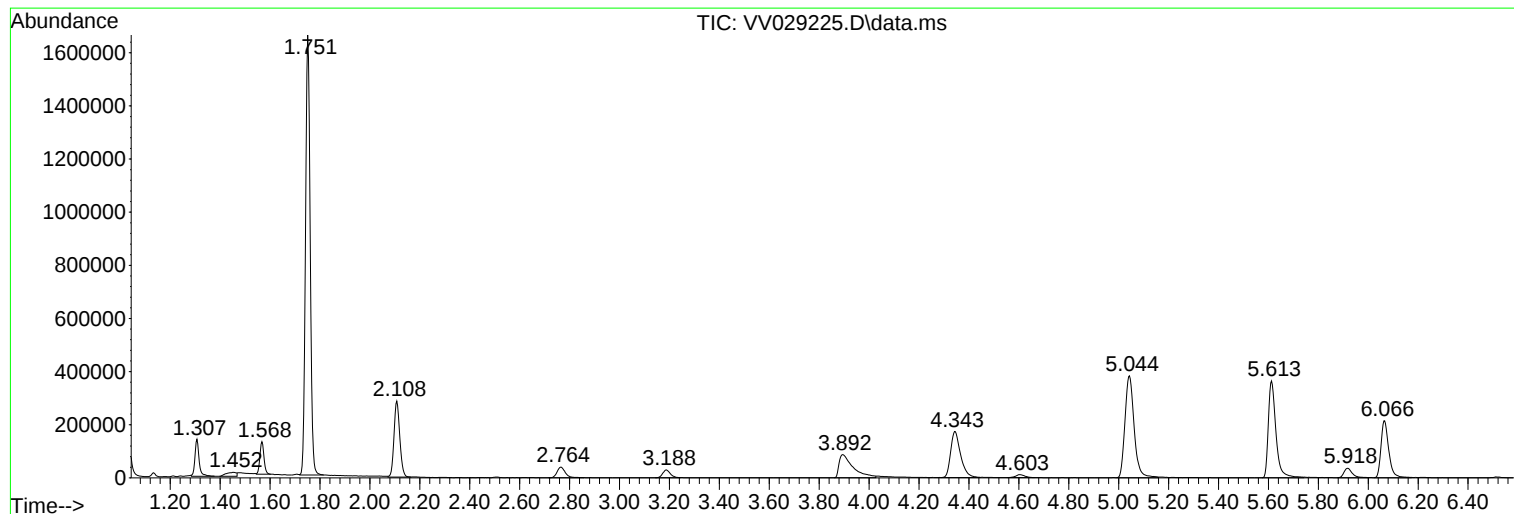

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029225.D
Acq On : 20 Nov 2022 15:13
Operator : SY/MD
Sample : N5652-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1K5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029225.D
Acq On : 20 Nov 2022 15:13
Operator : SY/MD
Sample : N5652-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1K5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc