

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029226.D
 Acq On : 20 Nov 2022 15:37
 Operator : SY/MD
 Sample : N5652-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1K6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029226.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.130	22	28	37	rVB	27225	26390	2.74%	0.323%
2	1.307	75	83	99	rVV	135086	148507	15.44%	1.820%
3	1.510	130	146	148	rBV	7232	16156	1.68%	0.198%
4	1.568	156	164	178	rVB	120384	140438	14.60%	1.721%
5	1.751	215	221	231	rVB	17519	22363	2.32%	0.274%
6	2.105	321	331	348	rVB	243511	358779	37.29%	4.396%
7	2.767	525	537	551	rBV2	10996	23459	2.44%	0.287%
8	3.905	874	891	932	rBV	69976	327297	34.02%	4.010%
9	4.342	1009	1027	1058	rBV	164143	437595	45.49%	5.362%
10	5.043	1229	1245	1282	rBV2	378957	962059	100.00%	11.788%
11	5.613	1411	1422	1460	rBV	314553	660283	68.63%	8.091%
12	5.915	1506	1516	1536	rBV4	37699	81839	8.51%	1.003%
13	6.066	1548	1563	1589	rBV	206818	439013	45.63%	5.379%
14	6.985	1838	1849	1871	rBV	89614	177153	18.41%	2.171%
15	7.310	1937	1950	1990	rBV	449321	822919	85.54%	10.084%
16	7.622	2037	2047	2062	rBV	48638	90311	9.39%	1.107%
17	7.934	2131	2144	2147	rBV	13525	19480	2.02%	0.239%
18	7.973	2148	2156	2175	rVB	56068	101091	10.51%	1.239%
19	8.088	2182	2192	2239	rBV	346767	854593	88.83%	10.472%
20	8.847	2416	2428	2451	rBV	458086	772807	80.33%	9.469%
21	10.210	2840	2852	2871	rBV	154383	250761	26.07%	3.073%
22	10.374	2892	2903	2917	rVB	35357	59970	6.23%	0.735%
23	11.243	3161	3173	3205	rBV	421399	680994	70.79%	8.344%
24	11.532	3256	3263	3273	rBV2	5495	9885	1.03%	0.121%
25	11.615	3278	3289	3309	rVV	410739	667224	69.35%	8.176%
26	12.242	3473	3484	3495	rBV3	6170	9679	1.01%	0.119%




Sum of corrected areas: 8161045

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029226.D
Acq On : 20 Nov 2022 15:37
Operator : SY/MD
Sample : N5652-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

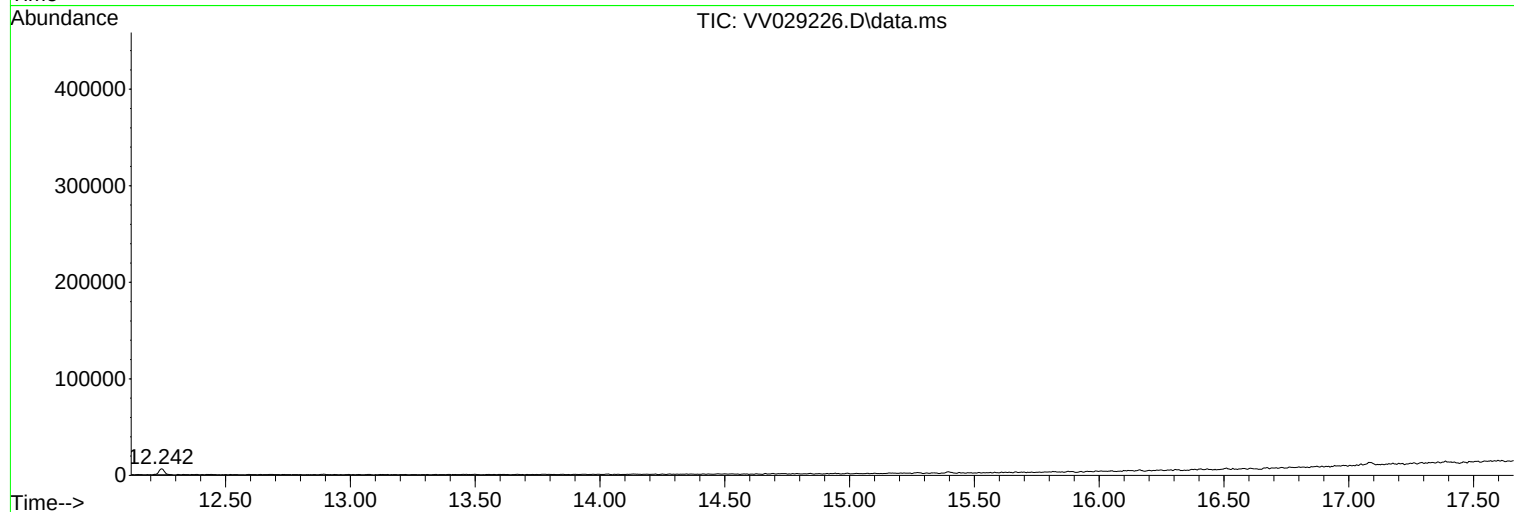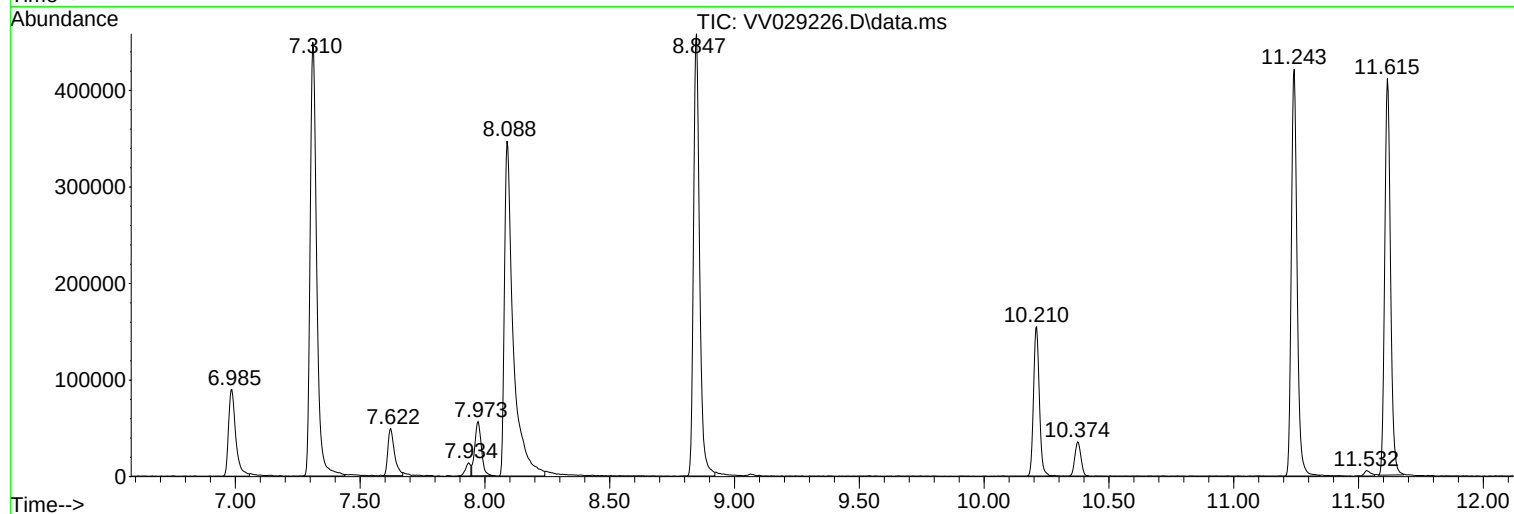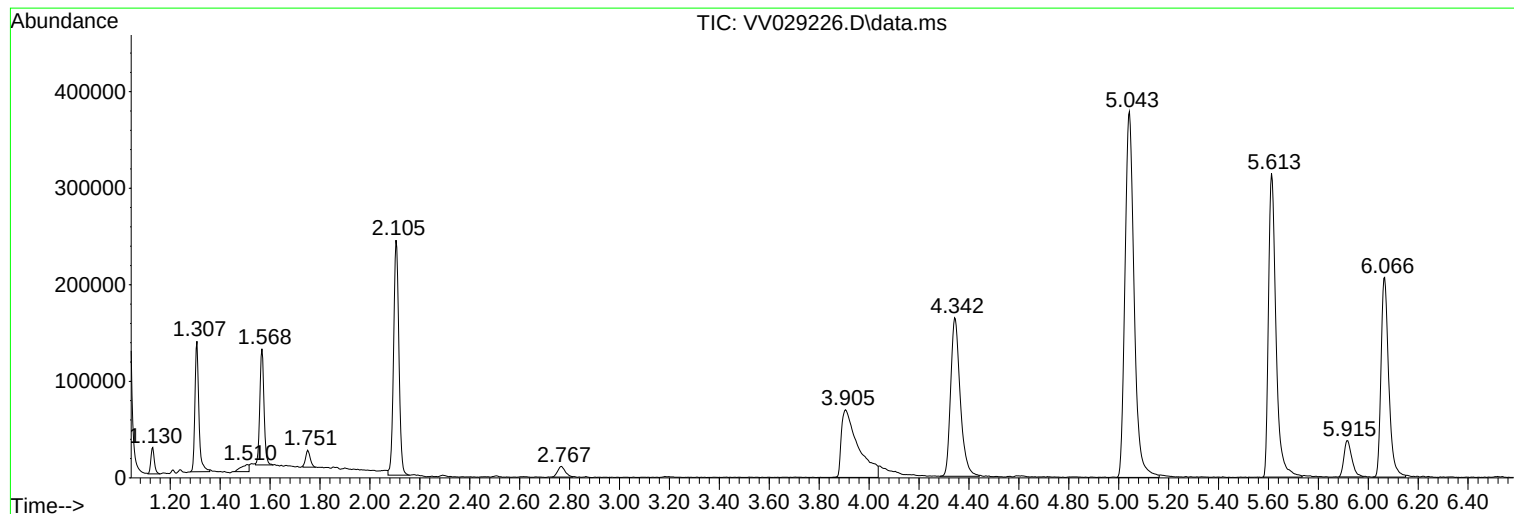

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029226.D
Acq On : 20 Nov 2022 15:37
Operator : SY/MD
Sample : N5652-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029226.D
Acq On : 20 Nov 2022 15:37
Operator : SY/MD
Sample : N5652-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc