

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029230.D
 Acq On : 20 Nov 2022 17:15
 Operator : SY/MD
 Sample : N5652-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1L6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029230.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.130	21	28	47	rBV	118897	120323	12.73%	1.323%
2	1.307	74	83	99	rBV	133691	146345	15.48%	1.610%
3	1.462	118	131	132	rBV8	9602	17714	1.87%	0.195%
4	1.568	157	164	181	rVB	121243	142980	15.12%	1.573%
5	1.751	212	221	238	rVB	211587	279861	29.60%	3.078%
6	2.105	321	331	349	rVB	234217	350356	37.06%	3.854%
7	2.764	518	536	561	rBV	172645	385633	40.79%	4.242%
8	3.188	653	668	686	rBV2	17726	38424	4.06%	0.423%
9	3.902	873	890	944	rBV2	80978	373734	39.53%	4.111%
10	4.342	1010	1027	1051	rBV	161010	434007	45.90%	4.774%
11	5.043	1229	1245	1285	rBV2	370258	945499	100.00%	10.400%
12	5.612	1409	1422	1452	rBV	324695	678772	71.79%	7.466%
13	5.911	1502	1515	1549	rBV	94736	206378	21.83%	2.270%
14	6.066	1549	1563	1587	rBV	207949	435636	46.07%	4.792%
15	6.985	1838	1849	1872	rBV	87482	173896	18.39%	1.913%
16	7.310	1938	1950	1974	rBV	435804	791872	83.75%	8.710%
17	7.622	2034	2047	2067	rBV	47308	91303	9.66%	1.004%
18	7.934	2130	2144	2150	rBV2	20566	38539	4.08%	0.424%
19	7.973	2150	2156	2176	rVB2	32364	57223	6.05%	0.629%
20	8.088	2182	2192	2237	rBV	341509	838833	88.72%	9.227%
21	8.847	2417	2428	2468	rBV	471613	810338	85.70%	8.913%
22	10.210	2840	2852	2871	rBV	157978	252205	26.67%	2.774%
23	10.378	2890	2904	2918	rVB	52524	89614	9.48%	0.986%
24	11.242	3162	3173	3199	rBV	434227	715043	75.63%	7.865%
25	11.615	3276	3289	3312	rBV	417426	663663	70.19%	7.300%
26	12.246	3469	3485	3494	rBV2	7815	13224	1.40%	0.145%




Sum of corrected areas: 9091415

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029230.D
Acq On : 20 Nov 2022 17:15
Operator : SY/MD
Sample : N5652-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1L6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

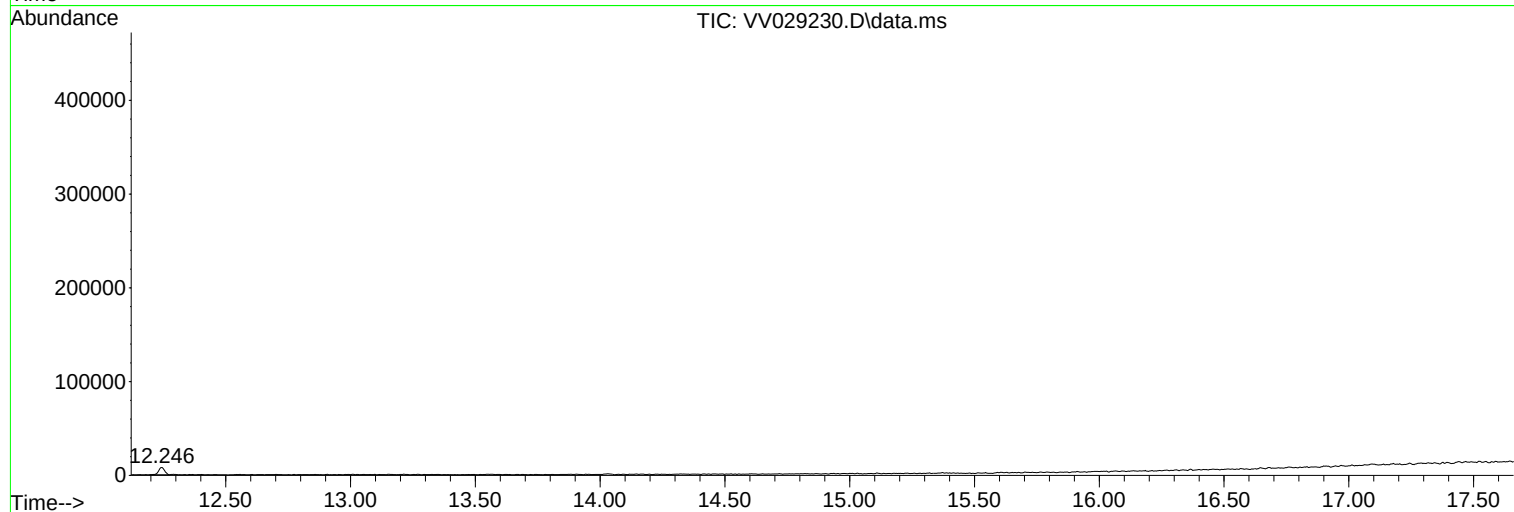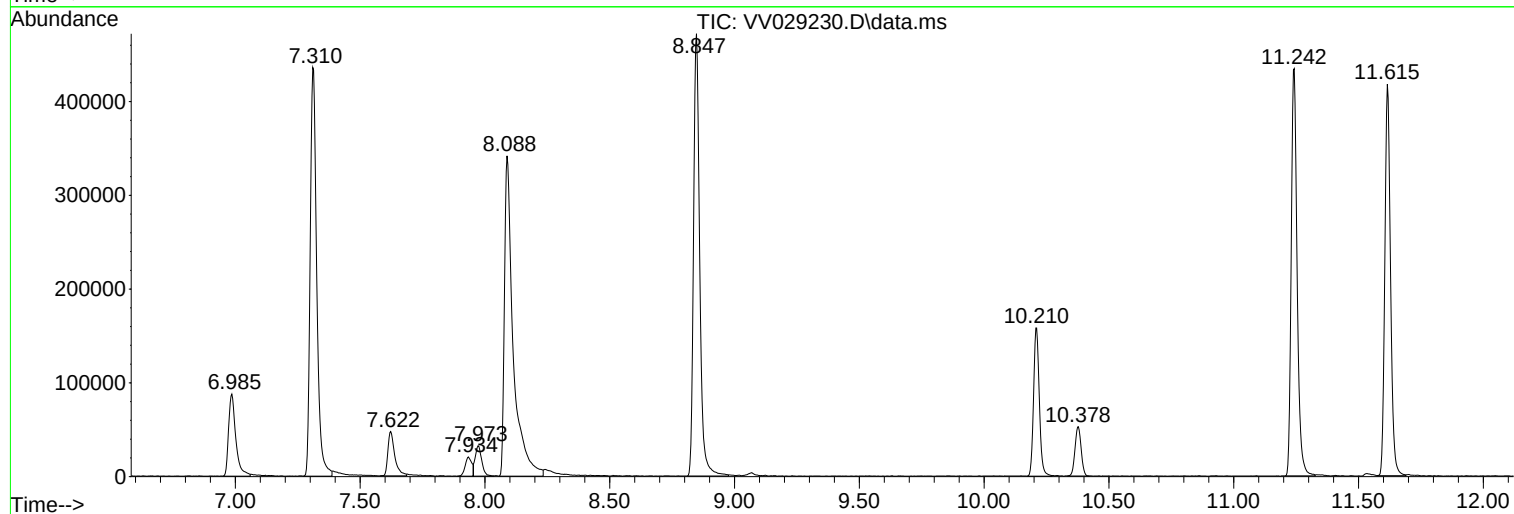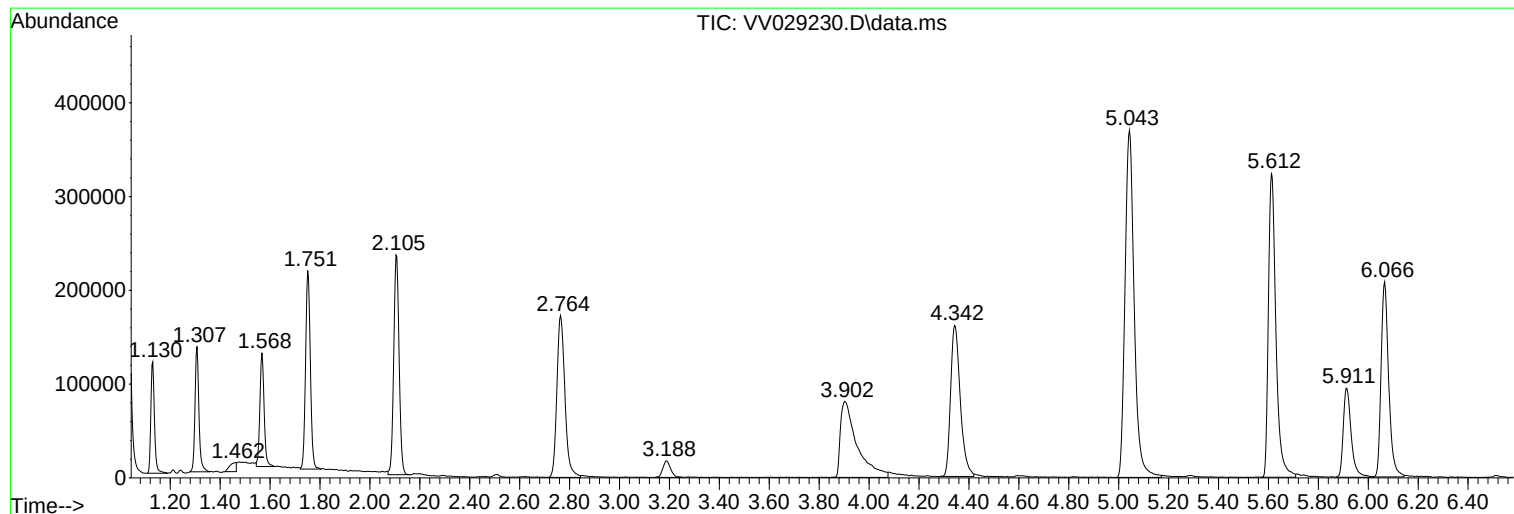

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029230.D
Acq On : 20 Nov 2022 17:15
Operator : SY/MD
Sample : N5652-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1L6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029230.D
Acq On : 20 Nov 2022 17:15
Operator : SY/MD
Sample : N5652-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1L6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------