

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029231.D
 Acq On : 20 Nov 2022 17:40
 Operator : SY/MD
 Sample : N5652-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1L7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029231.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.130	21	28	38	rVB	33254	32842	3.53%	0.393%
2	1.307	75	83	96	rVB	127096	137690	14.81%	1.649%
3	1.449	112	127	129	rBV2	18257	35705	3.84%	0.428%
4	1.568	157	164	177	rVB	115669	136420	14.68%	1.633%
5	1.754	216	222	231	rVB	8972	11952	1.29%	0.143%
6	2.105	320	331	345	rVB	227511	333754	35.90%	3.996%
7	2.764	519	536	559	rBV	45492	101386	10.91%	1.214%
8	3.188	653	668	679	rBV3	6099	13205	1.42%	0.158%
9	3.899	877	889	925	rBV2	73530	306738	33.00%	3.673%
10	4.342	1007	1027	1063	rBV	161407	447985	48.19%	5.364%
11	5.043	1228	1245	1288	rBV2	365790	929606	100.00%	11.131%
12	5.613	1410	1422	1449	rBV	345128	715482	76.97%	8.567%
13	5.915	1504	1516	1540	rBV2	63403	138987	14.95%	1.664%
14	6.066	1551	1563	1585	rBV	202978	426070	45.83%	5.102%
15	6.985	1838	1849	1869	rBV	87773	171400	18.44%	2.052%
16	7.310	1936	1950	1984	rBV	431454	785555	84.50%	9.406%
17	7.622	2037	2047	2066	rBV	47221	90962	9.79%	1.089%
18	7.934	2133	2144	2150	rBV	17952	32689	3.52%	0.391%
19	7.973	2150	2156	2175	rVB2	25096	43776	4.71%	0.524%
20	8.088	2182	2192	2232	rBV	339682	840138	90.38%	10.060%
21	8.847	2416	2428	2457	rBV	503016	838238	90.17%	10.037%
22	10.207	2837	2851	2869	rBV	154476	251080	27.01%	3.006%
23	10.378	2891	2904	2918	rVB2	47430	80864	8.70%	0.968%
24	11.243	3161	3173	3198	rBV	473380	776537	83.53%	9.298%
25	11.616	3278	3289	3314	rVV	405520	660061	71.00%	7.903%
26	12.243	3474	3484	3497	rVB2	7557	12539	1.35%	0.150%




Sum of corrected areas: 8351661

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029231.D
Acq On : 20 Nov 2022 17:40
Operator : SY/MD
Sample : N5652-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1L7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

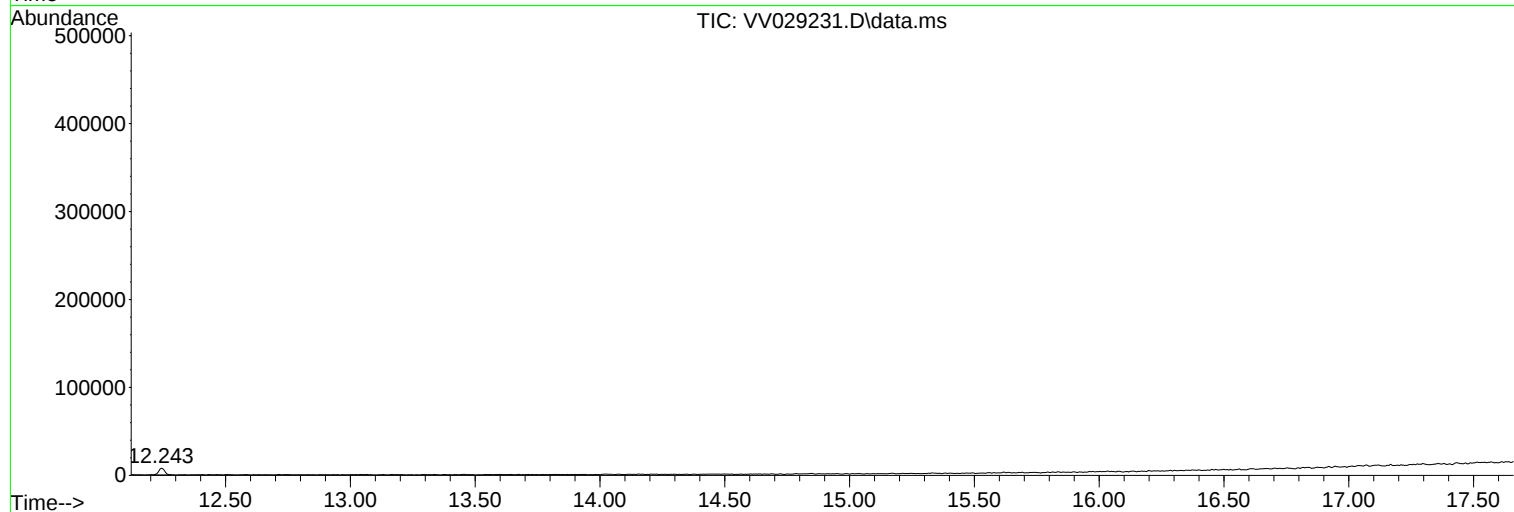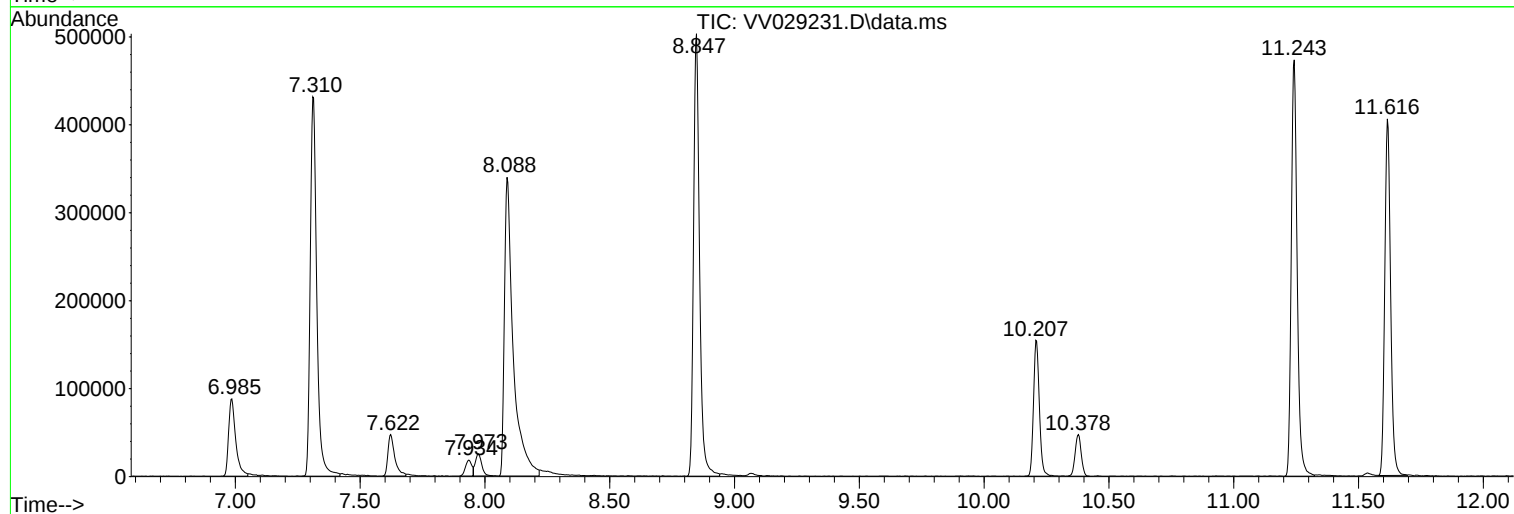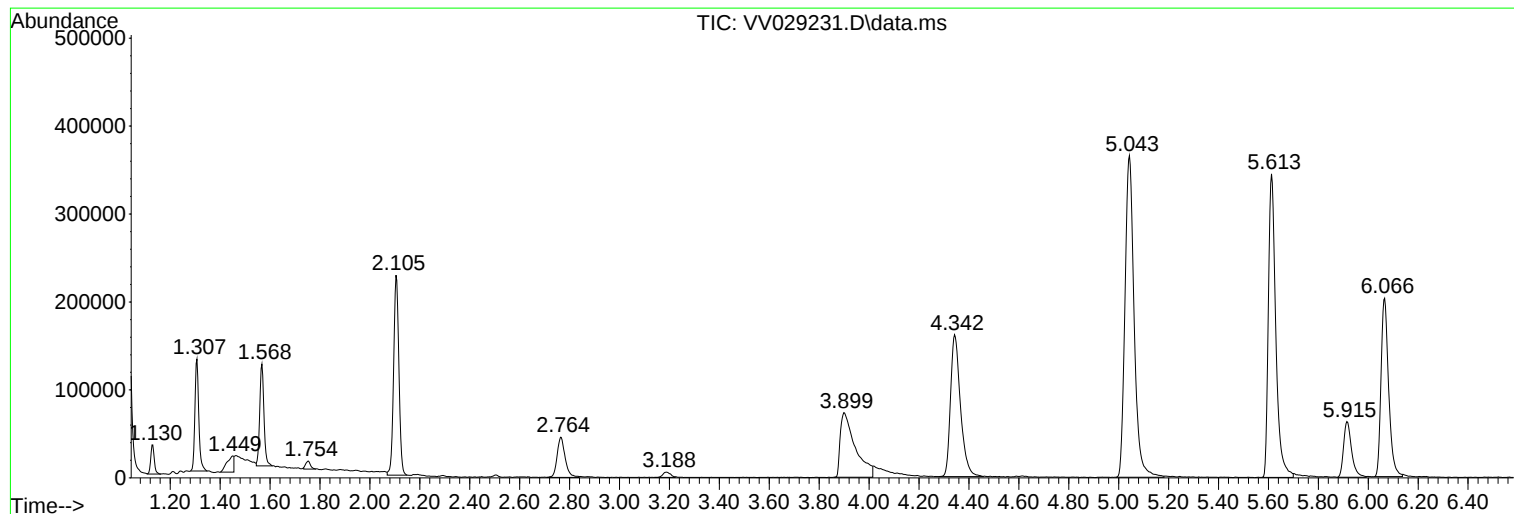

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029231.D
Acq On : 20 Nov 2022 17:40
Operator : SY/MD
Sample : N5652-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1L7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029231.D
Acq On : 20 Nov 2022 17:40
Operator : SY/MD
Sample : N5652-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1L7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc