

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029232.D
 Acq On : 20 Nov 2022 18:04
 Operator : SY/MD
 Sample : N5652-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1L8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	102	rVB	131859	146924	15.88%	1.869%
2	1.439	111	124	126	rBV	16362	30366	3.28%	0.386%
3	1.568	157	164	178	rVB	115068	133907	14.48%	1.703%
4	2.108	321	332	347	rVB	232255	342561	37.03%	4.357%
5	3.892	877	887	928	rBV2	89620	333955	36.10%	4.247%
6	4.343	1009	1027	1062	rBV	161771	446222	48.24%	5.675%
7	5.044	1229	1245	1279	rBV2	364271	925066	100.00%	11.765%
8	5.613	1411	1422	1451	rBV	325883	675191	72.99%	8.587%
9	5.918	1503	1517	1538	rVB5	15628	38148	4.12%	0.485%
10	6.066	1546	1563	1597	rBV	206010	434916	47.01%	5.531%
11	6.982	1837	1848	1879	rBV	88703	176616	19.09%	2.246%
12	7.310	1939	1950	1978	rBV	432073	781932	84.53%	9.945%
13	7.622	2037	2047	2066	rBV	46071	90984	9.84%	1.157%
14	7.937	2133	2145	2152	rBV2	13282	24683	2.67%	0.314%
15	7.979	2152	2158	2168	rVB4	7544	11910	1.29%	0.151%
16	8.088	2181	2192	2231	rBV	347225	829647	89.69%	10.552%
17	8.847	2416	2428	2460	rBV	469800	797396	86.20%	10.141%
18	10.211	2839	2852	2875	rBV	151898	249234	26.94%	3.170%
19	10.374	2892	2903	2918	rVB	32819	58204	6.29%	0.740%
20	11.243	3162	3173	3197	rBV	415544	684152	73.96%	8.701%
21	11.616	3277	3289	3315	rBV	394198	650750	70.35%	8.276%




Sum of corrected areas: 7862764

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029232.D
Acq On : 20 Nov 2022 18:04
Operator : SY/MD
Sample : N5652-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1L8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

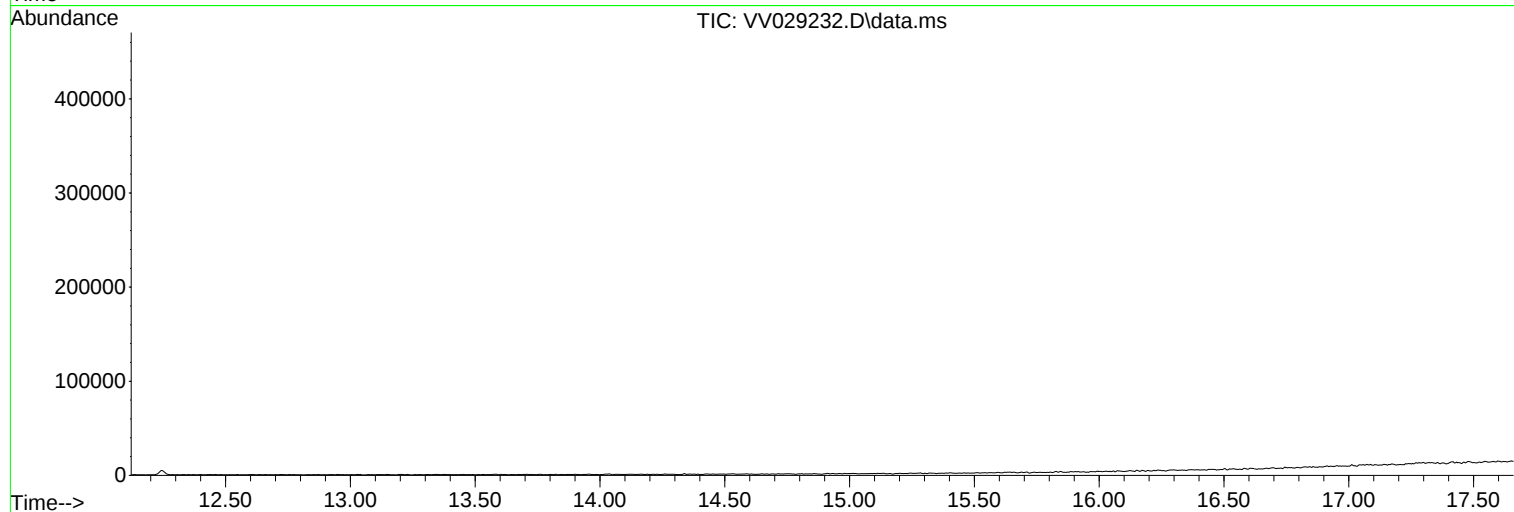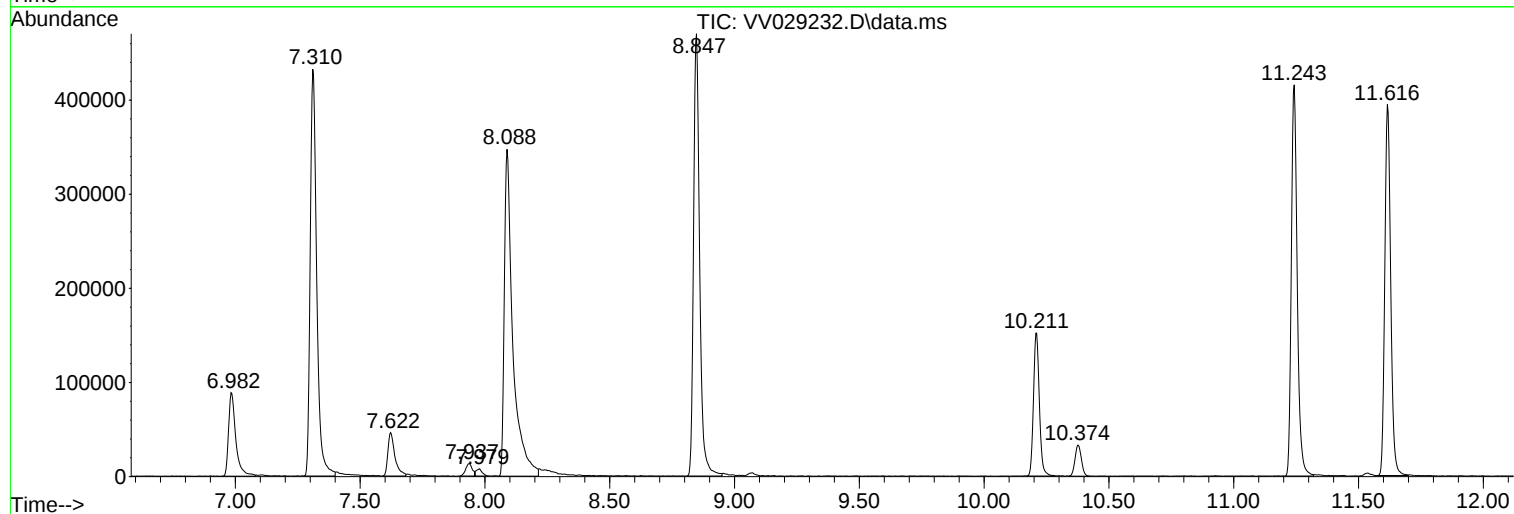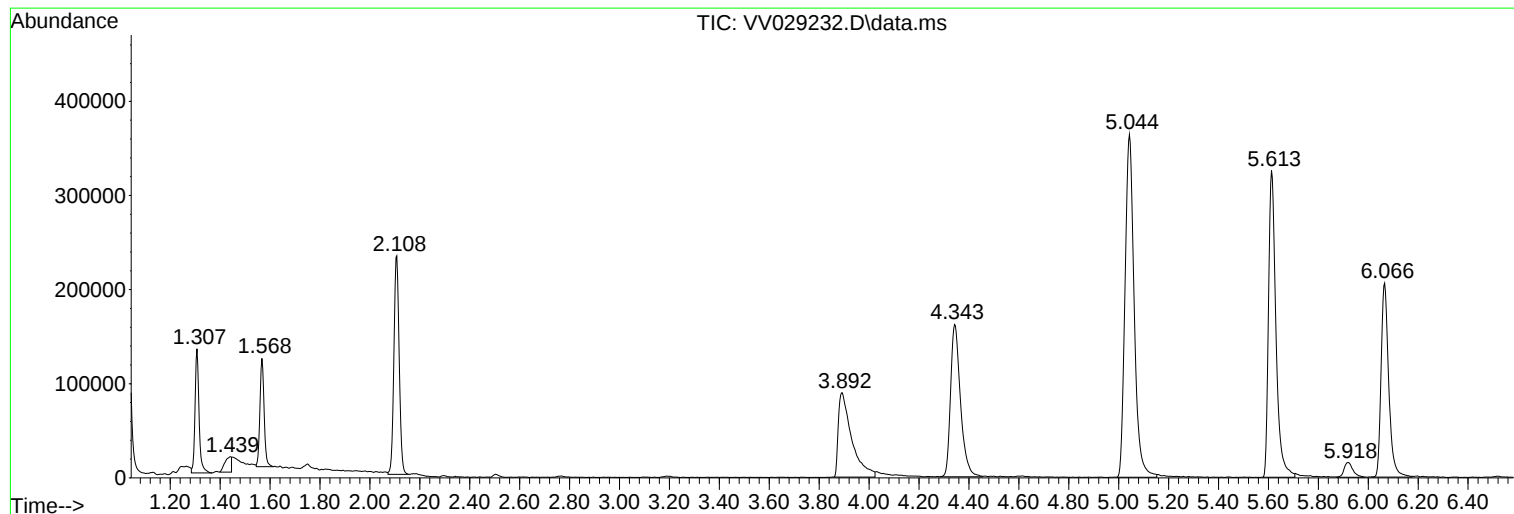

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029232.D
Acq On : 20 Nov 2022 18:04
Operator : SY/MD
Sample : N5652-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1L8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029232.D
Acq On : 20 Nov 2022 18:04
Operator : SY/MD
Sample : N5652-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1L8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc