

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029234.D
 Acq On : 20 Nov 2022 18:53
 Operator : SY/MD
 Sample : N5652-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1M0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029234.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	104	rVB	128687	147614	15.97%	1.728%
2	1.458	113	130	132	rBV2	13792	30626	3.31%	0.359%
3	1.568	157	164	181	rVB	118103	140294	15.18%	1.642%
4	1.706	201	207	214	rBV	18384	20950	2.27%	0.245%
5	1.751	215	221	232	rVB	28193	34907	3.78%	0.409%
6	2.108	321	332	347	rVB2	251497	393143	42.54%	4.602%
7	2.764	522	536	558	rBV	19518	45124	4.88%	0.528%
8	3.188	654	668	690	rBV	44176	94812	10.26%	1.110%
9	3.899	874	889	918	rBV2	80131	327413	35.42%	3.833%
10	4.342	1011	1027	1063	rBV2	166213	475061	51.40%	5.561%
11	4.603	1092	1108	1129	rVB	10353	25470	2.76%	0.298%
12	5.043	1227	1245	1273	rBV2	361356	924281	100.00%	10.820%
13	5.612	1408	1422	1444	rBV	341599	705048	76.28%	8.254%
14	5.915	1505	1516	1540	rBV2	66392	143243	15.50%	1.677%
15	6.066	1548	1563	1590	rBV	206079	434292	46.99%	5.084%
16	6.982	1838	1848	1868	rBV	91423	177846	19.24%	2.082%
17	7.310	1938	1950	1974	rBV	430113	777736	84.14%	9.105%
18	7.622	2036	2047	2069	rBV	48971	93658	10.13%	1.096%
19	7.937	2134	2145	2149	rBV	16592	29164	3.16%	0.341%
20	7.972	2149	2156	2172	rVB2	43171	77373	8.37%	0.906%
21	8.088	2181	2192	2238	rBV	342123	839943	90.88%	9.833%
22	8.847	2416	2428	2452	rBV	495213	828114	89.60%	9.694%
23	10.210	2839	2852	2872	rBV	154129	253535	27.43%	2.968%
24	10.377	2891	2904	2917	rVB2	46528	79839	8.64%	0.935%
25	11.242	3161	3173	3198	rBV	464761	757401	81.94%	8.867%
26	11.535	3255	3264	3278	rBV4	5721	12213	1.32%	0.143%
27	11.615	3278	3289	3310	rVV	403691	658327	71.23%	7.707%
28	12.246	3474	3485	3496	rBV	8786	14748	1.60%	0.173%




Sum of corrected areas: 8542175

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029234.D
Acq On : 20 Nov 2022 18:53
Operator : SY/MD
Sample : N5652-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1M0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

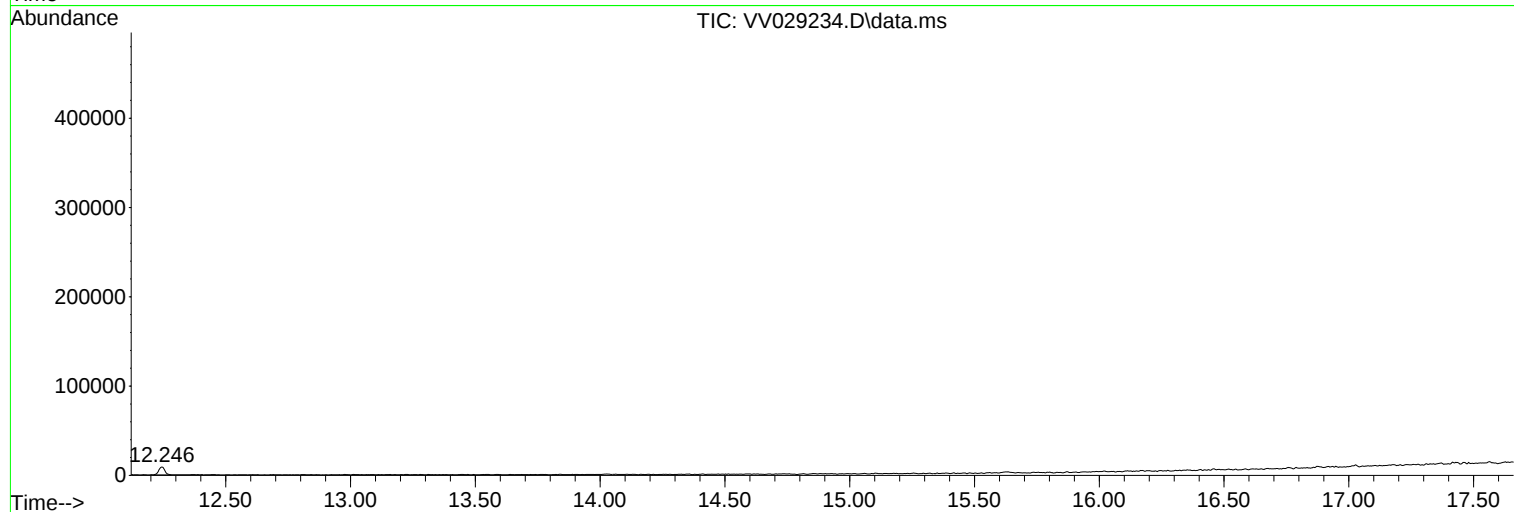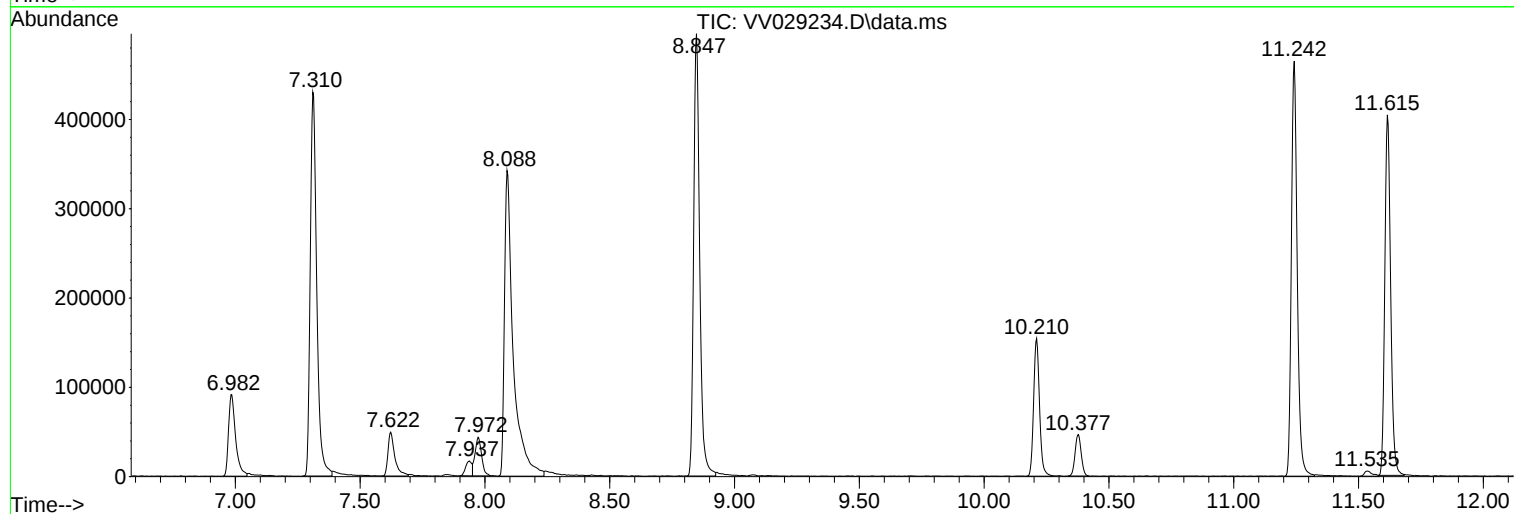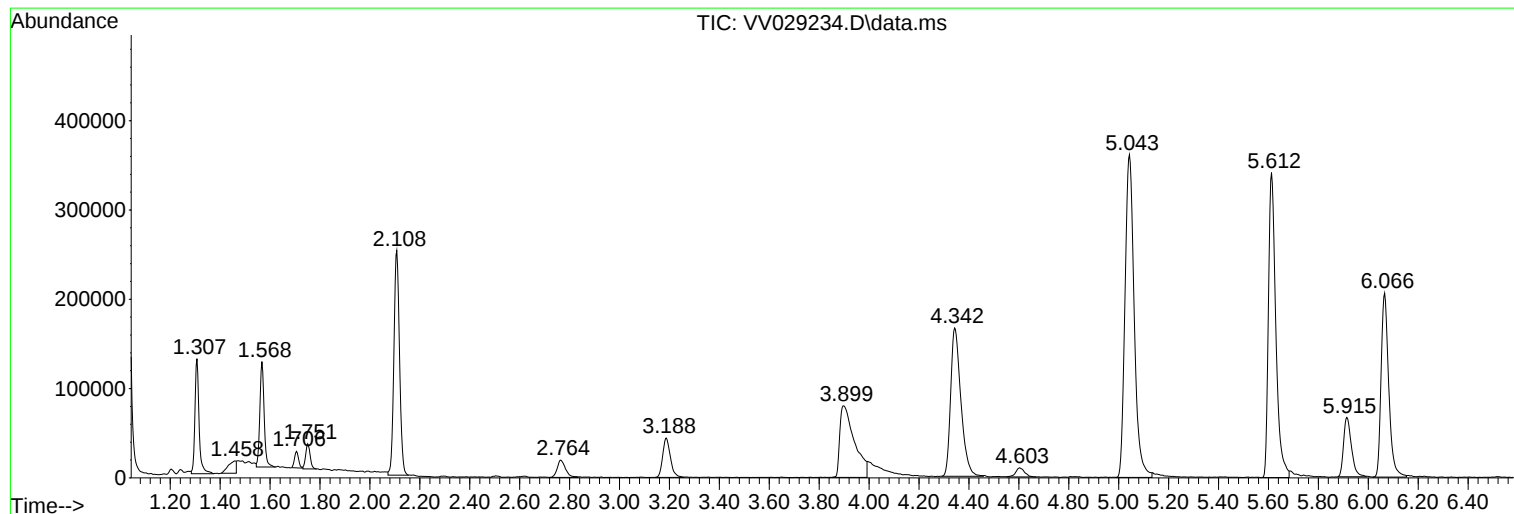

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029234.D
Acq On : 20 Nov 2022 18:53
Operator : SY/MD
Sample : N5652-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1M0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029234.D
Acq On : 20 Nov 2022 18:53
Operator : SY/MD
Sample : N5652-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1M0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc