

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029244.D
 Acq On : 20 Nov 2022 23:45
 Operator : SY/MD
 Sample : N5648-22
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H46F9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029244.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	72	83	102	rVB	121018	143113	16.49%	1.945%
2	1.568	156	164	176	rVB	109336	125201	14.43%	1.702%
3	2.105	321	331	349	rVB	209476	312982	36.07%	4.255%
4	3.908	882	892	920	rBV	42105	175205	20.19%	2.382%
5	4.342	1012	1027	1055	rVB	147919	376512	43.39%	5.118%
6	5.043	1229	1245	1281	rBV2	341487	867779	100.00%	11.797%
7	5.612	1409	1422	1445	rBV	323723	666704	76.83%	9.063%
8	6.066	1549	1563	1592	rBV	190910	407770	46.99%	5.543%
9	6.985	1836	1849	1876	rBV2	80515	161556	18.62%	2.196%
10	7.310	1939	1950	1974	rBV	395780	717952	82.73%	9.760%
11	7.622	2038	2047	2068	rBV2	43068	86122	9.92%	1.171%
12	7.934	2131	2144	2158	rBV2	13240	23423	2.70%	0.318%
13	8.091	2183	2193	2255	rBV2	274514	819074	94.39%	11.135%
14	8.847	2416	2428	2464	rBV	464679	797147	91.86%	10.837%
15	10.210	2841	2852	2873	rBV	143185	239788	27.63%	3.260%
16	10.374	2888	2903	2917	rBV2	32619	55060	6.34%	0.748%
17	11.242	3161	3173	3194	rBV	453106	731995	84.35%	9.951%
18	11.615	3277	3289	3317	rBV	386390	628168	72.39%	8.539%
19	12.242	3472	3484	3494	rVB2	6925	11384	1.31%	0.155%
20	12.667	3607	3616	3628	rBV5	6253	9176	1.06%	0.125%




Sum of corrected areas: 7356111

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029244.D
Acq On : 20 Nov 2022 23:45
Operator : SY/MD
Sample : N5648-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46F9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

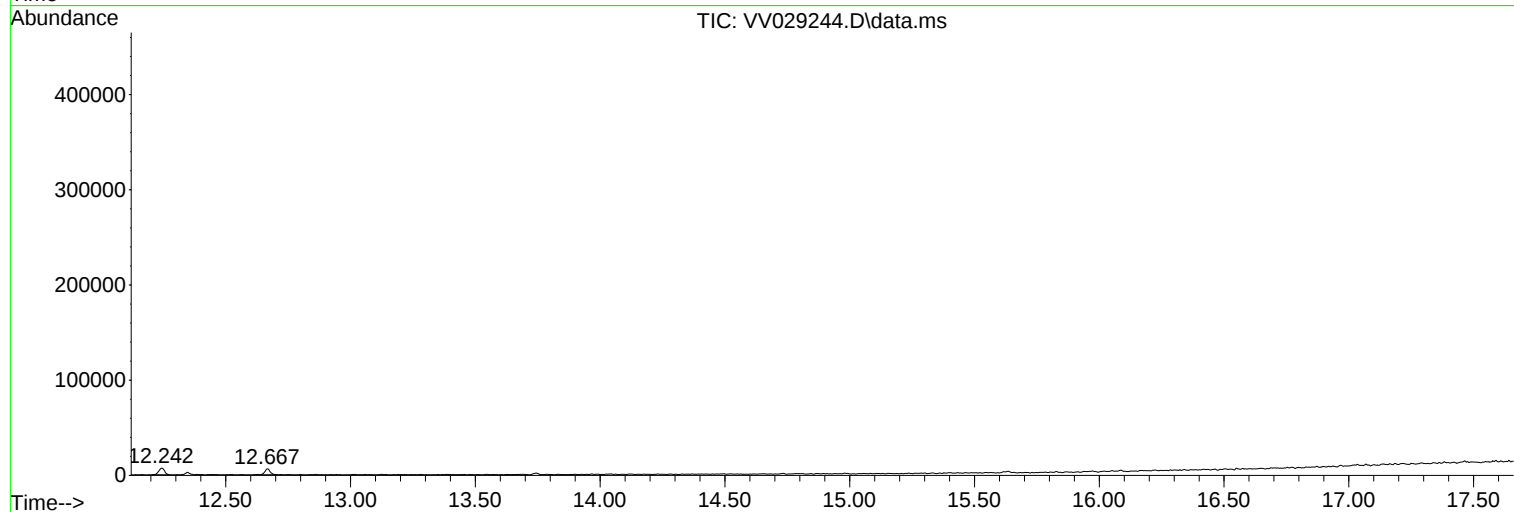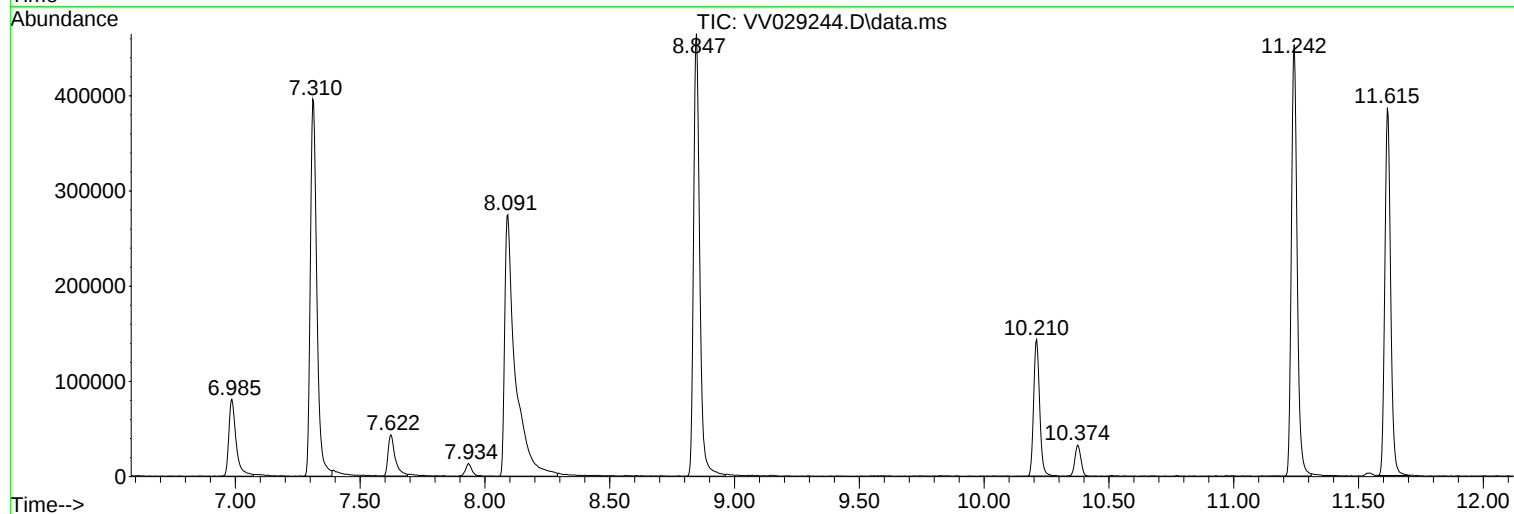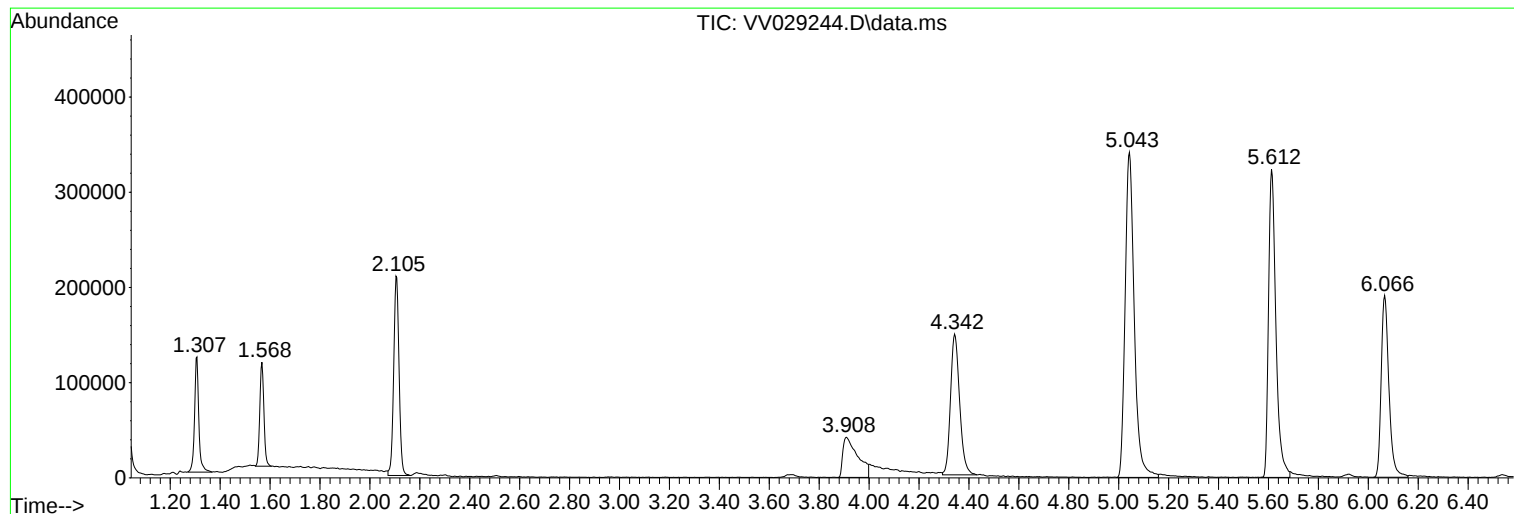

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029244.D
Acq On : 20 Nov 2022 23:45
Operator : SY/MD
Sample : N5648-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46F9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029244.D
Acq On : 20 Nov 2022 23:45
Operator : SY/MD
Sample : N5648-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46F9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc