

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029248.D
 Acq On : 21 Nov 2022 01:22
 Operator : SY/MD
 Sample : N5666-03DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGXP5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029248.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	16	21	26	rBV3	10077	9666	1.18%	0.125%
2	1.217	48	55	71	rBV	47109	48402	5.92%	0.628%
3	1.307	74	83	101	rBV	107268	120238	14.70%	1.560%
4	1.413	111	116	123	rBV	10080	10979	1.34%	0.142%
5	1.568	156	164	178	rVB	102884	119096	14.56%	1.546%
6	2.108	321	332	348	rVB3	211098	340969	41.68%	4.425%
7	2.503	445	455	470	rVB2	15303	26795	3.28%	0.348%
8	3.188	653	668	687	rBV2	44733	95306	11.65%	1.237%
9	3.908	877	892	937	rBV2	277602	818146	100.00%	10.618%
10	4.342	1013	1027	1053	rVB	141402	361521	44.19%	4.692%
11	4.603	1093	1108	1124	rVB3	14979	36124	4.42%	0.469%
12	5.043	1227	1245	1272	rBV2	318480	813174	99.39%	10.553%
13	5.612	1410	1422	1459	rBV	290066	613736	75.02%	7.965%
14	5.915	1504	1516	1546	rVB3	62648	135440	16.55%	1.758%
15	6.066	1551	1563	1592	rBV	178428	380141	46.46%	4.933%
16	6.985	1838	1849	1866	rBV	76601	147734	18.06%	1.917%
17	7.310	1936	1950	1994	rBV	348816	645865	78.94%	8.382%
18	7.622	2037	2047	2069	rBV3	41541	80842	9.88%	1.049%
19	8.091	2183	2193	2242	rBV	252092	770192	94.14%	9.995%
20	8.847	2416	2428	2461	rBV	409964	699080	85.45%	9.073%
21	10.210	2838	2852	2875	rBV	141202	236350	28.89%	3.067%
22	10.374	2895	2903	2914	rVB2	5622	9921	1.21%	0.129%
23	11.242	3162	3173	3197	rBV	386803	632070	77.26%	8.203%
24	11.615	3277	3289	3312	rBV	338988	553602	67.67%	7.185%




Sum of corrected areas: 7705389

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029248.D
Acq On : 21 Nov 2022 01:22
Operator : SY/MD
Sample : N5666-03DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGXP5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

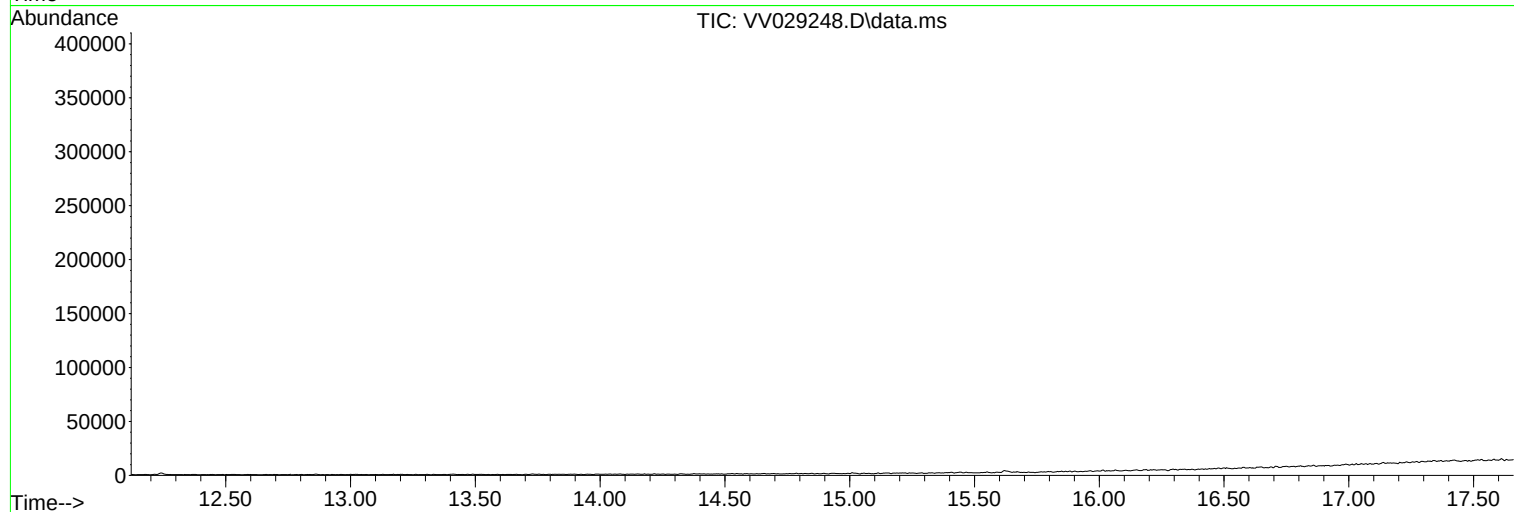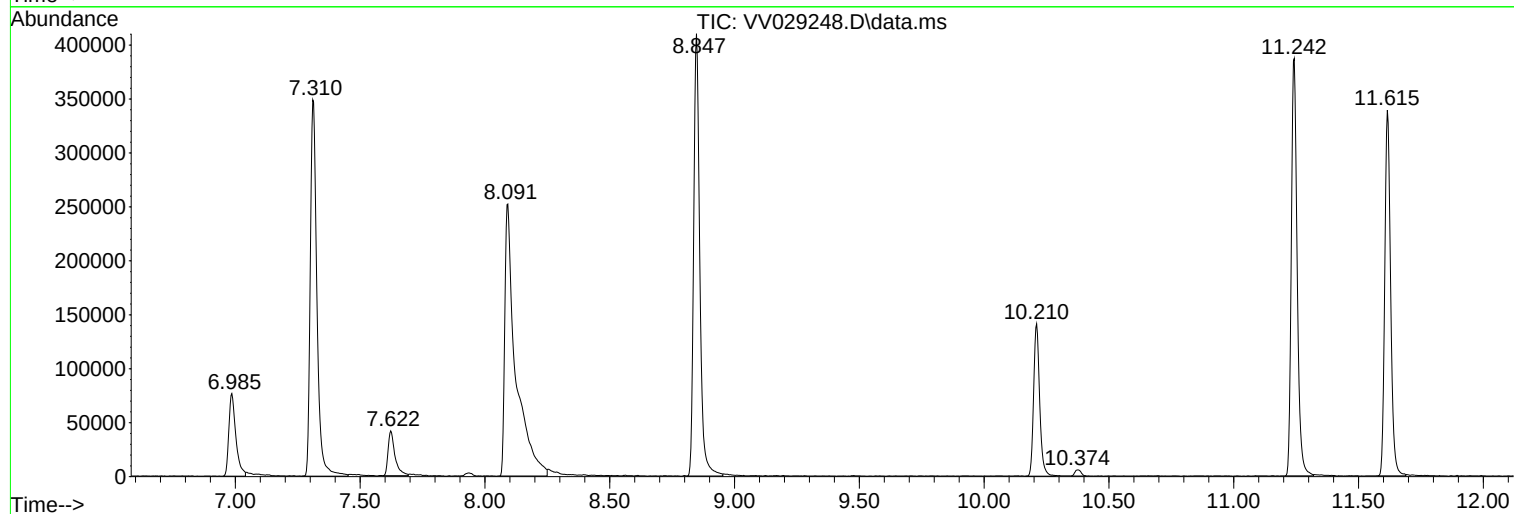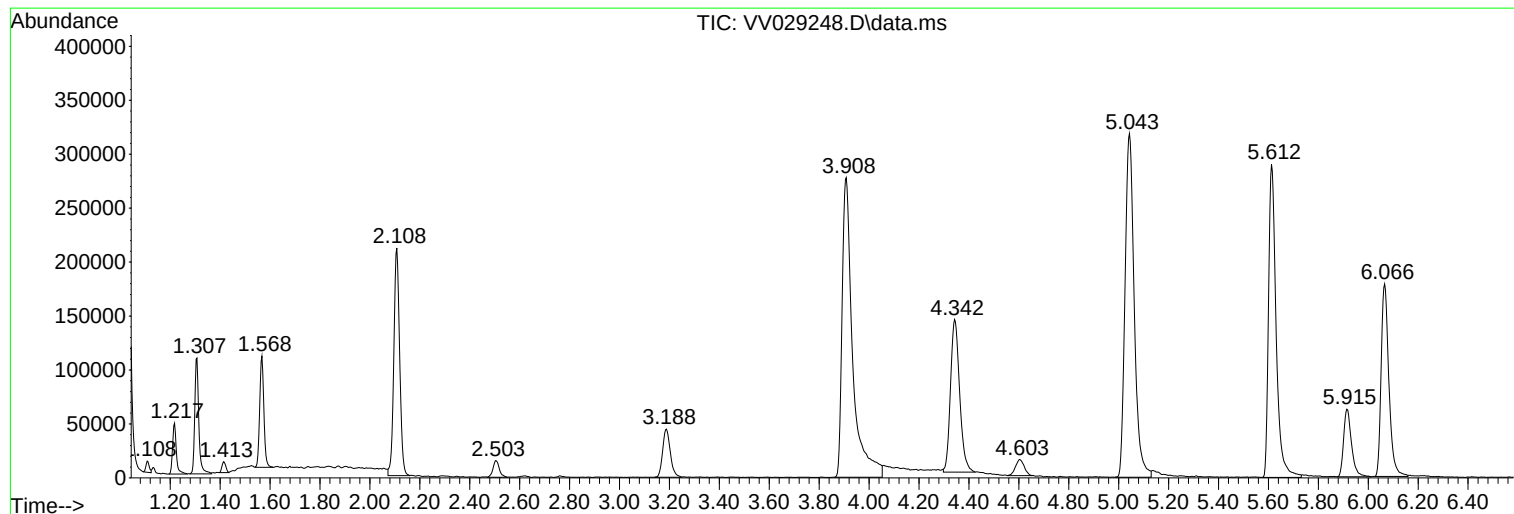

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029248.D
Acq On : 21 Nov 2022 01:22
Operator : SY/MD
Sample : N5666-03DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGXP5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
Data File : VV029248.D
Acq On : 21 Nov 2022 01:22
Operator : SY/MD
Sample : N5666-03DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGXP5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc