
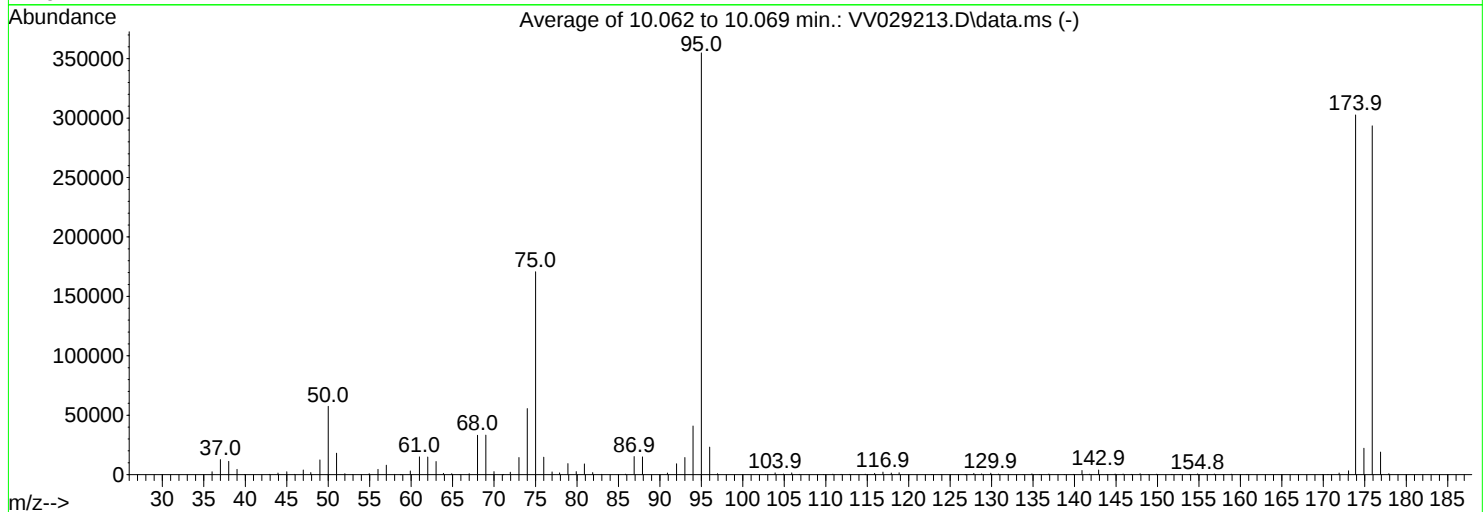


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112022\
 Data File : VV029213.D
 Acq On : 20 Nov 2022 09:52
 Operator : SY/MD
 Sample : BFB202
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB202

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Nov 21 03:37:08 2022

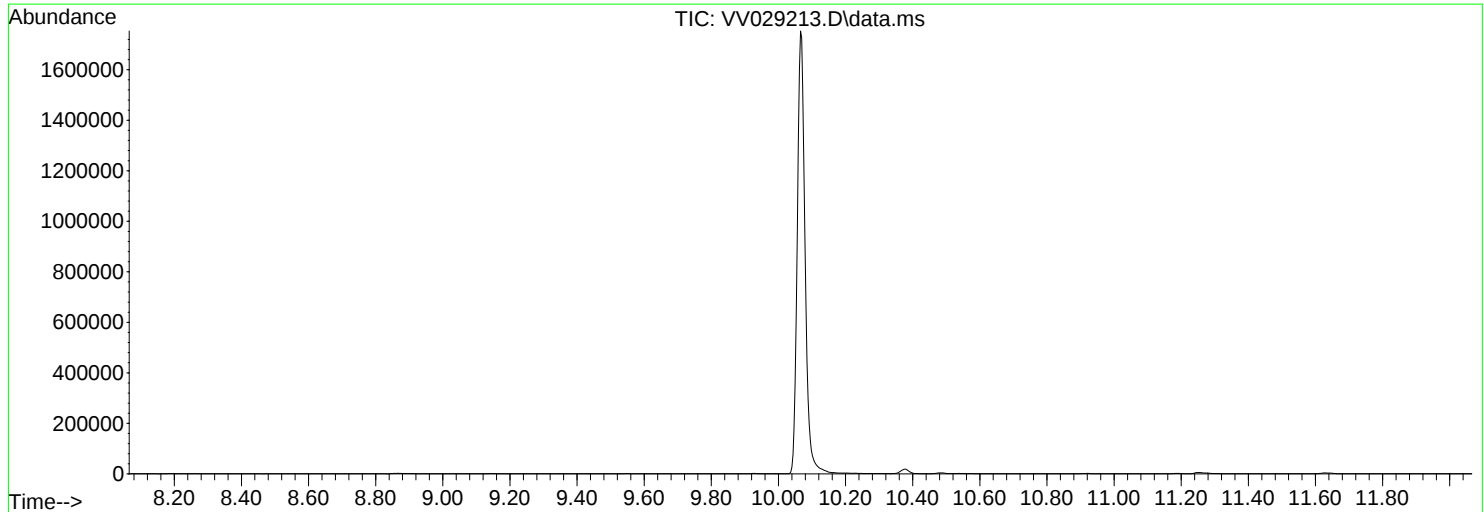

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	57472	PASS
75	95	30	80	48.1	170731	PASS
95	95	100	100	100.0	354923	PASS
96	95	5	9	6.5	23107	PASS
173	174	0.00	2	1.1	3280	PASS
174	95	50	120	85.3	302635	PASS
175	174	5	9	7.3	22187	PASS
176	174	95	105	97.0	293461	PASS
177	176	5	10	6.5	18960	PASS

m/z	Abundance
36.00	2471.0
37.00	12515.0
38.00	11177.0
39.00	4374.0
39.90	375.0
42.90	234.0
44.00	1778.0
45.00	2580.0
46.00	362.0
47.00	3886.0
47.90	1866.0
49.00	12364.0
50.00	57680.0
51.00	18144.0
52.00	874.0
52.90	168.0
54.90	882.0
56.00	4433.0
57.00	7917.0
58.00	351.0
59.90	3198.0
61.00	15280.0
62.00	14916.0
63.00	10973.0
63.90	1025.0
64.90	736.0
65.90	111.0
67.00	742.0
68.00	33184.0
69.00	33240.0
70.00	2363.0
72.00	1980.0
73.00	14184.0
74.00	55616.0
75.00	173632.0
76.00	14328.0
77.00	2344.0
77.90	1471.0
78.90	9631.0
79.90	2662.0
80.90	9205.0
81.90	1835.0
82.90	304.0
85.80	400.0
86.90	15164.0
87.90	15572.0
90.90	1327.0
92.00	9261.0
93.00	14218.0
94.00	42112.0
95.00	359104.0
96.00	23016.0
96.90	733.0
102.80	162.0
103.90	1586.0
104.90	531.0
105.90	1554.0
106.80	275.0
109.70	168.0
110.90	477.0
111.80	277.0
113.00	255.0
114.70	468.0
115.90	1052.0
116.90	2153.0
117.90	1285.0
118.80	1624.0
122.90	126.0
123.90	257.0
126.80	102.0
127.90	1214.0
128.80	780.0
129.90	1246.0
130.90	452.0
133.80	149.0
134.80	659.0
136.90	604.0
138.80	150.0
139.90	315.0
140.90	3738.0
141.80	344.0
142.90	4073.0
143.90	212.0
144.90	501.0
145.80	590.0
146.80	249.0
147.90	850.0
148.90	186.0
149.90	391.0
151.80	192.0
152.70	350.0
153.90	259.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

154.90	620.0
155.90	176.0
156.90	583.0
157.90	117.0
158.90	371.0
160.80	343.0
169.90	175.0
170.50	173.0
171.90	1185.0
173.10	3415.0
173.90	313344.0
174.90	22952.0
175.90	305152.0
176.90	19248.0
177.90	766.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
39.90	257.0
43.80	354.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
36.00	2198.0
37.00	12399.0
38.00	10782.0
39.00	4339.0
40.00	389.0
42.90	221.0
44.00	1626.0
45.00	2272.0
45.90	265.0
47.00	3938.0
47.90	1720.0
49.00	11871.0
50.00	55120.0
51.00	17208.0
52.00	831.0
53.00	144.0
55.00	776.0
56.00	4289.0
57.00	7722.0
58.00	267.0
59.90	2974.0
61.00	14040.0
62.00	14283.0
63.00	10892.0
63.90	1161.0
64.90	905.0
65.90	155.0
67.00	824.0
68.00	31944.0
69.00	32128.0
70.00	2710.0
71.00	107.0
71.90	1924.0
73.00	14102.0
74.00	53824.0
75.00	162176.0
76.00	14593.0
77.00	2087.0
77.90	1493.0
78.90	8597.0
79.90	2472.0
80.90	8678.0
81.90	1675.0
83.00	196.0
85.90	470.0
86.90	14924.0
87.90	13768.0
90.90	1259.0
92.00	8833.0
93.00	14153.0
94.00	38528.0
95.00	338240.0
96.00	22456.0
97.00	771.0
102.80	150.0
103.90	1455.0
104.90	446.0
105.90	1479.0
106.80	326.0
109.80	180.0
110.80	381.0
111.90	250.0
112.80	218.0
114.70	316.0
115.90	1038.0
116.90	2090.0
117.90	1237.0
118.90	1727.0
122.70	138.0
123.90	127.0
127.80	1047.0
128.80	654.0
129.90	1199.0
130.80	511.0
133.80	114.0
134.90	637.0
135.80	175.0
136.90	545.0
138.70	157.0
139.90	293.0
140.90	3242.0
141.80	374.0
142.90	3477.0
143.90	193.0
144.90	519.0
145.90	419.0
146.90	267.0
147.90	795.0
148.90	170.0
149.90	329.0
151.70	226.0
152.80	253.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

153.90	173.0
154.80	684.0
155.90	180.0
156.80	417.0
158.90	388.0
160.80	330.0
170.60	170.0
171.90	1343.0
173.00	3039.0
173.90	281408.0
174.90	20608.0
175.90	271360.0
176.90	17912.0
177.90	688.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
36.00	2527.0
37.00	13057.0
38.00	11618.0
39.00	4540.0
39.90	418.0
42.90	242.0
44.00	1775.0
45.00	2552.0
46.00	338.0
47.00	4066.0
47.90	1843.0
49.00	12884.0
50.00	59616.0
51.00	18680.0
52.00	912.0
52.90	158.0
55.00	896.0
56.00	4598.0
57.00	8257.0
58.00	316.0
58.70	105.0
59.90	3297.0
61.00	15556.0
62.00	15409.0
63.00	11468.0
63.90	1090.0
64.90	825.0
65.90	148.0
67.00	820.0
68.00	34328.0
69.00	34312.0
70.00	2704.0
71.10	118.0
71.90	2057.0
73.00	14805.0
74.00	57480.0
75.00	176384.0
76.00	15273.0
77.00	2334.0
77.90	1544.0
78.90	9635.0
79.90	2675.0
80.90	9337.0
81.90	1825.0
83.00	265.0
85.80	430.0
86.90	15690.0
87.90	15591.0
90.90	1414.0
92.00	9406.0
93.00	15052.0
94.00	42184.0
95.00	367424.0
96.00	23848.0
97.00	802.0
102.70	164.0
103.90	1661.0
104.90	498.0
105.90	1640.0
106.80	333.0
109.80	194.0
110.80	455.0
111.80	266.0
112.90	241.0
114.80	457.0
115.90	1138.0
116.90	2282.0
117.90	1367.0
118.90	1694.0
122.80	140.0
123.90	211.0
127.90	1173.0
128.80	738.0
129.90	1269.0
130.90	532.0
133.80	164.0
134.90	689.0
135.80	155.0
136.90	624.0
138.70	137.0
139.90	324.0
140.90	3613.0
141.80	361.0
142.90	4133.0
143.90	198.0
144.90	566.0
145.80	520.0
146.90	274.0
147.90	912.0
148.90	173.0
149.90	378.0
151.80	238.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

152.70	316.0
153.90	259.0
154.80	686.0
155.90	204.0
156.90	506.0
158.90	411.0
160.80	377.0
169.90	148.0
170.50	177.0
171.90	1371.0
173.10	3387.0
173.90	313152.0
174.90	23000.0
175.90	303872.0
176.90	19720.0
177.90	824.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202