

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
 Data File : VV038213.D
 Acq On : 20 Nov 2024 14:20
 Operator : SY/MD
 Sample : P4882-17DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3J4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038213.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.272	65	72	90	rBV	101019	127962	12.06%	1.357%
2	1.526	143	151	161	rBV	98462	128619	12.12%	1.364%
3	2.044	263	312	367	rVB3	288621	1060986	100.00%	11.250%
4	2.436	424	434	447	rVB3	10142	16608	1.57%	0.176%
5	2.699	505	516	536	rVB4	5332	13021	1.23%	0.138%
6	3.806	851	860	897	rBV	92051	350578	33.04%	3.717%
7	4.240	979	995	1028	rBV2	156527	415560	39.17%	4.406%
8	4.947	1201	1215	1253	rBV2	344900	904964	85.29%	9.595%
9	5.526	1384	1395	1427	rBV	267172	599604	56.51%	6.358%
10	5.825	1477	1488	1519	rBV	325362	691258	65.15%	7.330%
11	5.982	1525	1537	1563	rVB	198646	426621	40.21%	4.524%
12	6.912	1817	1826	1857	rBV2	84437	186351	17.56%	1.976%
13	7.240	1916	1928	1953	rBV	349564	668682	63.02%	7.090%
14	7.558	2017	2027	2049	rBV	51875	112497	10.60%	1.193%
15	7.899	2115	2133	2161	rBV	133154	239916	22.61%	2.544%
16	8.030	2164	2174	2211	rBV	444164	987481	93.07%	10.470%
17	8.780	2395	2407	2436	rBV	460333	816687	76.97%	8.659%
18	10.149	2821	2833	2860	rBV	189458	318904	30.06%	3.381%
19	11.181	3142	3154	3186	rBV	424403	707437	66.68%	7.501%
20	11.554	3255	3270	3297	rBV	384530	657406	61.96%	6.971%




Sum of corrected areas: 9431142

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038213.D
Acq On : 20 Nov 2024 14:20
Operator : SY/MD
Sample : P4882-17DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3J4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

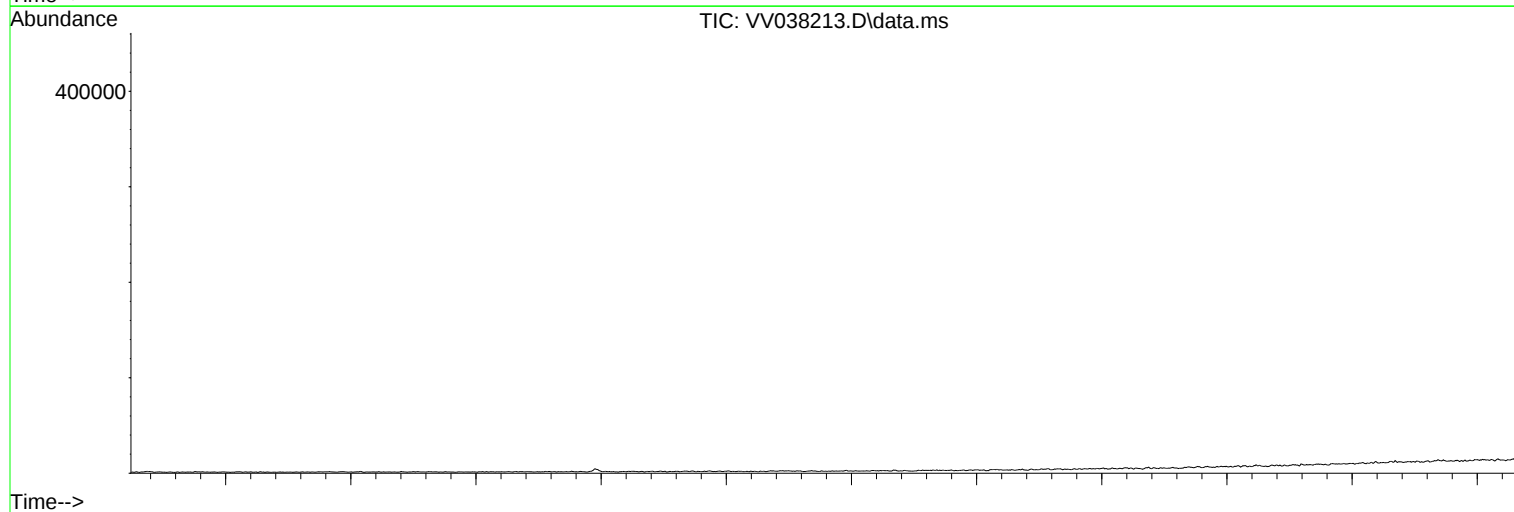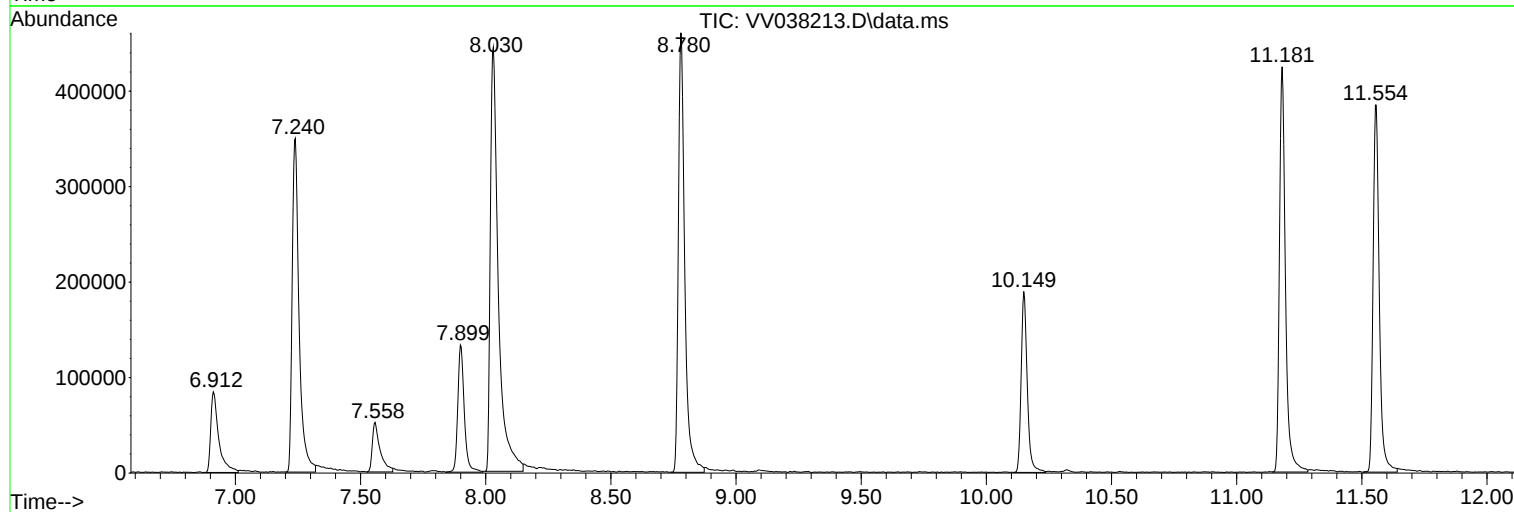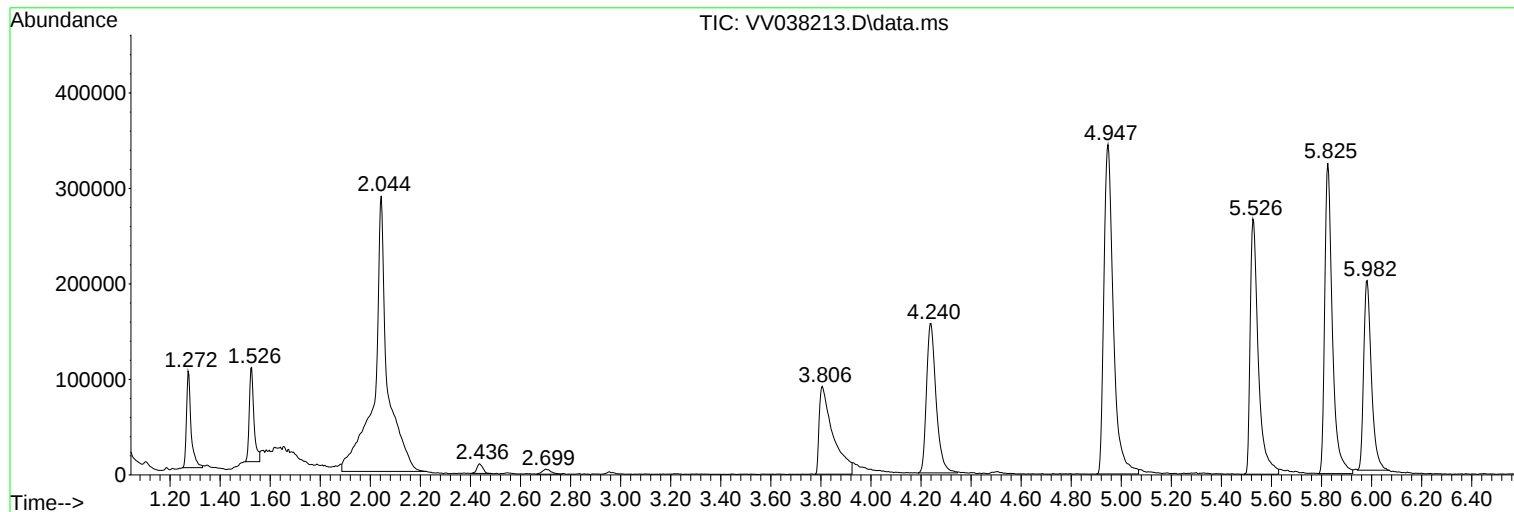

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038213.D
Acq On : 20 Nov 2024 14:20
Operator : SY/MD
Sample : P4882-17DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3J4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038213.D
Acq On : 20 Nov 2024 14:20
Operator : SY/MD
Sample : P4882-17DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3J4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------