

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
 Data File : VV038214.D
 Acq On : 20 Nov 2024 14:44
 Operator : SY/MD
 Sample : P4883-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3J7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038214.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	85	rBV	121147	125451	3.06%	0.996%
2	1.526	144	151	167	rBV	108779	131485	3.21%	1.044%
3	1.828	234	245	273	rBV	2779138	4101690	100.00%	32.554%
4	2.053	306	315	326	rVV	209088	304185	7.42%	2.414%
5	2.442	425	436	453	rVB2	36201	61241	1.49%	0.486%
6	3.780	839	852	904	rBV	115883	386268	9.42%	3.066%
7	4.243	980	996	1026	rBV	151491	406784	9.92%	3.228%
8	4.503	1063	1077	1097	rBV4	20251	53861	1.31%	0.427%
9	4.950	1202	1216	1250	rBV3	322299	865191	21.09%	6.867%
10	5.529	1386	1396	1421	rBV	257740	554866	13.53%	4.404%
11	5.825	1476	1488	1523	rBV	397375	847411	20.66%	6.726%
12	5.982	1526	1537	1560	rBV	195594	415098	10.12%	3.294%
13	6.911	1817	1826	1861	rBV	76894	168763	4.11%	1.339%
14	7.239	1916	1928	1948	rBV	330863	626903	15.28%	4.975%
15	7.558	2014	2027	2042	rBV2	46601	93392	2.28%	0.741%
16	7.902	2122	2134	2154	rVB2	133526	235777	5.75%	1.871%
17	8.017	2161	2170	2209	rBV	430532	893153	21.78%	7.089%
18	8.780	2396	2407	2442	rBV	437851	796122	19.41%	6.319%
19	10.146	2821	2832	2856	rBV2	173773	291316	7.10%	2.312%
20	11.181	3138	3154	3185	rBV	369586	636995	15.53%	5.056%
21	11.554	3257	3270	3294	rBV	353902	603874	14.72%	4.793%




Sum of corrected areas: 12599826

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038214.D
Acq On : 20 Nov 2024 14:44
Operator : SY/MD
Sample : P4883-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

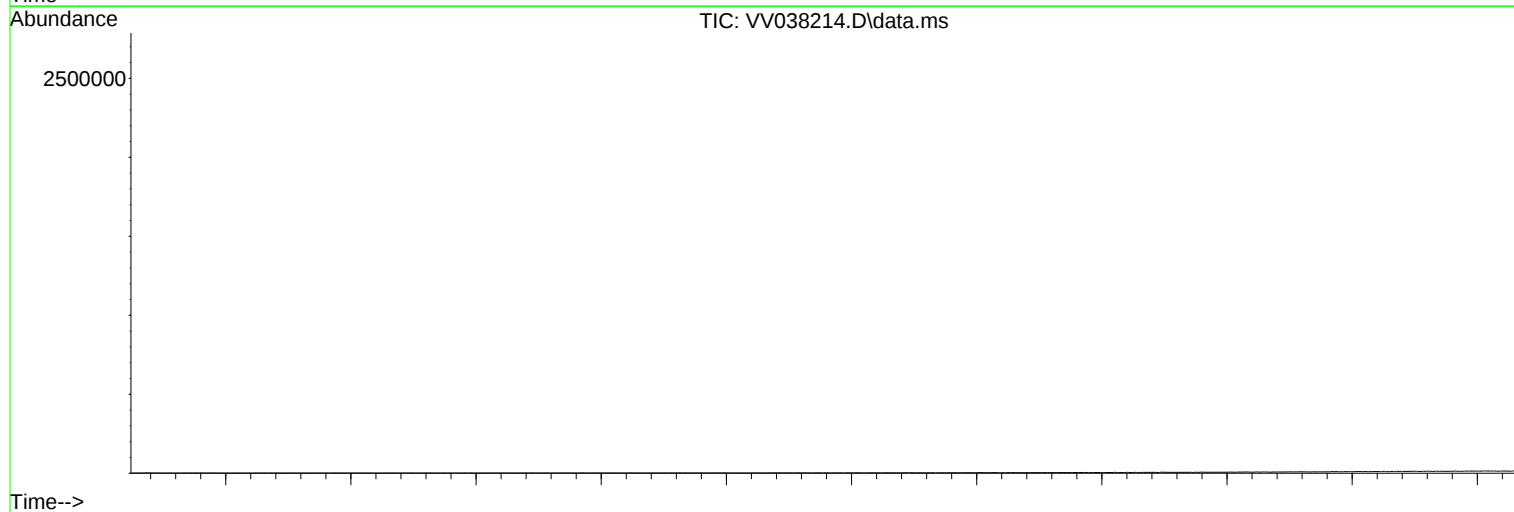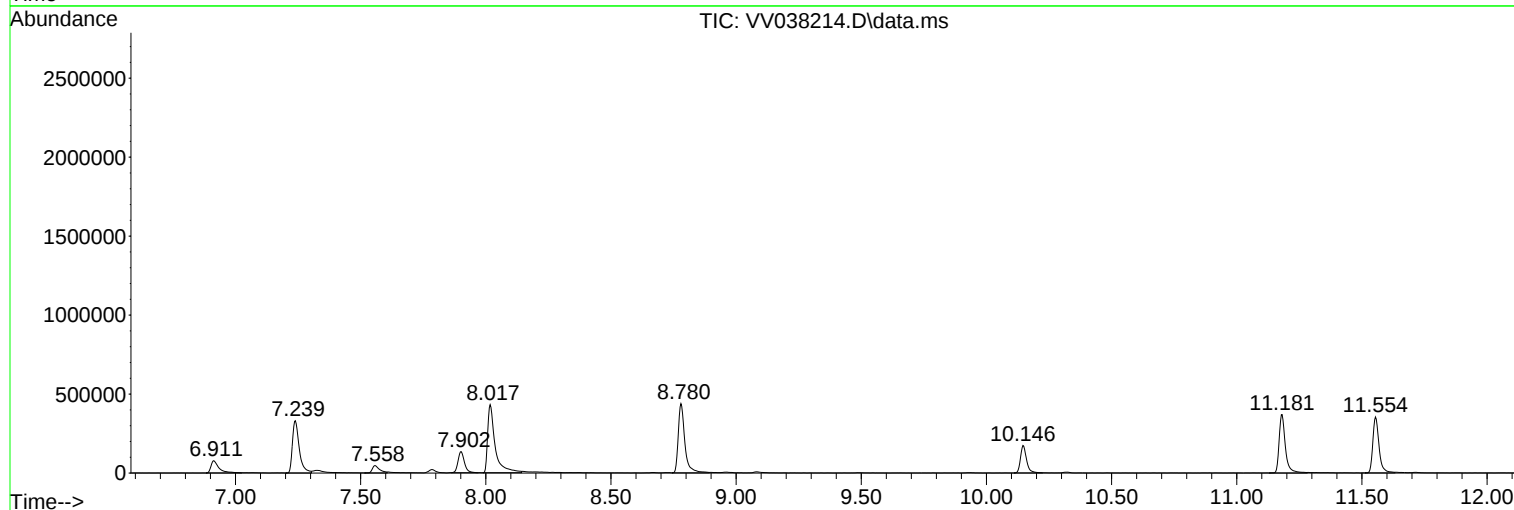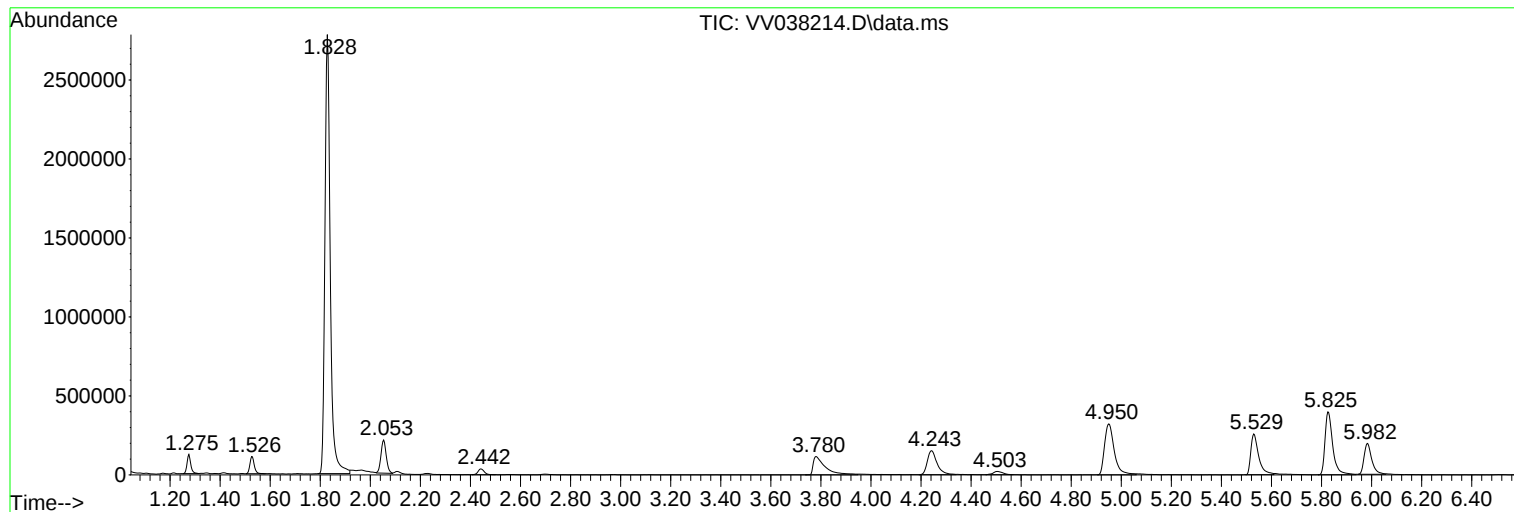

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038214.D
Acq On : 20 Nov 2024 14:44
Operator : SY/MD
Sample : P4883-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038214.D
Acq On : 20 Nov 2024 14:44
Operator : SY/MD
Sample : P4883-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
