

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
 Data File : VV038217.D
 Acq On : 20 Nov 2024 15:57
 Operator : SY/MD
 Sample : P4883-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3K1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038217.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.709	197	208	232	rBV	3279743	4374404	34.67%	12.460%
2	1.834	233	247	306	rVV	8292904	12618632	100.00%	35.944%
3	2.053	306	315	356	rVB3	276850	521595	4.13%	1.486%
4	2.439	423	435	454	rBV	182064	302186	2.39%	0.861%
5	3.802	842	859	903	rBV2	624018	1769092	14.02%	5.039%
6	4.240	978	995	1027	rBV2	142890	390248	3.09%	1.112%
7	4.503	1060	1077	1099	rBV	130865	348065	2.76%	0.991%
8	4.950	1199	1216	1240	rBV3	310179	813310	6.45%	2.317%
9	5.529	1386	1396	1430	rBV	256364	566724	4.49%	1.614%
10	5.821	1474	1487	1525	rBV	3986923	7776385	61.63%	22.151%
11	5.982	1526	1537	1564	rVB2	187829	413244	3.27%	1.177%
12	6.911	1813	1826	1859	rBV2	73125	161700	1.28%	0.461%
13	7.239	1918	1928	1944	rBV	325453	595184	4.72%	1.695%
14	7.317	1944	1952	1970	rVB	74455	152565	1.21%	0.435%
15	7.899	2112	2133	2156	rBV	552970	972936	7.71%	2.771%
16	8.017	2161	2170	2206	rBV	421979	835152	6.62%	2.379%
17	8.780	2397	2407	2442	rBV	445788	870880	6.90%	2.481%
18	10.146	2821	2832	2854	rBV	163582	283643	2.25%	0.808%
19	11.178	3143	3153	3175	rBV	392089	660949	5.24%	1.883%
20	11.554	3248	3270	3301	rBV	357038	679724	5.39%	1.936%

Sum of corrected areas: 35106618




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038217.D
Acq On : 20 Nov 2024 15:57
Operator : SY/MD
Sample : P4883-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3K1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

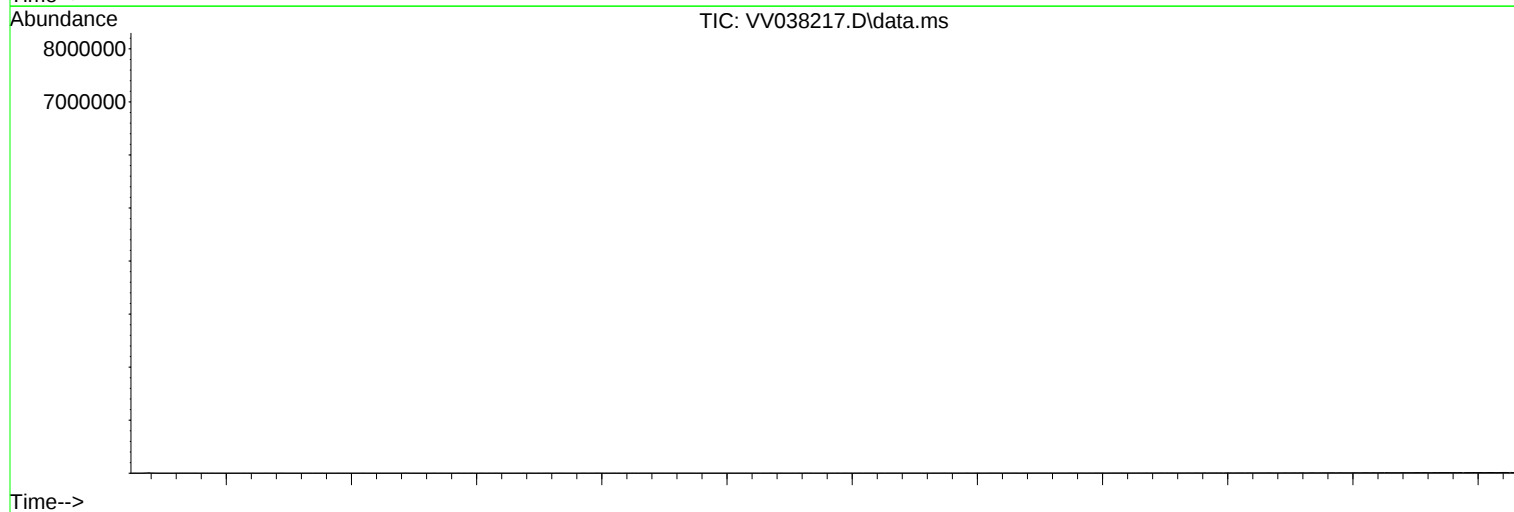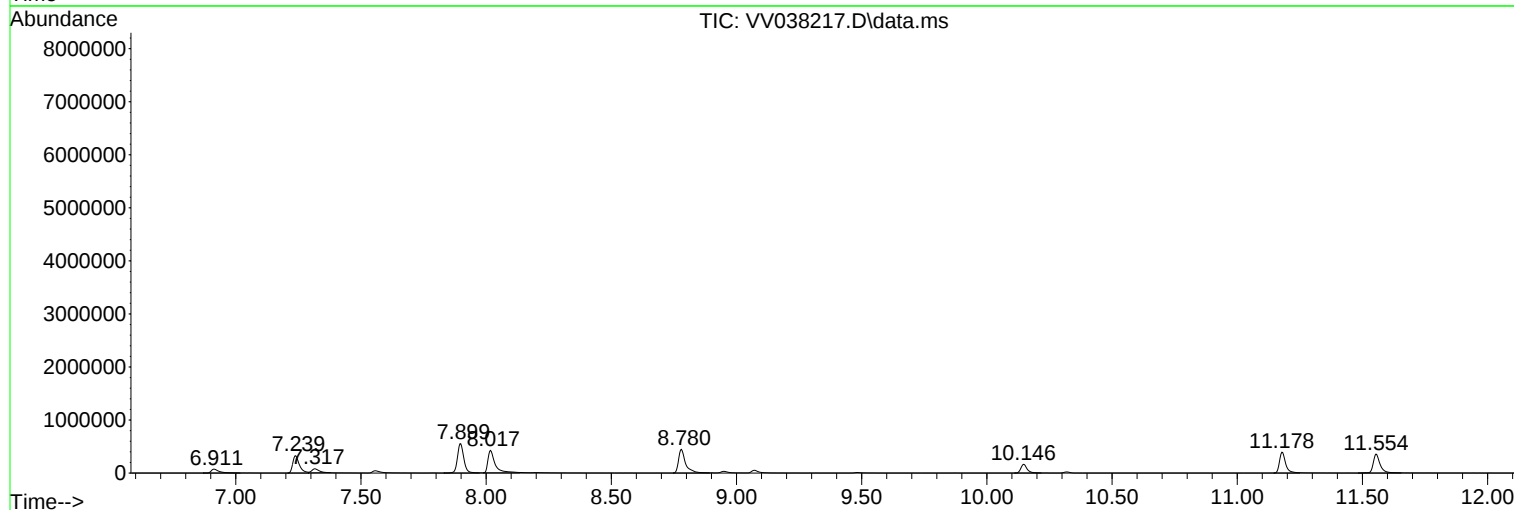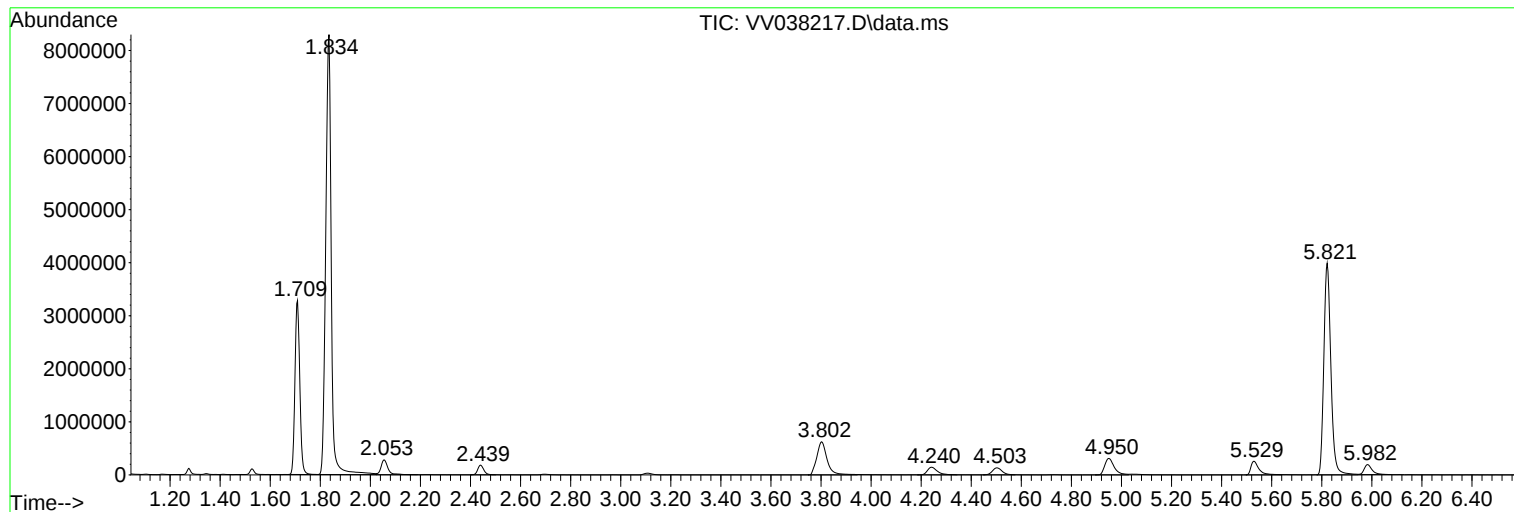

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038217.D
Acq On : 20 Nov 2024 15:57
Operator : SY/MD
Sample : P4883-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3K1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038217.D
Acq On : 20 Nov 2024 15:57
Operator : SY/MD
Sample : P4883-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3K1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc