

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
 Data File : VV038222.D
 Acq On : 20 Nov 2024 17:58
 Operator : SY/MD
 Sample : P4883-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3K6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038222.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	85	rBV	118348	125415	1.87%	0.803%
2	1.529	144	152	168	rBV	113375	135969	2.03%	0.870%
3	1.944	246	281	309	rBV2	1001971	6704690	100.00%	42.910%
4	2.442	426	436	453	rVB	55753	94572	1.41%	0.605%
5	3.796	845	857	893	rBV	105736	352905	5.26%	2.259%
6	4.239	980	995	1025	rBV2	149754	402252	6.00%	2.574%
7	4.506	1058	1078	1102	rBV2	64124	175450	2.62%	1.123%
8	4.950	1202	1216	1250	rBV3	321592	858177	12.80%	5.492%
9	5.529	1386	1396	1431	rBV	253984	565260	8.43%	3.618%
10	5.828	1477	1489	1522	rBV	298411	636098	9.49%	4.071%
11	5.982	1526	1537	1566	rVB2	193036	414152	6.18%	2.651%
12	6.915	1817	1827	1853	rBV	73312	161007	2.40%	1.030%
13	7.239	1914	1928	1946	rBV	336026	624672	9.32%	3.998%
14	7.323	1946	1954	1974	rVB	35471	79893	1.19%	0.511%
15	7.558	2016	2027	2050	rBV2	43527	96059	1.43%	0.615%
16	7.898	2112	2133	2156	rBV	462170	827226	12.34%	5.294%
17	8.021	2162	2171	2219	rBV	424277	920833	13.73%	5.893%
18	8.779	2394	2407	2442	rBV	452281	836106	12.47%	5.351%
19	10.146	2821	2832	2854	rBV	174048	295699	4.41%	1.892%
20	11.178	3143	3153	3185	rBV	391214	667286	9.95%	4.271%
21	11.554	3259	3270	3297	rVB	366882	651148	9.71%	4.167%




Sum of corrected areas: 15624869

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038222.D
Acq On : 20 Nov 2024 17:58
Operator : SY/MD
Sample : P4883-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

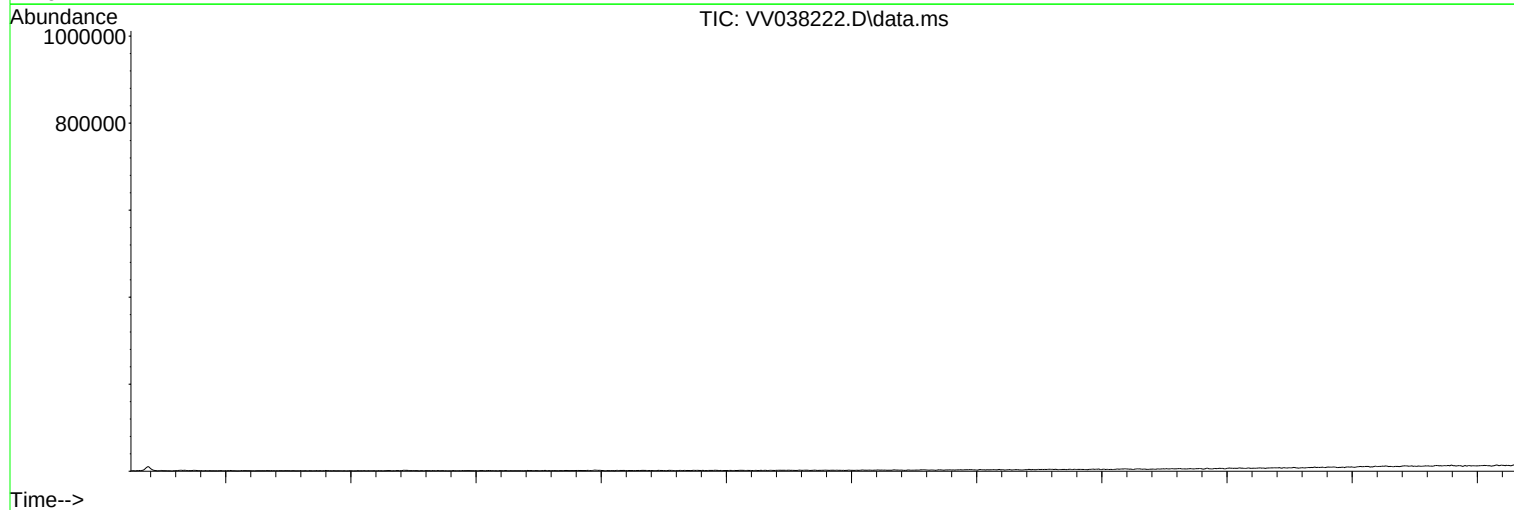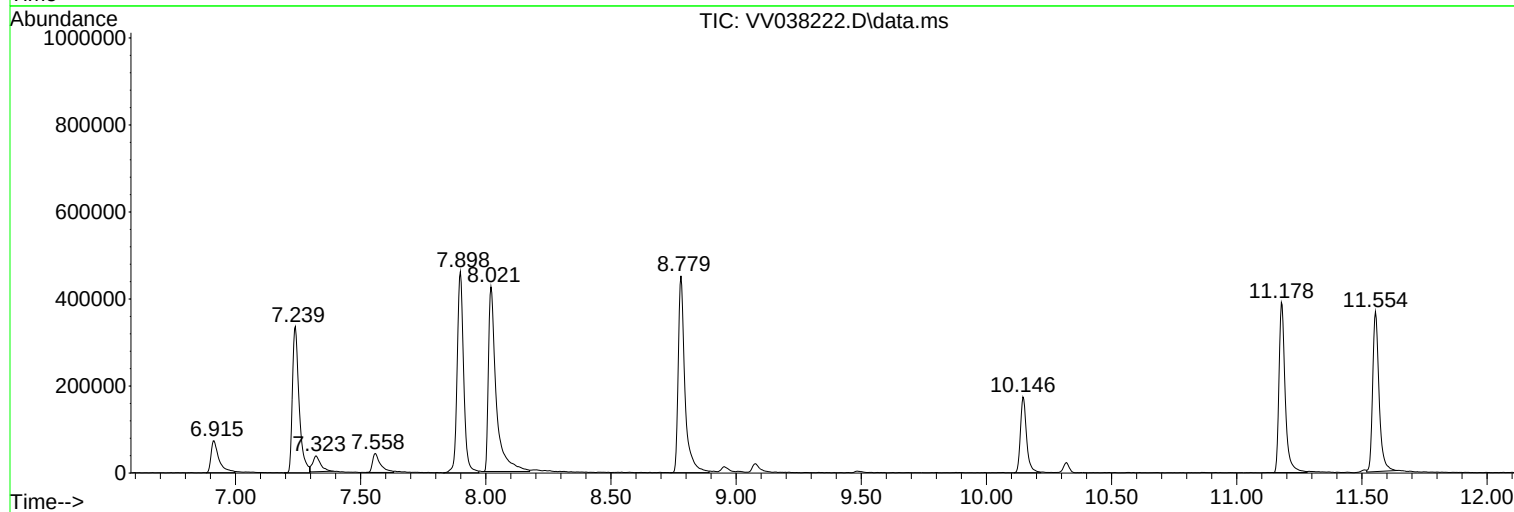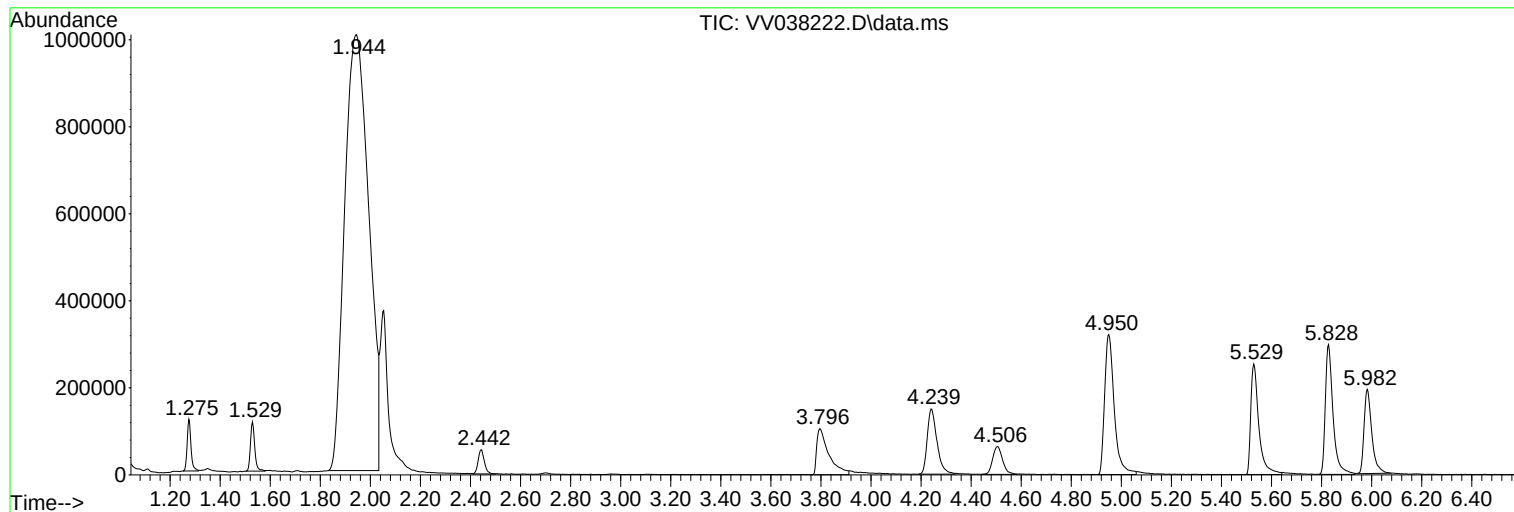

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038222.D
Acq On : 20 Nov 2024 17:58
Operator : SY/MD
Sample : P4883-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038222.D
Acq On : 20 Nov 2024 17:58
Operator : SY/MD
Sample : P4883-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc