

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
 Data File : VV038224.D
 Acq On : 20 Nov 2024 18:46
 Operator : SY/MD
 Sample : P4883-11
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3K8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038224.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	60	73	88	rBV	117107	133228	1.72%	0.861%
2	1.529	144	152	163	rBV	110697	127925	1.65%	0.827%
3	1.941	246	280	309	rBV2	1153869	7740817	100.00%	50.051%
4	3.793	845	856	903	rBV	99564	352713	4.56%	2.281%
5	4.243	979	996	1037	rBV2	146939	402428	5.20%	2.602%
6	4.503	1061	1077	1100	rBV3	44939	118667	1.53%	0.767%
7	4.950	1200	1216	1255	rBV2	312303	838411	10.83%	5.421%
8	5.529	1384	1396	1431	rBV2	266169	592676	7.66%	3.832%
9	5.835	1480	1491	1517	rBV2	63946	150448	1.94%	0.973%
10	5.982	1523	1537	1568	rBV	182592	403566	5.21%	2.609%
11	6.915	1816	1827	1848	rBV2	69270	151196	1.95%	0.978%
12	7.240	1917	1928	1946	rBV	321297	598029	7.73%	3.867%
13	7.558	2017	2027	2060	rBV	43072	97784	1.26%	0.632%
14	7.899	2112	2133	2158	rBV2	208989	393665	5.09%	2.545%
15	8.021	2162	2171	2222	rBV	409675	898630	11.61%	5.810%
16	8.780	2396	2407	2437	rBV	459283	853674	11.03%	5.520%
17	10.146	2818	2832	2853	rBV	166922	283869	3.67%	1.835%
18	11.178	3143	3153	3182	rBV	417194	706637	9.13%	4.569%
19	11.555	3259	3270	3298	rVB	356571	621633	8.03%	4.019%




Sum of corrected areas: 15465996

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038224.D
Acq On : 20 Nov 2024 18:46
Operator : SY/MD
Sample : P4883-11
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3K8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

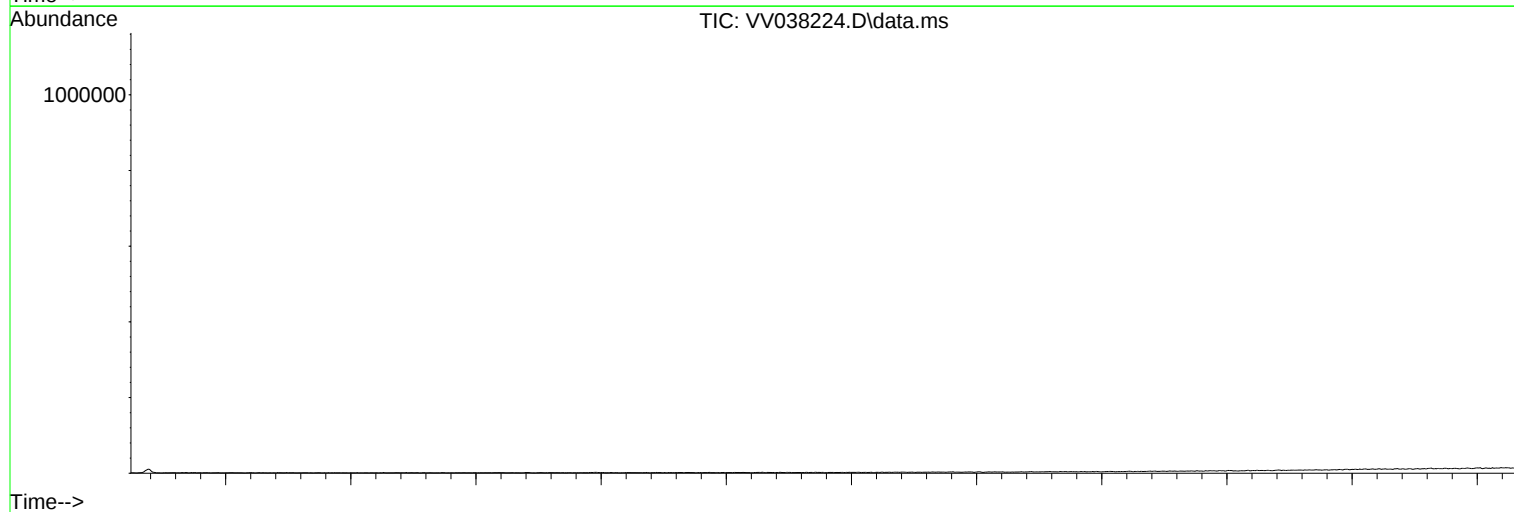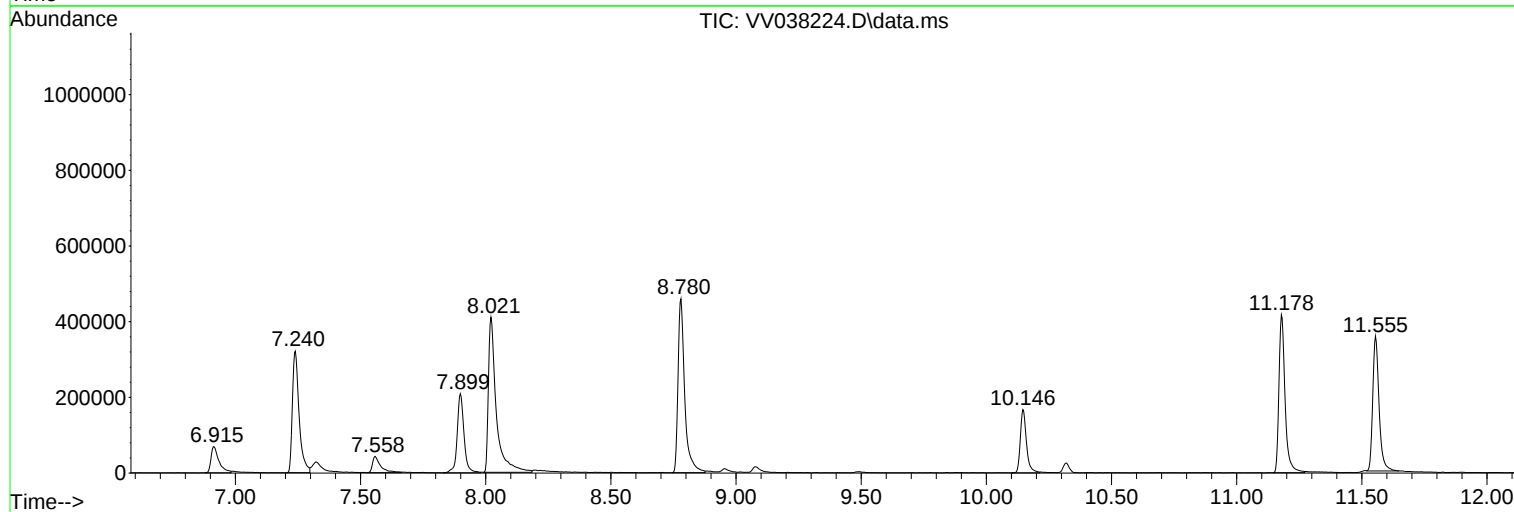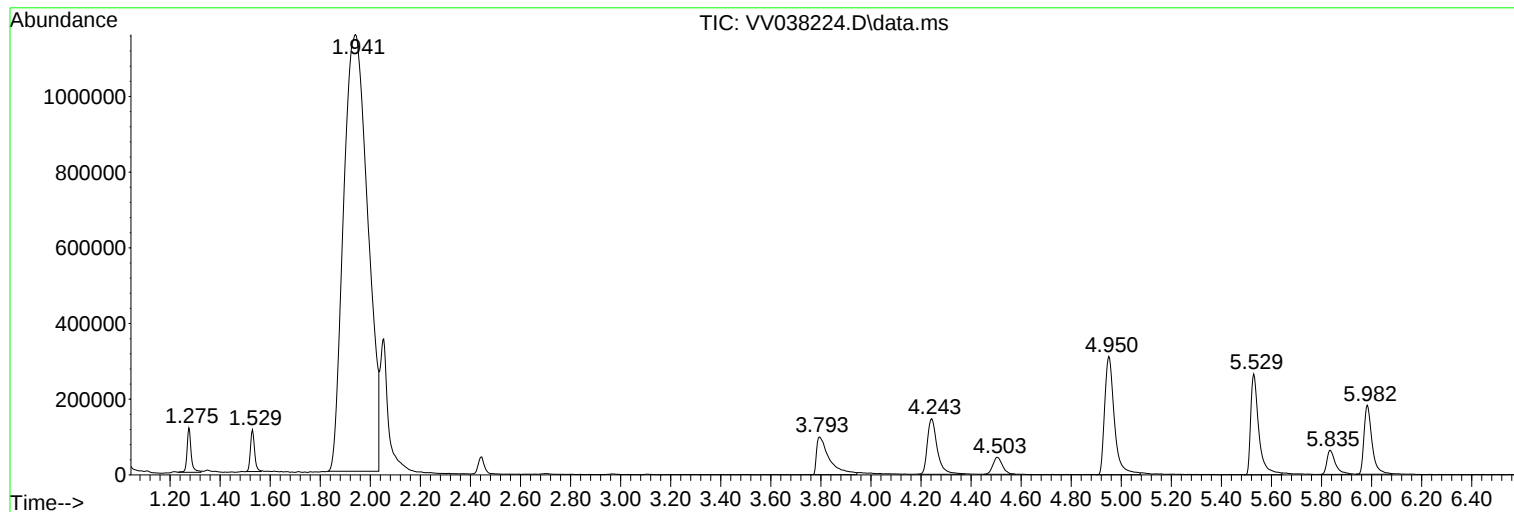

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038224.D
Acq On : 20 Nov 2024 18:46
Operator : SY/MD
Sample : P4883-11
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3K8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038224.D
Acq On : 20 Nov 2024 18:46
Operator : SY/MD
Sample : P4883-11
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3K8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
