

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
 Data File : VV038225.D
 Acq On : 20 Nov 2024 19:10
 Operator : SY/MD
 Sample : VIBLK402
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK402

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038225.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	61	73	89	rBV	136997	154997	18.69%	2.221%
2	1.529	144	152	164	rBV	116364	137451	16.57%	1.970%
3	2.053	305	315	334	rVB	225565	334994	40.39%	4.801%
4	3.802	851	859	888	rBV	80577	264987	31.95%	3.798%
5	4.243	976	996	1024	rBV2	148929	397113	47.88%	5.691%
6	4.950	1202	1216	1258	rBV3	313228	829457	100.00%	11.887%
7	5.529	1384	1396	1447	rBV	245441	559249	67.42%	8.015%
8	5.841	1485	1493	1509	rVB	4501	10286	1.24%	0.147%
9	5.982	1520	1537	1562	rBV	184506	404914	48.82%	5.803%
10	6.915	1817	1827	1862	rBV2	68463	155468	18.74%	2.228%
11	7.239	1914	1928	1958	rBV	326282	627834	75.69%	8.997%
12	7.558	2017	2027	2057	rBV2	40428	93393	11.26%	1.338%
13	7.866	2111	2123	2132	rBV3	7786	14253	1.72%	0.204%
14	8.024	2163	2172	2209	rBV	318851	731955	88.25%	10.490%
15	8.779	2393	2407	2437	rBV	417232	740433	89.27%	10.611%
16	10.146	2819	2832	2860	rBV	158607	271329	32.71%	3.888%
17	10.320	2877	2886	2899	rVB3	15735	24786	2.99%	0.355%
18	11.178	3142	3153	3183	rBV	364683	627471	75.65%	8.992%
19	11.554	3258	3270	3298	rBV	351707	589205	71.04%	8.444%
20	12.191	3457	3468	3479	rVB3	4802	8345	1.01%	0.120%

Sum of corrected areas: 6977920




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038225.D
Acq On : 20 Nov 2024 19:10
Operator : SY/MD
Sample : VIBLK402
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK402

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

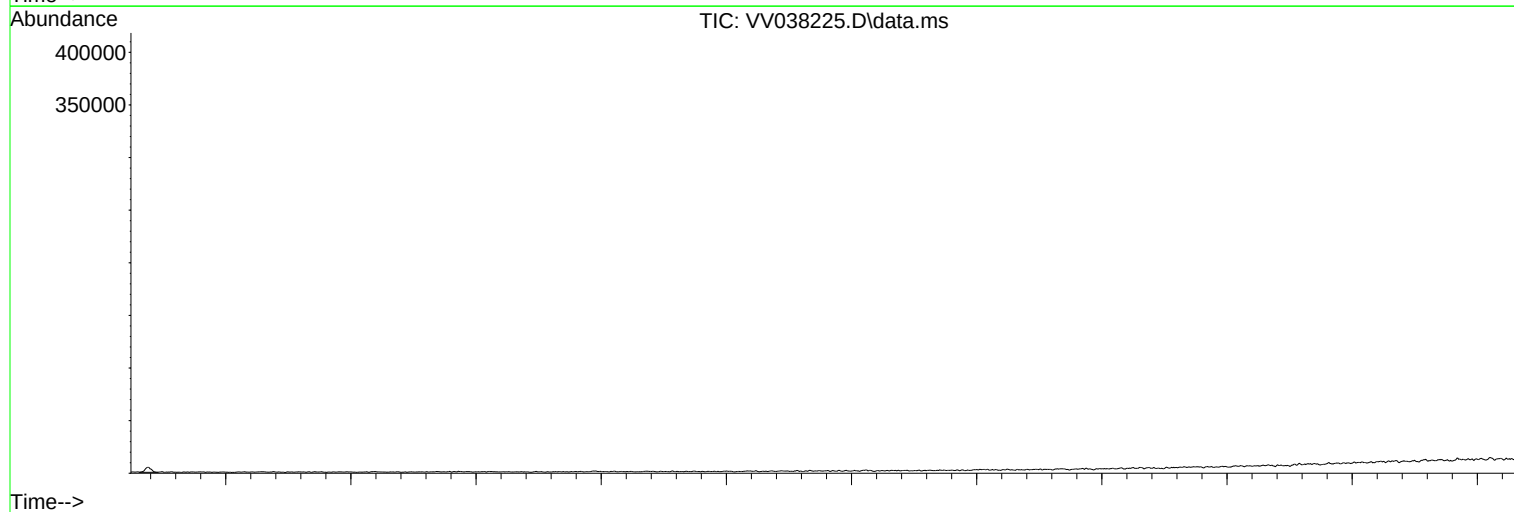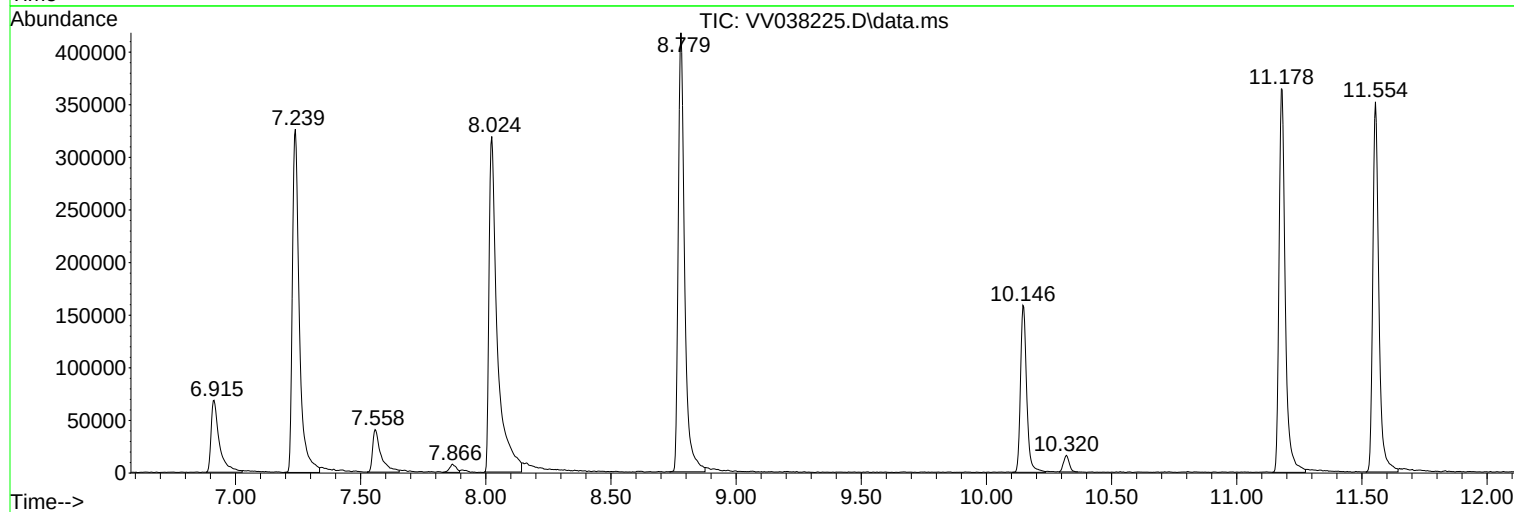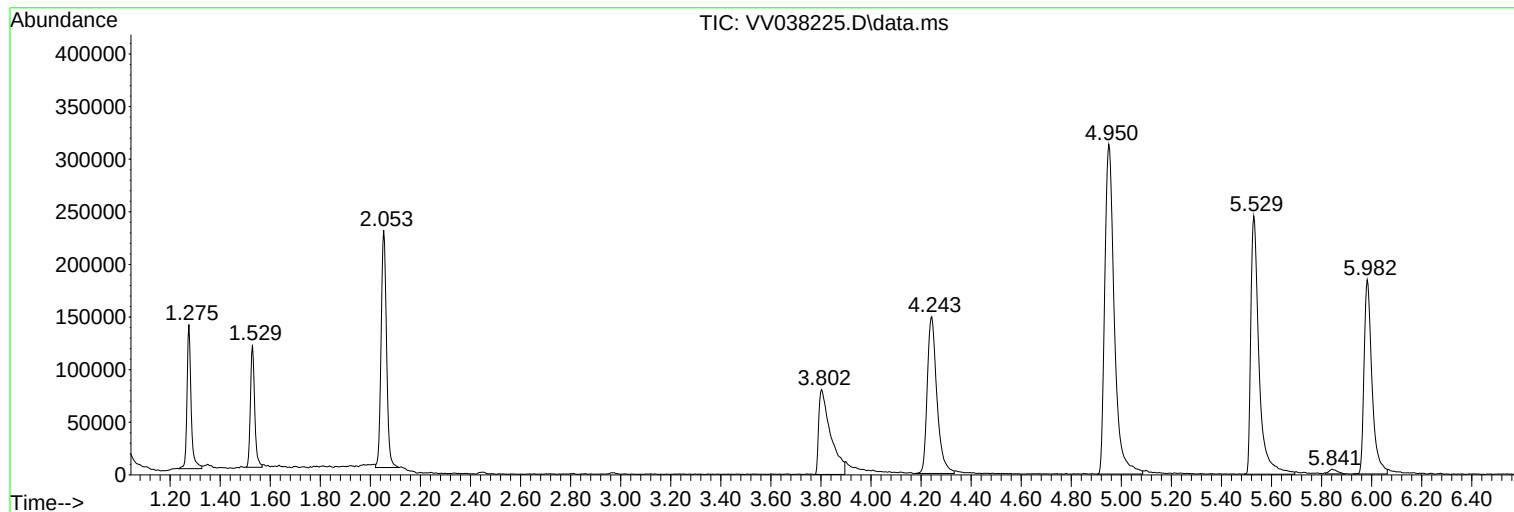

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038225.D
Acq On : 20 Nov 2024 19:10
Operator : SY/MD
Sample : VIBLK402
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK402

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038225.D
Acq On : 20 Nov 2024 19:10
Operator : SY/MD
Sample : VIBLK402
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK402

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
