
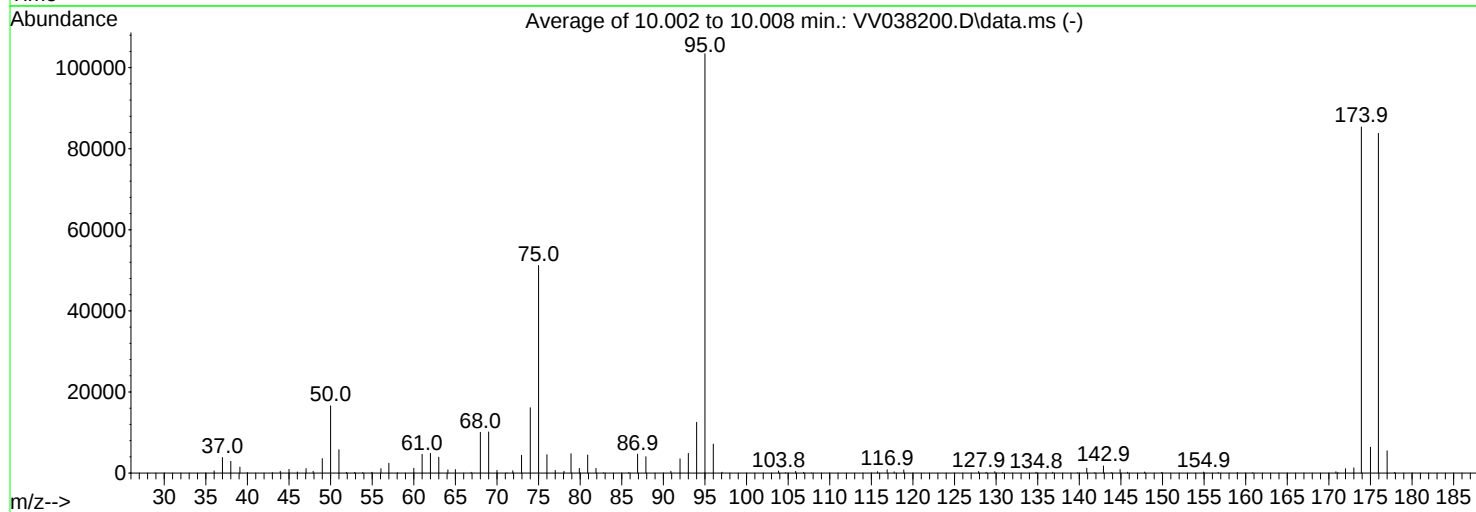


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112024\
Data File : VV038200.D
Acq On : 20 Nov 2024 08:06
Operator : SY/MD
Sample : BFB288
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB288

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Nov 25 00:21:44 2024

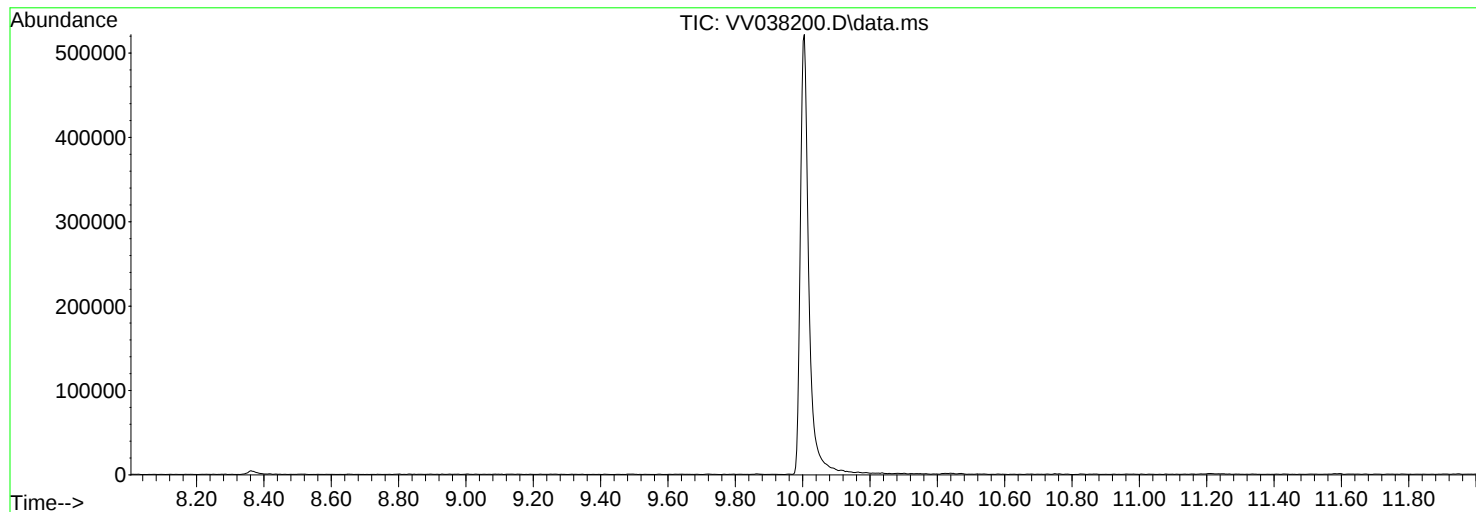

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	16592	PASS
75	95	30	80	49.5	51211	PASS
95	95	100	100	100.0	103429	PASS
96	95	5	9	6.9	7164	PASS
173	174	0.00	2	1.5	1311	PASS
174	95	50	120	82.5	85365	PASS
175	174	5	9	7.5	6381	PASS
176	174	95	105	98.1	83784	PASS
177	176	5	10	6.6	5509	PASS

Scan 2775 (9.963 min): VV038200.D\data.ms
BFB288

m/z	Abundance
39.90	377.0
44.00	457.0

Instrument :
MSVOA_V
ClientSampleId :
BFB288

m/z	Abundance
36.00	601.0
37.00	3942.0
38.00	2934.0
39.10	1598.0
39.80	382.0
44.00	1019.0
45.00	980.0
46.10	337.0
47.00	1096.0
48.00	477.0
49.00	3766.0
50.00	16880.0
51.00	5797.0
51.90	168.0
52.90	208.0
53.80	136.0
54.90	224.0
56.00	1089.0
57.00	2385.0
58.10	125.0
60.00	1150.0
61.00	4620.0
62.00	4892.0
63.00	4219.0
64.10	834.0
65.00	843.0
66.90	129.0
68.00	10285.0
69.00	10067.0
70.00	753.0
71.20	108.0
71.90	649.0
73.00	4585.0
74.00	16408.0
75.00	53024.0
76.00	4453.0
77.00	681.0
78.10	409.0
78.90	4893.0
79.90	1226.0
80.90	4583.0
81.90	1171.0
82.80	121.0
85.90	187.0
86.90	5065.0
87.90	4364.0
90.90	507.0
92.00	3509.0
93.00	4823.0
94.00	12818.0
95.00	105760.0
96.00	7677.0
97.00	248.0
103.80	563.0
104.70	115.0
105.90	431.0
106.80	153.0
115.80	357.0
116.90	967.0
117.70	365.0
118.90	780.0
127.90	464.0
128.90	222.0
129.80	294.0
130.90	158.0
134.80	169.0
136.80	186.0
139.80	118.0
140.90	1307.0
141.90	132.0
142.90	1883.0
143.80	105.0
144.90	926.0
145.70	235.0
147.80	301.0
149.90	200.0
154.90	238.0
156.70	108.0
160.80	156.0
170.80	355.0
172.00	978.0
173.00	1277.0
173.90	86256.0
175.00	6762.0
176.00	82904.0
177.00	5604.0
178.00	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB288

m/z	Abundance
36.00	566.0
37.00	3908.0
38.00	3048.0
39.10	1527.0
39.80	361.0
43.00	109.0
43.90	938.0
45.00	976.0
46.00	290.0
47.10	1143.0
47.90	453.0
49.00	3696.0
50.00	17136.0
51.00	6012.0
51.90	192.0
52.90	200.0
53.80	125.0
54.90	218.0
56.10	1095.0
57.00	2450.0
58.00	104.0
60.00	1277.0
61.00	4779.0
62.00	4934.0
63.00	3978.0
64.10	840.0
65.00	877.0
66.90	235.0
68.00	10450.0
69.00	10446.0
70.00	707.0
71.90	598.0
72.90	4444.0
74.00	16576.0
75.00	52784.0
76.00	4716.0
77.00	700.0
78.10	457.0
78.90	5012.0
79.90	1113.0
80.90	4633.0
81.90	1187.0
82.80	108.0
85.80	166.0
86.90	4711.0
87.90	4149.0
90.90	507.0
92.00	3755.0
93.00	5116.0
94.00	12946.0
95.00	106800.0
96.00	7376.0
97.10	231.0
103.90	485.0
104.70	120.0
105.90	451.0
106.90	173.0
115.70	370.0
116.90	843.0
117.70	314.0
118.90	797.0
127.90	374.0
128.80	203.0
129.80	363.0
130.80	130.0
134.80	223.0
136.80	224.0
139.80	109.0
140.90	1250.0
141.80	104.0
142.90	1786.0
143.80	104.0
144.90	940.0
145.80	215.0
147.90	259.0
149.90	196.0
154.90	287.0
156.70	138.0
159.00	167.0
160.80	102.0
170.80	361.0
172.00	1090.0
173.00	1343.0
173.90	87992.0
175.00	6522.0
176.00	86752.0
177.00	5761.0
177.90	174.0

Instrument :
MSVOA_V
ClientSampleId :
BFB288

m/z	Abundance
36.00	526.0
37.00	3663.0
38.00	2739.0
39.10	1319.0
40.00	294.0
43.00	142.0
43.90	767.0
45.00	872.0
45.90	201.0
47.00	1129.0
47.80	434.0
49.00	3223.0
50.00	15759.0
51.00	5487.0
51.90	217.0
52.90	151.0
53.90	104.0
55.00	176.0
56.00	1111.0
57.00	2469.0
60.00	1164.0
61.00	4493.0
62.00	4794.0
63.00	3557.0
64.10	705.0
65.00	862.0
66.90	253.0
68.00	9438.0
69.00	9882.0
70.00	607.0
71.90	468.0
72.90	4173.0
74.00	15367.0
75.00	47824.0
76.00	4452.0
77.00	669.0
77.90	458.0
78.90	4487.0
79.90	1099.0
80.90	4173.0
81.90	1111.0
85.80	135.0
86.90	4236.0
87.90	3609.0
90.90	373.0
92.00	3283.0
93.00	4636.0
94.00	11812.0
95.00	97728.0
96.00	6438.0
97.10	176.0
103.90	436.0
104.70	117.0
105.90	420.0
106.90	178.0
107.80	121.0
115.80	340.0
116.90	706.0
117.80	284.0
118.90	744.0
127.90	329.0
128.70	164.0
129.90	443.0
130.70	108.0
134.80	267.0
136.80	231.0
140.90	1062.0
142.90	1594.0
143.90	135.0
144.90	851.0
145.90	174.0
147.90	224.0
149.90	152.0
155.00	281.0
156.70	132.0
159.00	217.0
170.90	315.0
171.10	327.0
172.00	1168.0
173.00	1312.0
173.90	81848.0
175.00	5858.0
175.90	81696.0
177.00	5162.0
177.80	158.0

Instrument :
MSVOA_V
ClientSampleId :
BFB288