

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112222\
 Data File : VV029272.D
 Acq On : 22 Nov 2022 19:20
 Operator : SY/MD
 Sample : VV1122WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK274

Quant Time: Nov 23 01:46:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 23 01:46:18 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	292296	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	259446	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	118413	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	143190	5.136	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 102.800%		
7) Chloroethane-d5	1.565	69	112224	5.142	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 102.800%		
11) 1,1-Dichloroethene-d2	2.101	63	188117	3.961	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 79.200%		
20) 2-Butanone-d5	3.918	46	222403	54.038	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 108.080%		
24) Chloroform-d	4.339	84	198865	5.029	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 100.600%		
26) 1,2-Dichloroethane-d4	5.024	65	101462	5.425	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 108.600%		
32) Benzene-d6	5.040	84	453305	5.359	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 107.200%		
36) 1,2-Dichloropropane-d6	6.063	67	146675	5.488	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 109.800%		
41) Toluene-d8	7.307	98	395770	5.193	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 103.800%		
43) trans-1,3-Dichloroprop...	7.616	79	45738	5.140	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 102.800%		
46) 2-Hexanone-d5	8.088	63	105091	65.877	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 131.760%#		
56) 1,1,2,2-Tetrachloroeth...	10.207	84	72127	5.429	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 108.600%		
66) 1,2-Dichlorobenzene-d4	11.616	152	120418	5.271	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 105.400%		
Target Compounds						Qvalue
16) Methylene chloride	2.500	84	9112	0.268	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112222\
Data File : VV029272.D
Acq On : 22 Nov 2022 19:20
Operator : SY/MD
Sample : VV1122WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK274


Quant Time: Nov 23 01:46:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 23 01:46:18 2022
Response via : Initial Calibration

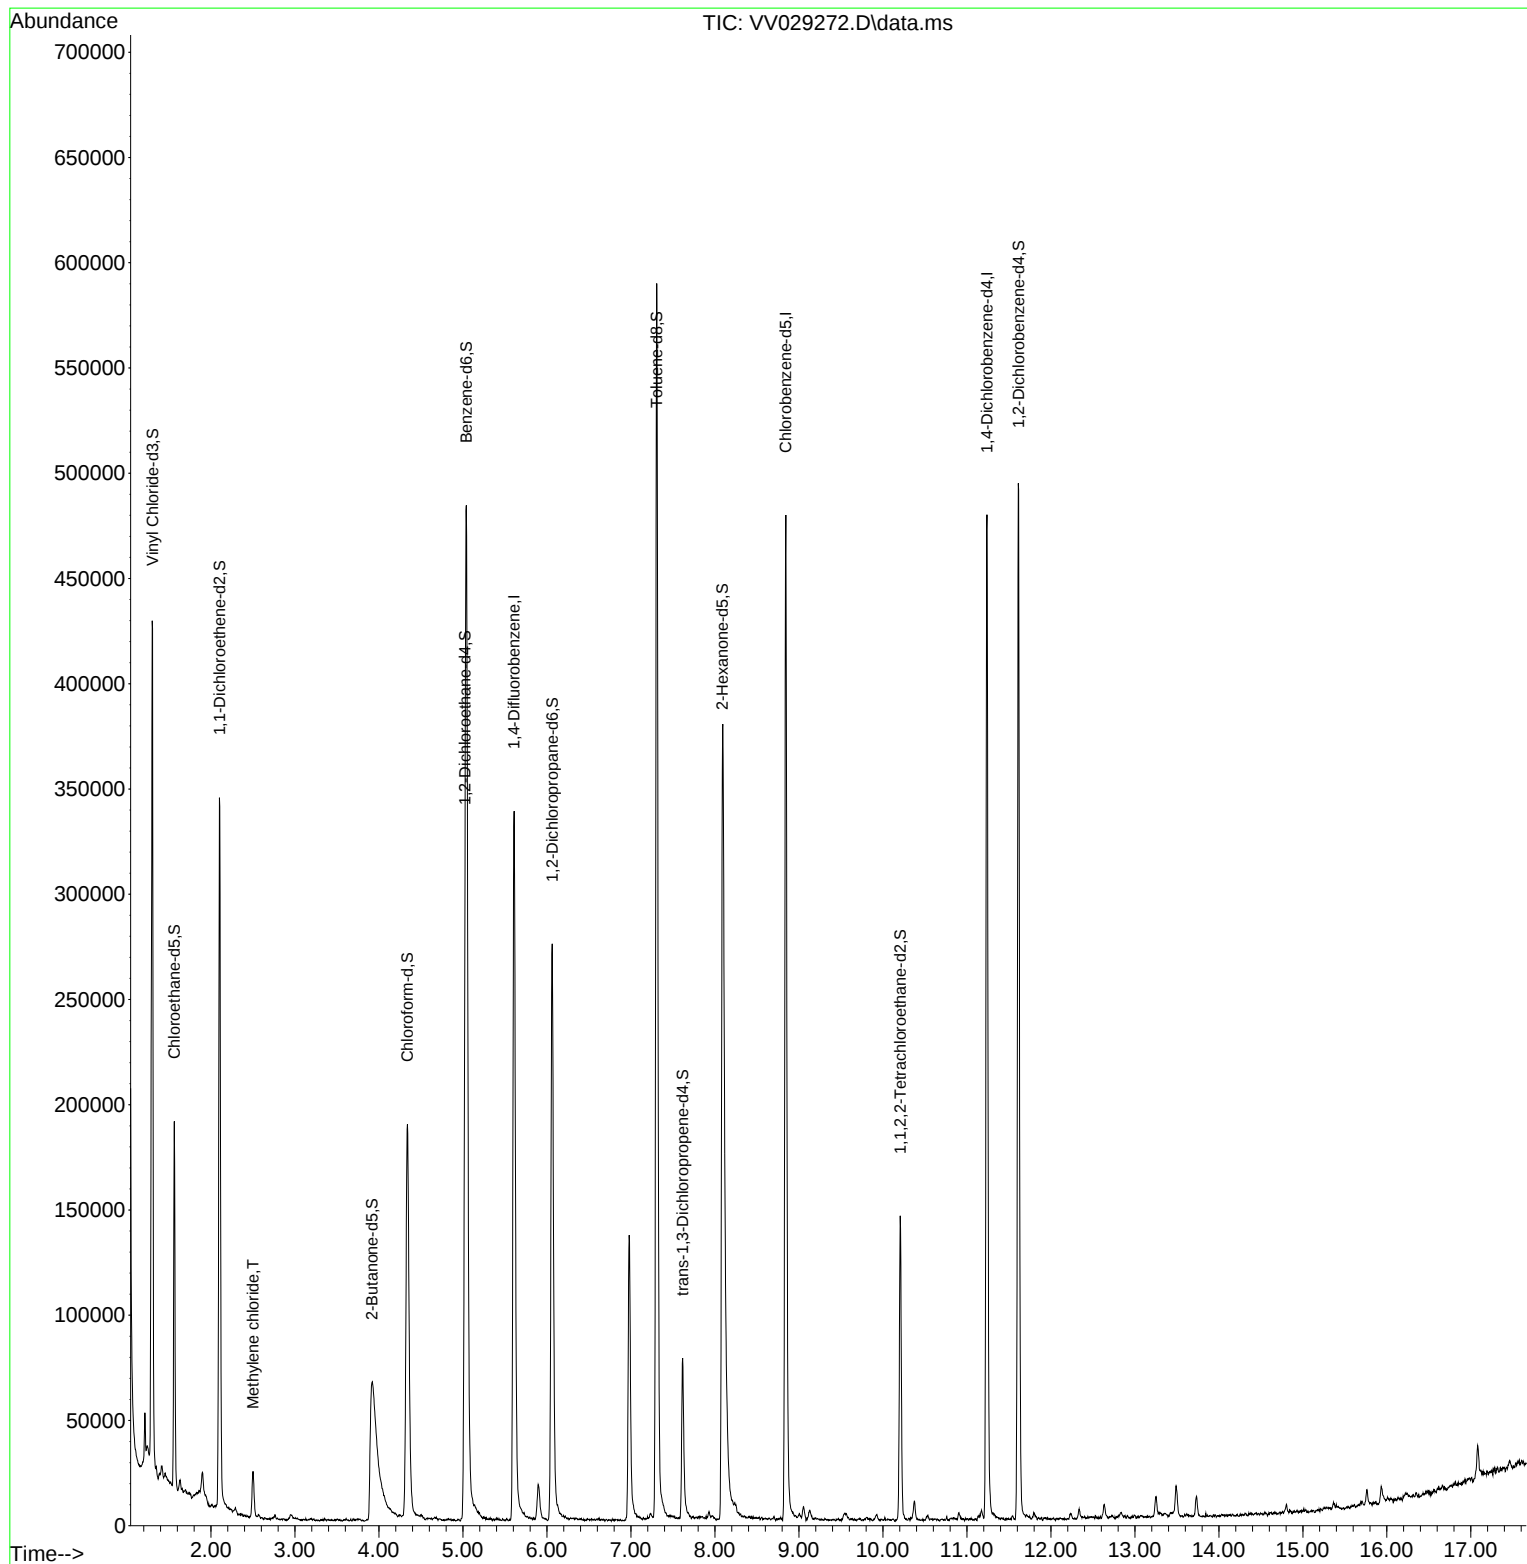

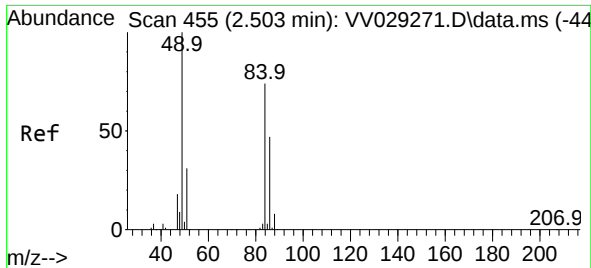

#16
Methylene chloride
Concen: 0.268 ug/L
RT: 2.500 min Scan# 41
Delta R.T. -0.003 min
Lab File: VV029272.D
Acq: 22 Nov 2022 19:20

Instrument :
MSVOA_V
ClientSampleId :
VBLK274

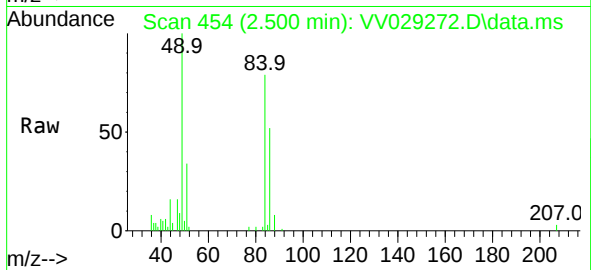

Tgt Ion: 84 Resp: 9112
Ion Ratio Lower Upper
84 100
86 66.5 44.2 82.2
49 126.8 91.9 170.7

