

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112222\
 Data File : VV029274.D
 Acq On : 22 Nov 2022 20:09
 Operator : SY/MD
 Sample : N5666-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 23 04:45:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 23 01:46:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	298224	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	266151	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	121325	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	147173	5.174	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	103.400%	
7) Chloroethane-d5	1.564	69	113174	5.082	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	101.600%	
11) 1,1-Dichloroethene-d2	2.101	63	187197	3.863	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	77.200%	
20) 2-Butanone-d5	3.915	46	218340	51.996	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	104.000%	
24) Chloroform-d	4.339	84	196589	4.873	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.400%	
26) 1,2-Dichloroethane-d4	5.027	65	101998	5.345	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	107.000%	
32) Benzene-d6	5.043	84	445225	5.131	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.600%	
36) 1,2-Dichloropropane-d6	6.063	67	144184	5.259	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	105.200%	
41) Toluene-d8	7.307	98	387678	4.959	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	99.200%	
43) trans-1,3-Dichloroprop...	7.616	79	44205	4.842	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	96.800%	
46) 2-Hexanone-d5	8.088	63	115691	70.694	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	141.380%#	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	73892	5.421	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	108.400%	
66) 1,2-Dichlorobenzene-d4	11.616	152	121419	5.188	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	103.800%	
Target Compounds						
16) Methylene chloride	2.500	84	14440	0.417	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112222\
Data File : VV029274.D
Acq On : 22 Nov 2022 20:09
Operator : SY/MD
Sample : N5666-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Nov 23 04:45:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 23 01:46:18 2022
Response via : Initial Calibration

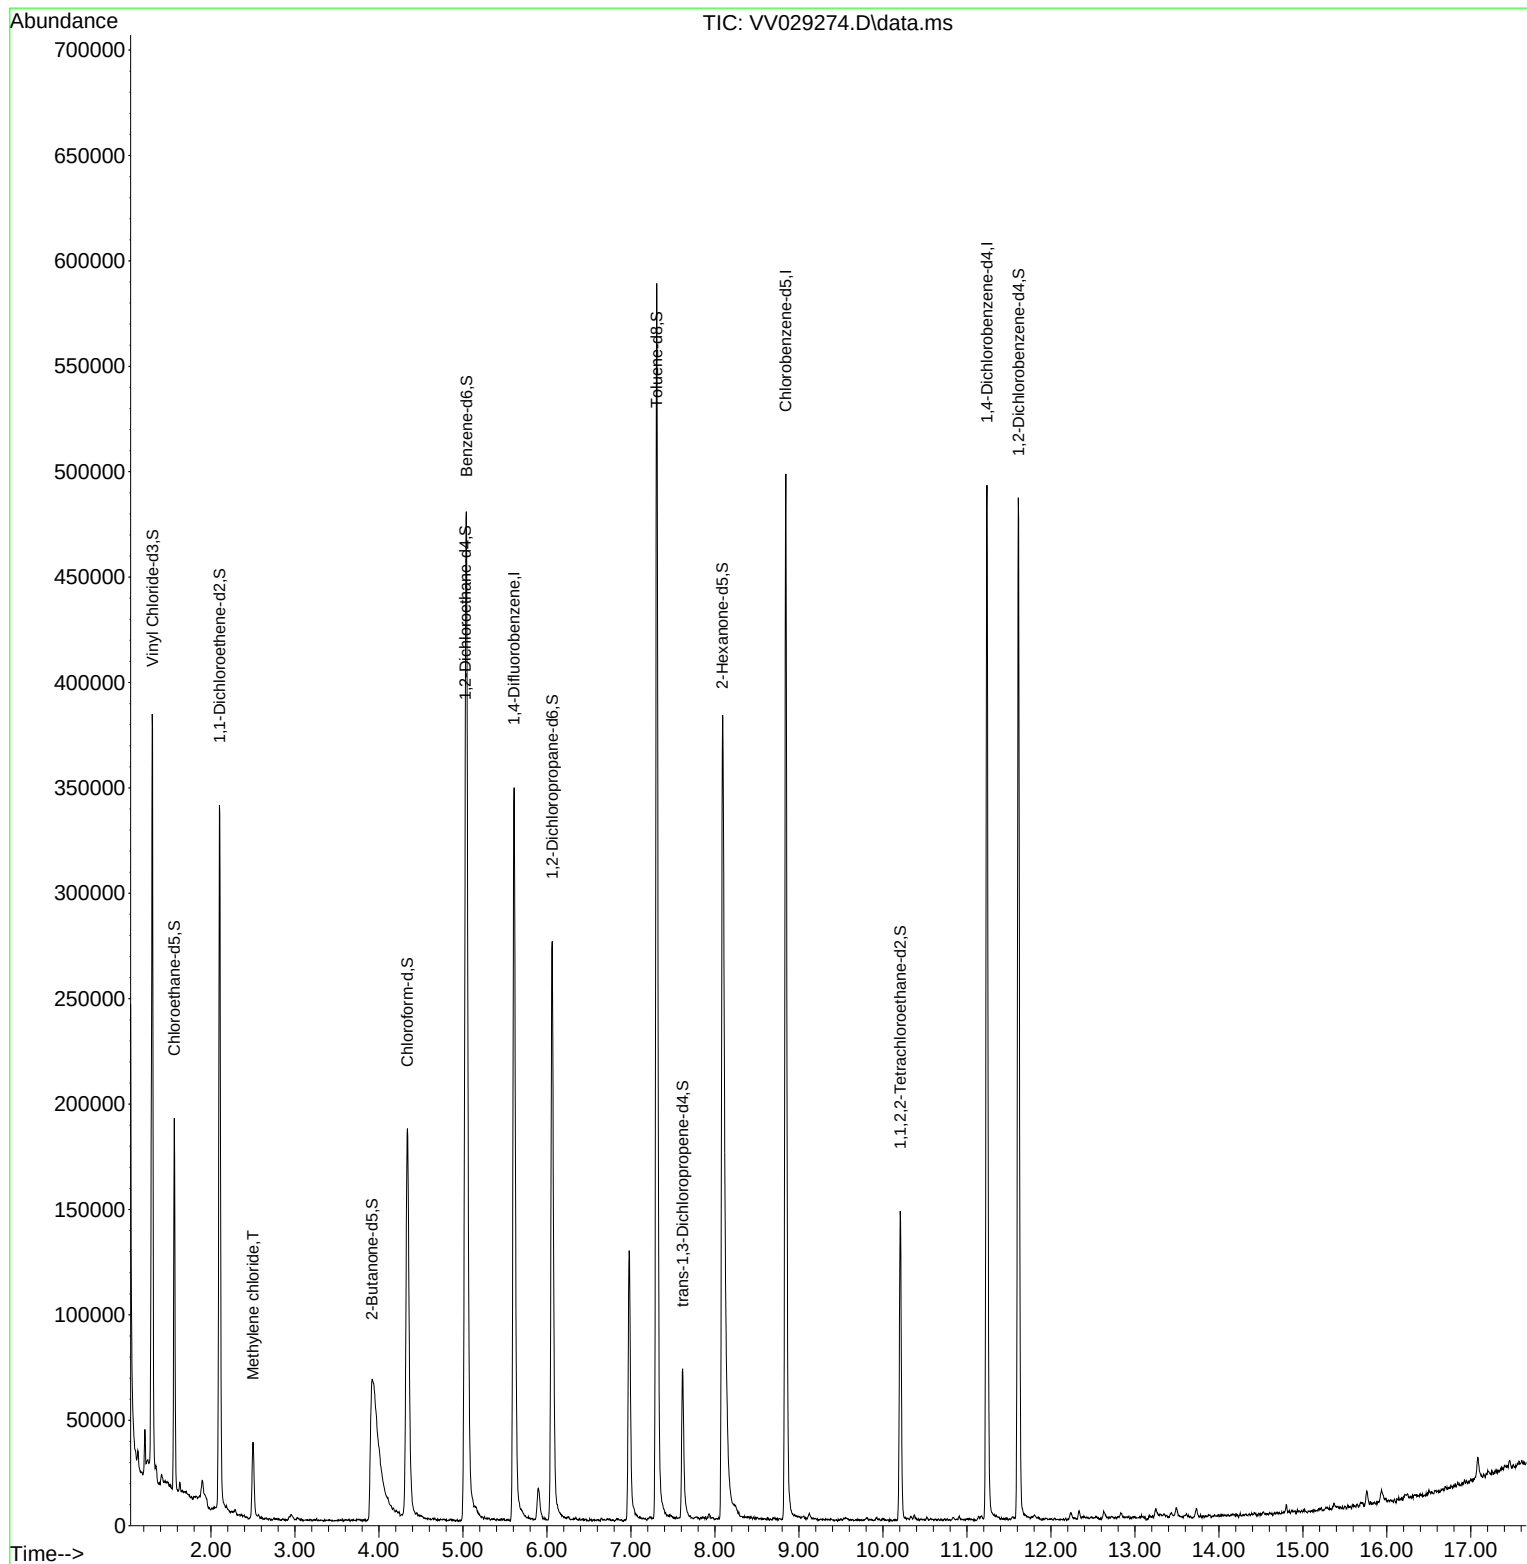

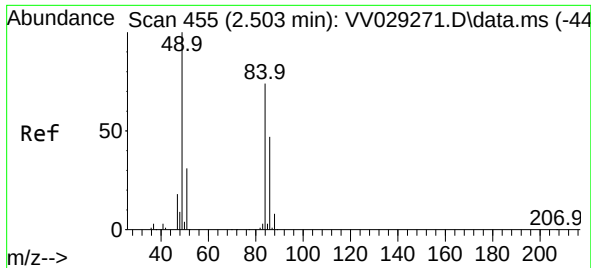

#16
Methylene chloride
Concen: 0.417 ug/L
RT: 2.500 min Scan# 41
Delta R.T. -0.003 min
Lab File: VV029274.D
Acq: 22 Nov 2022 20:09

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

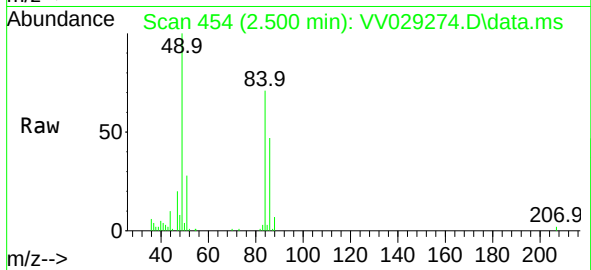

Tgt Ion: 84 Resp: 14440
Ion Ratio Lower Upper
84 100
86 66.8 44.2 82.2
49 141.7 91.9 170.7

