

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112222\
 Data File : VW029279.D
 Acq On : 22 Nov 2022 22:11
 Operator : SY/MD
 Sample : N5651-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1M7

Quant Time: Nov 23 04:47:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 23 01:46:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	298188	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	263154	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	121525	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	92773	3.262	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	65.200%
7) Chloroethane-d5	1.564	69	81528	3.662	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	73.200%
11) 1,1-Dichloroethene-d2	2.105	63	114410	2.361	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	47.200%#
20) 2-Butanone-d5	3.892	46	222365	52.961	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.920%
24) Chloroform-d	4.339	84	157416	3.902	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.000%
26) 1,2-Dichloroethane-d4	5.024	65	82664	4.333	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.600%
32) Benzene-d6	5.043	84	319198	3.720	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	74.400%
36) 1,2-Dichloropropane-d6	6.063	67	113763	4.197	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.000%
41) Toluene-d8	7.310	98	255038	3.299	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	66.000%#
43) trans-1,3-Dichloroprop...	7.616	79	32123	3.559	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	71.200%
46) 2-Hexanone-d5	8.085	63	83341	51.506	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.020%
56) 1,1,2,2-Tetrachloroeth...	10.207	84	60815	4.513	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.200%
66) 1,2-Dichlorobenzene-d4	11.615	152	92591	3.949	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	79.000%#
Target Compounds						
13) Acetone	2.182	43	59869	17.189	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112222\
Data File : VV029279.D
Acq On : 22 Nov 2022 22:11
Operator : SY/MD
Sample : N5651-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1M7

Quant Time: Nov 23 04:47:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 23 01:46:18 2022
Response via : Initial Calibration

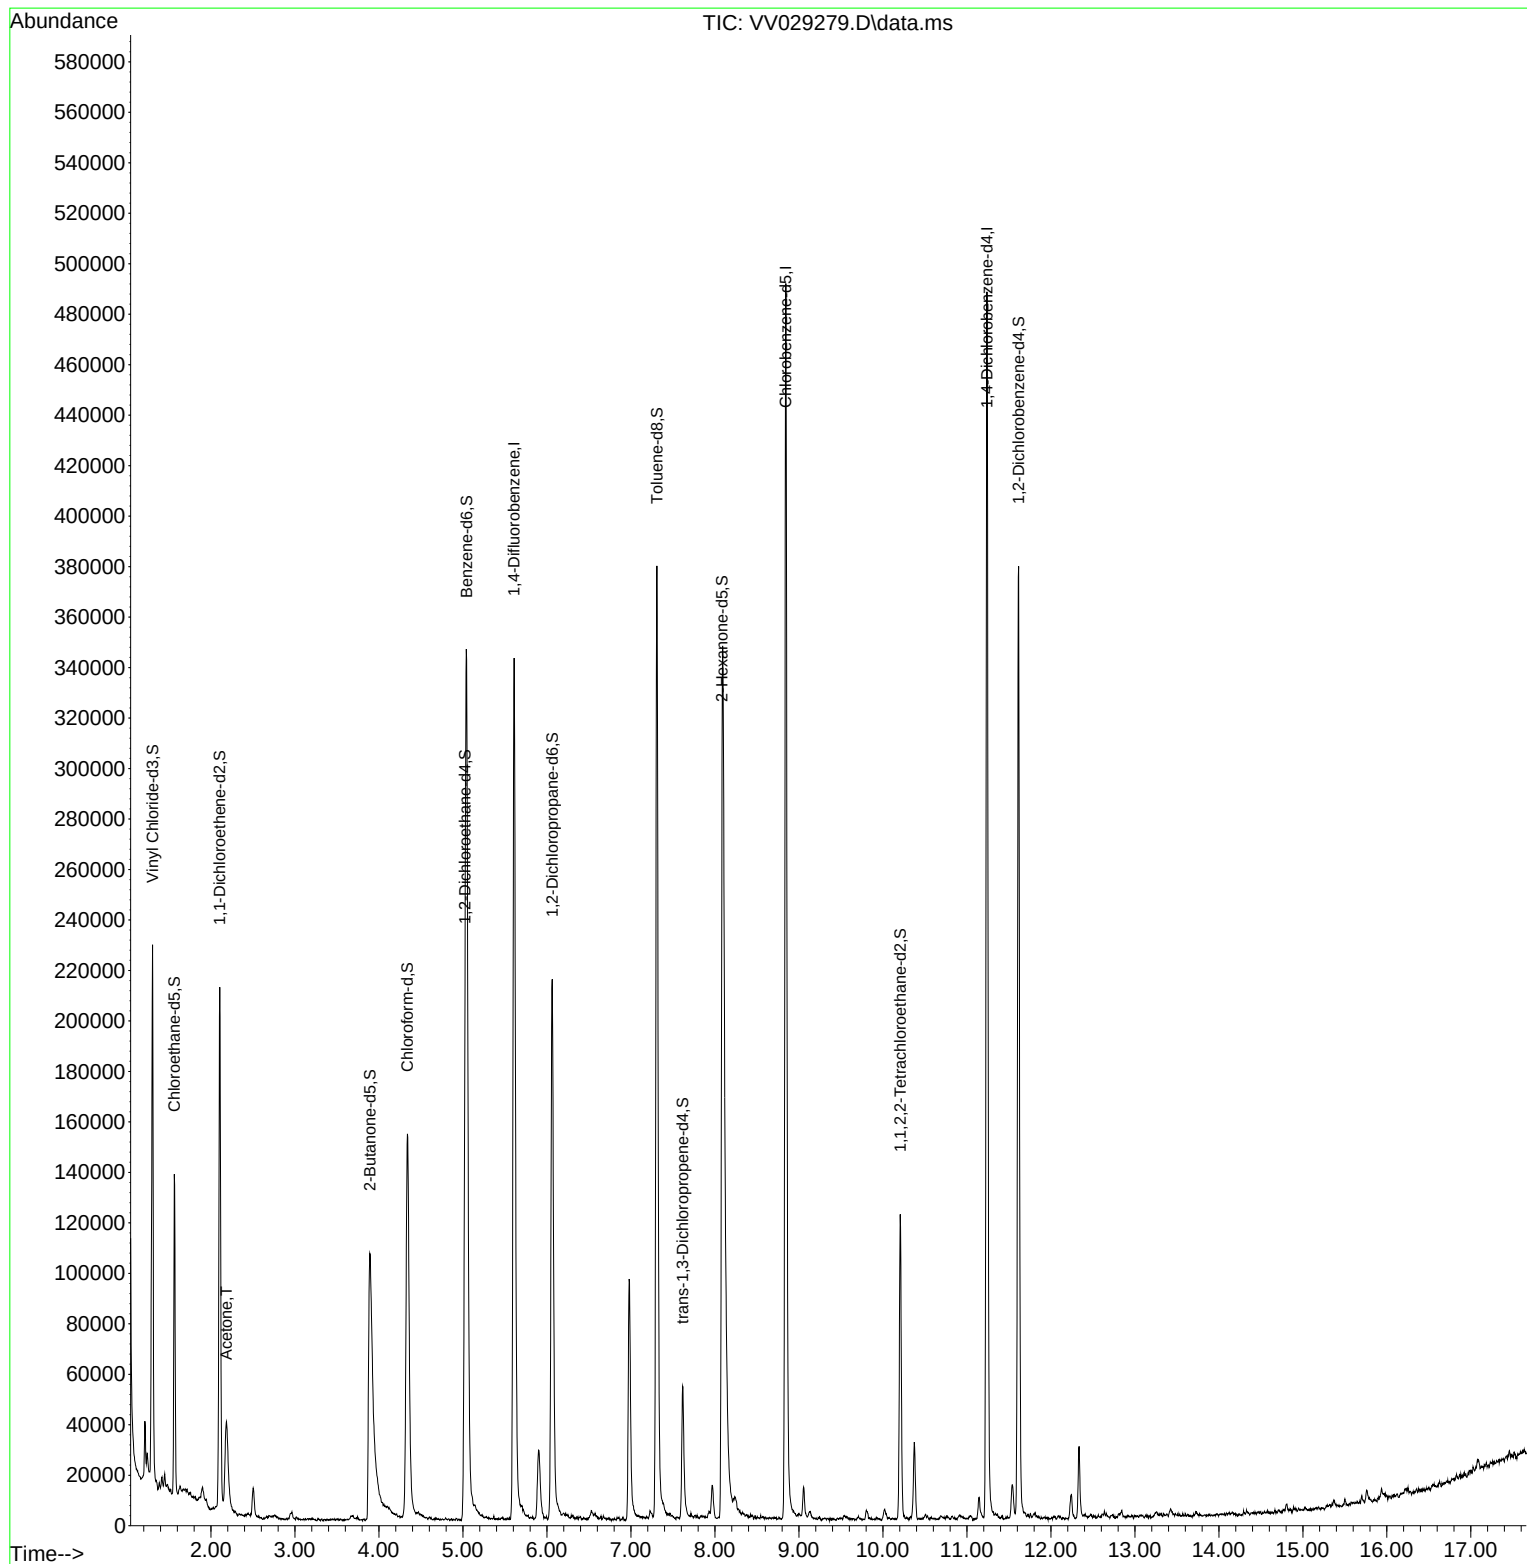

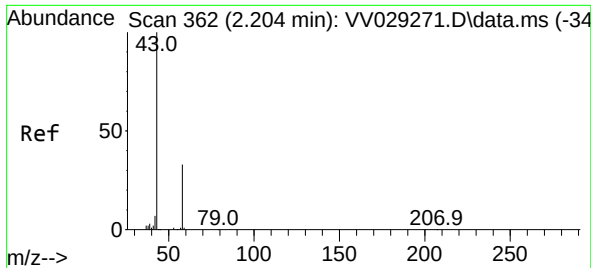

#13
 Acetone
 Concen: 17.189 ug/L
 RT: 2.182 min Scan# 31
 Delta R.T. -0.023 min
 Lab File: VV029279.D
 Acq: 22 Nov 2022 22:11

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1M7

Tgt Ion: 43 Resp: 59869
 Ion Ratio Lower Upper
 43 100
 58 34.8 0.0 65.2

