

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112222\
 Data File : VV029272.D
 Acq On : 22 Nov 2022 19:20
 Operator : SY/MD
 Sample : VV1122WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK274

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029272.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	50	54	58	rBV	20412	16558	1.35%	0.167%
2	1.301	71	81	94	rVB2	402710	560634	45.88%	5.670%
3	1.565	156	163	175	rVB	175430	199584	16.33%	2.019%
4	2.101	320	330	350	rBV	335916	487187	39.87%	4.927%
5	2.500	442	454	465	rBV	21952	37118	3.04%	0.375%
6	3.921	879	896	938	rBV2	65701	383270	31.36%	3.876%
7	4.339	1010	1026	1056	rBV	185798	480603	39.33%	4.861%
8	5.040	1227	1244	1272	rBV2	481277	1222030	100.00%	12.360%
9	5.609	1407	1421	1455	rBV	336726	711433	58.22%	7.196%
10	5.896	1498	1510	1526	rBV3	16656	38747	3.17%	0.392%
11	6.063	1544	1562	1581	rBV	273950	582320	47.65%	5.890%
12	6.979	1832	1847	1869	rBV	135553	265038	21.69%	2.681%
13	7.307	1936	1949	1981	rBV	586228	1056990	86.49%	10.691%
14	7.616	2034	2045	2065	rBV	76309	141404	11.57%	1.430%
15	8.095	2179	2194	2228	rBV6	377817	1004613	82.21%	10.161%
16	8.844	2415	2427	2452	rBV	477606	811452	66.40%	8.207%
17	10.207	2838	2851	2867	rBV	144397	233093	19.07%	2.358%
18	10.374	2893	2903	2914	rVB2	8753	14644	1.20%	0.148%
19	11.239	3160	3172	3192	rBV	476754	757133	61.96%	7.658%
20	11.612	3276	3288	3315	rBV	492288	796390	65.17%	8.055%
21	12.635	3595	3606	3618	rBV	6648	12668	1.04%	0.128%
22	13.252	3788	3798	3806	rBV5	9374	15959	1.31%	0.161%
23	13.490	3865	3872	3888	rVB	14615	27426	2.24%	0.277%
24	13.734	3936	3948	3956	rBV6	9635	16164	1.32%	0.163%
25	15.934	4625	4632	4643	rBV6	7690	14685	1.20%	0.149%




Sum of corrected areas: 9887143

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112222\
Data File : VV029272.D
Acq On : 22 Nov 2022 19:20
Operator : SY/MD
Sample : VV1122WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK274

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

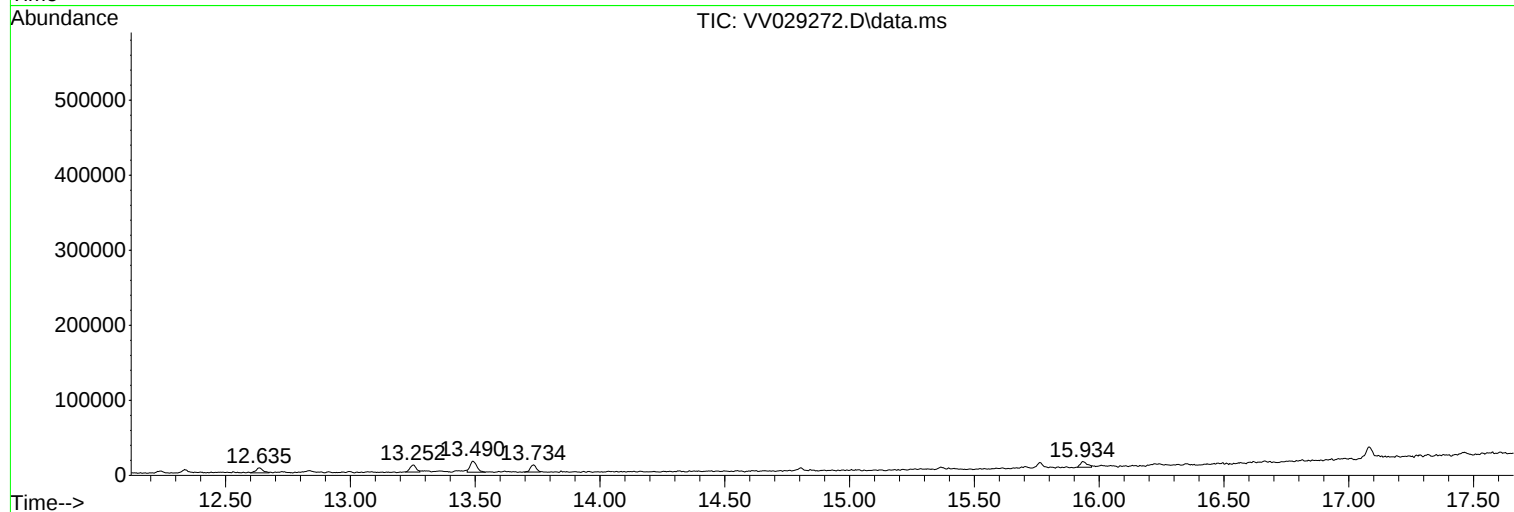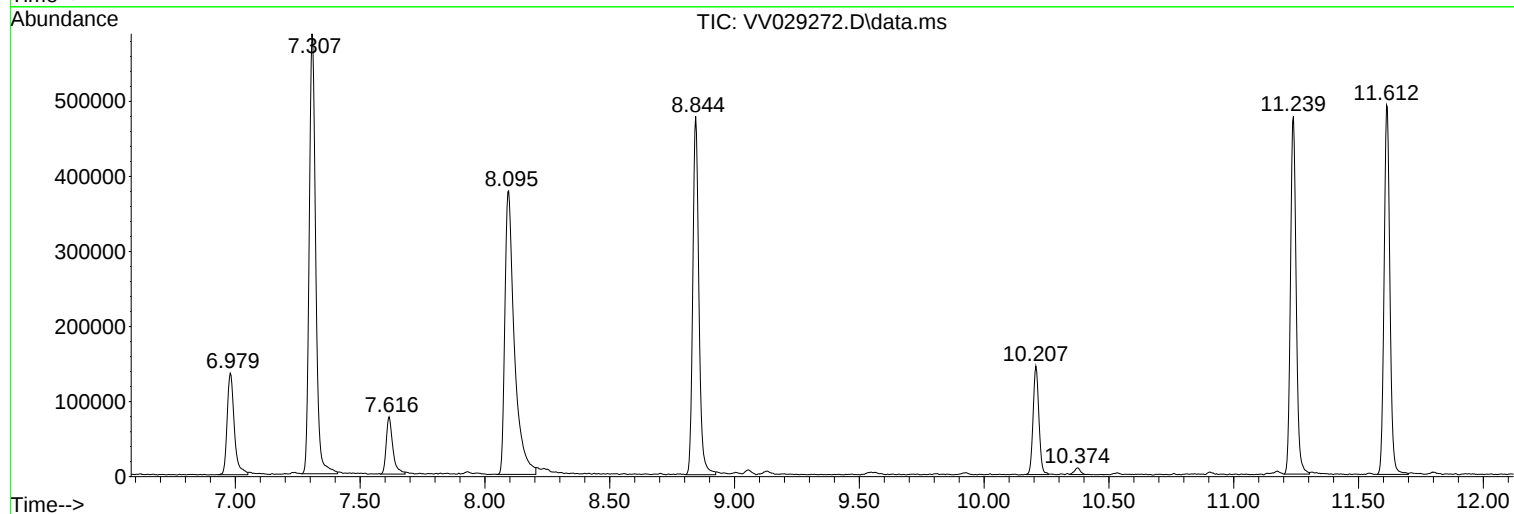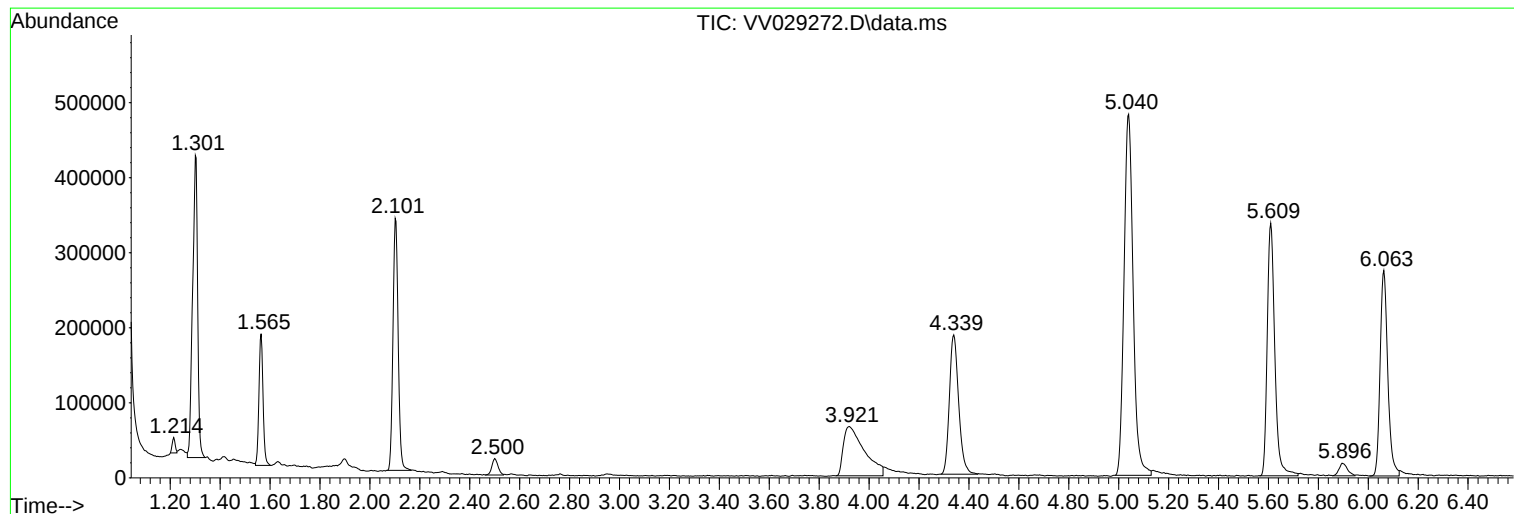

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112222\
Data File : VV029272.D
Acq On : 22 Nov 2022 19:20
Operator : SY/MD
Sample : VV1122WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK274

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112222\
Data File : VV029272.D
Acq On : 22 Nov 2022 19:20
Operator : SY/MD
Sample : VV1122WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK274

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
