

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112222\
 Data File : VV029273.D
 Acq On : 22 Nov 2022 19:44
 Operator : SY/MD
 Sample : VV1122WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK275

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029273.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	49	54	59	rBV	22377	21810	1.80%	0.220%
2	1.301	72	81	94	rVB2	380183	519082	42.83%	5.230%
3	1.564	156	163	177	rVB	176042	199748	16.48%	2.012%
4	2.101	320	330	351	rVB	344741	508851	41.98%	5.127%
5	2.500	443	454	467	rBV	35940	61072	5.04%	0.615%
6	3.918	880	895	955	rBV4	73434	449394	37.08%	4.528%
7	4.339	1005	1026	1054	rBV	187945	487091	40.19%	4.908%
8	5.040	1222	1244	1265	rBV2	483277	1211993	100.00%	12.211%
9	5.609	1405	1421	1444	rBV	345635	729492	60.19%	7.350%
10	5.899	1499	1511	1524	rBV2	16033	37325	3.08%	0.376%
11	6.063	1544	1562	1583	rBV	275424	578680	47.75%	5.830%
12	6.979	1832	1847	1873	rBV	129416	251943	20.79%	2.538%
13	7.307	1937	1949	1976	rBV	586960	1056519	87.17%	10.645%
14	7.616	2033	2045	2062	rBV	71005	130934	10.80%	1.319%
15	8.095	2178	2194	2233	rBV6	372232	1009796	83.32%	10.174%
16	8.844	2414	2427	2453	rBV	495251	838105	69.15%	8.444%
17	10.207	2838	2851	2869	rBV	144669	235466	19.43%	2.372%
18	11.239	3160	3172	3191	rBV	509161	791638	65.32%	7.976%
19	11.612	3274	3288	3316	rBV	496261	806429	66.54%	8.125%




Sum of corrected areas: 9925368

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112222\
Data File : VV029273.D
Acq On : 22 Nov 2022 19:44
Operator : SY/MD
Sample : VV1122WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK275

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

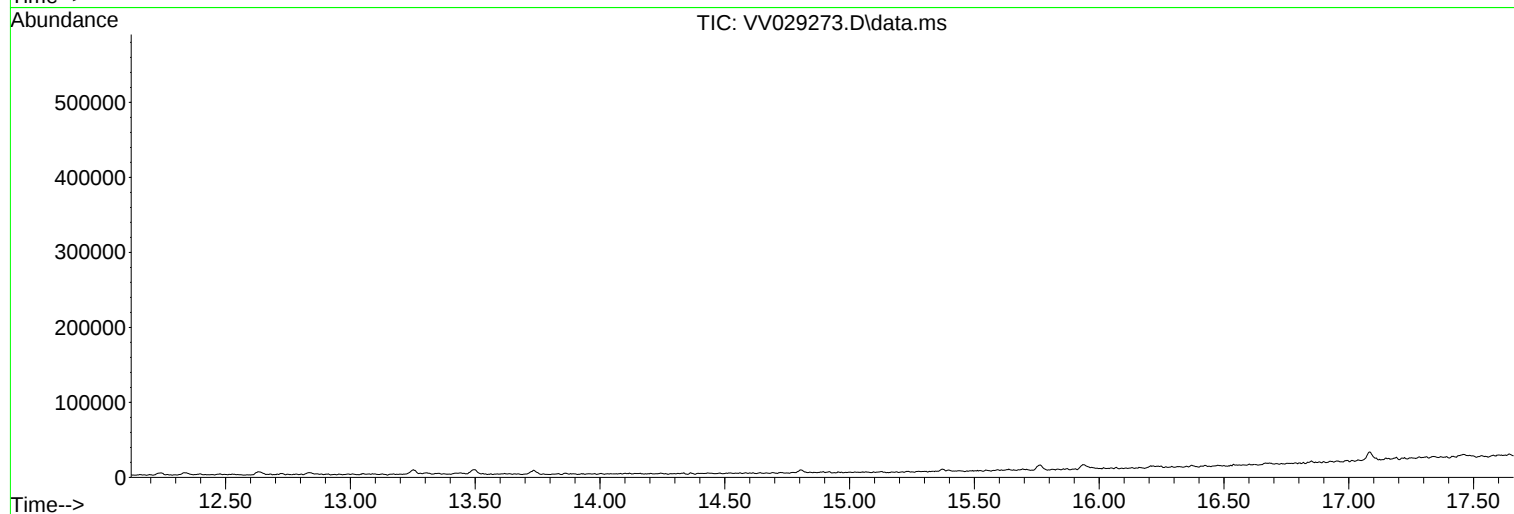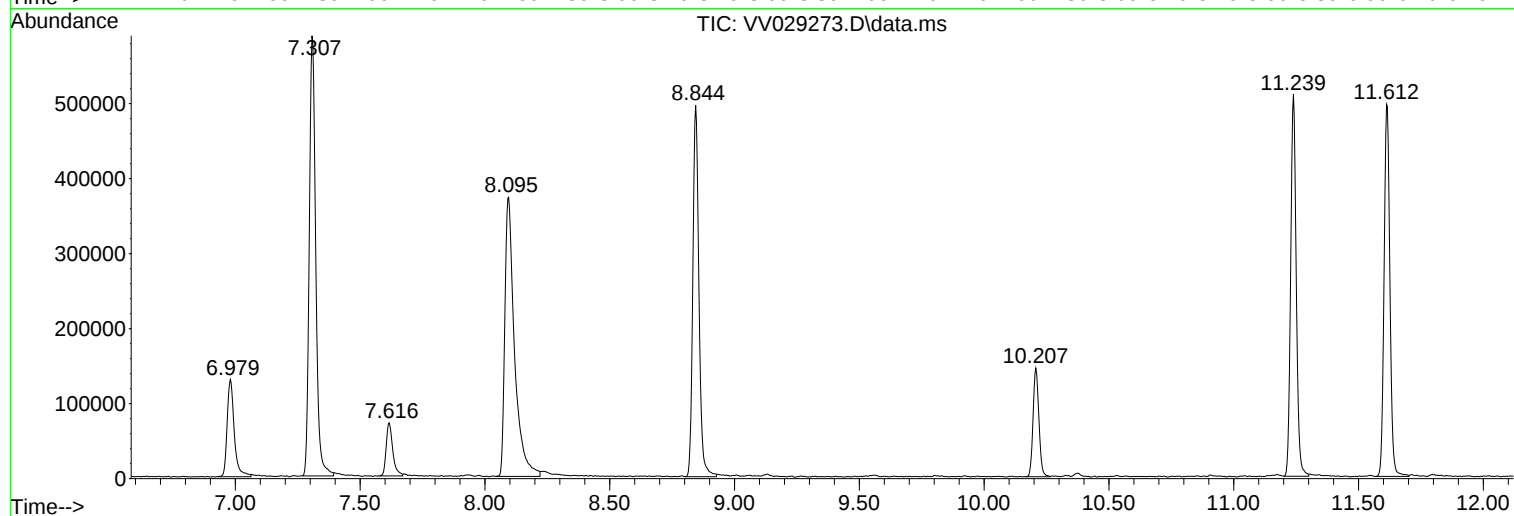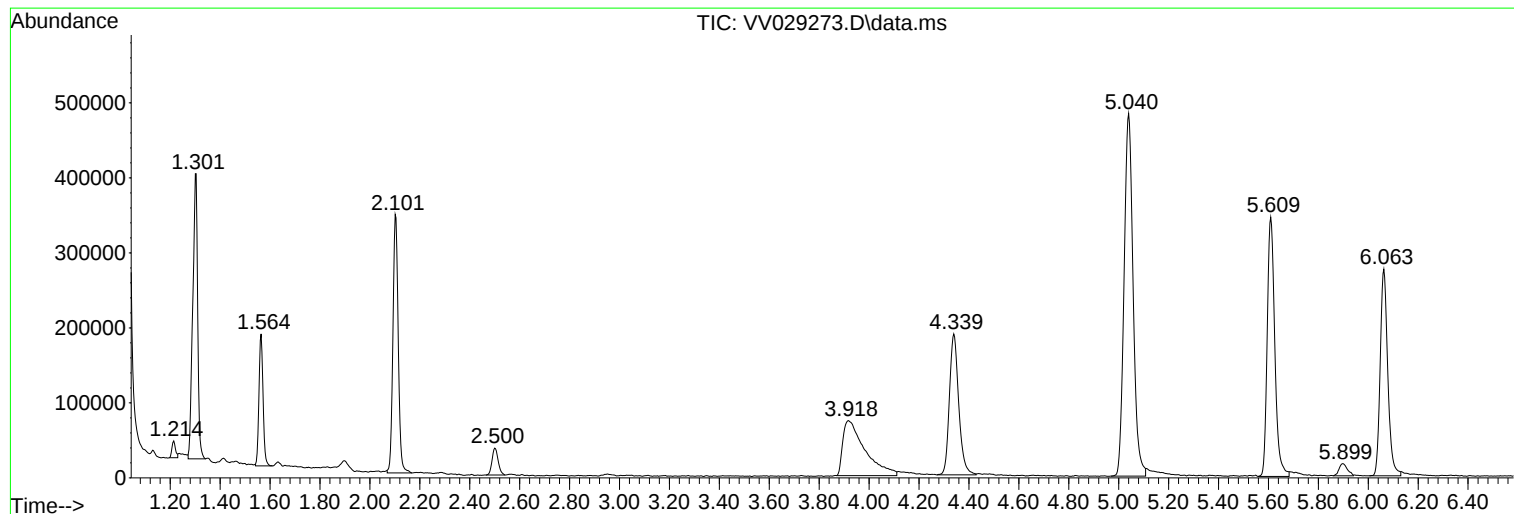

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112222\
Data File : VV029273.D
Acq On : 22 Nov 2022 19:44
Operator : SY/MD
Sample : VV1122WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK275

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112222\
Data File : VV029273.D
Acq On : 22 Nov 2022 19:44
Operator : SY/MD
Sample : VV1122WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK275

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc