

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112222\
 Data File : VV029275.D
 Acq On : 22 Nov 2022 20:33
 Operator : SY/MD
 Sample : N5648-02DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H46C6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029275.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	49	54	59	rBV	34034	30539	2.20%	0.285%
2	1.304	72	82	93	rVB3	323382	422333	30.45%	3.945%
3	1.565	156	163	176	rVB	129654	146025	10.53%	1.364%
4	2.101	321	330	349	rVB	224225	330855	23.85%	3.090%
5	2.500	440	454	469	rBV	51030	88692	6.39%	0.828%
6	2.764	522	536	561	rBV2	74803	171614	12.37%	1.603%
7	3.902	872	890	942	rBV2	437355	1387151	100.00%	12.956%
8	4.339	1011	1026	1052	rBV	149569	390091	28.12%	3.643%
9	5.040	1225	1244	1282	rBV2	364884	955274	68.87%	8.922%
10	5.609	1408	1421	1444	rBV	359415	737706	53.18%	6.890%
11	5.905	1496	1513	1538	rBV	526184	1075542	77.54%	10.045%
12	6.063	1549	1562	1588	rBV	217181	452266	32.60%	4.224%
13	6.979	1834	1847	1876	rBV	101590	199876	14.41%	1.867%
14	7.307	1935	1949	1983	rBV	406098	739018	53.28%	6.902%
15	7.616	2033	2045	2065	rBV	56730	106220	7.66%	0.992%
16	8.092	2178	2193	2230	rBV4	366619	974286	70.24%	9.100%
17	8.844	2415	2427	2452	rBV	500397	850383	61.30%	7.942%
18	10.207	2840	2851	2868	rBV	134989	216889	15.64%	2.026%
19	11.239	3159	3172	3189	rBV	514210	798973	57.60%	7.462%
20	11.612	3277	3288	3308	rBV	388411	633043	45.64%	5.913%




Sum of corrected areas: 10706776

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112222\
Data File : VV029275.D
Acq On : 22 Nov 2022 20:33
Operator : SY/MD
Sample : N5648-02DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46C6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

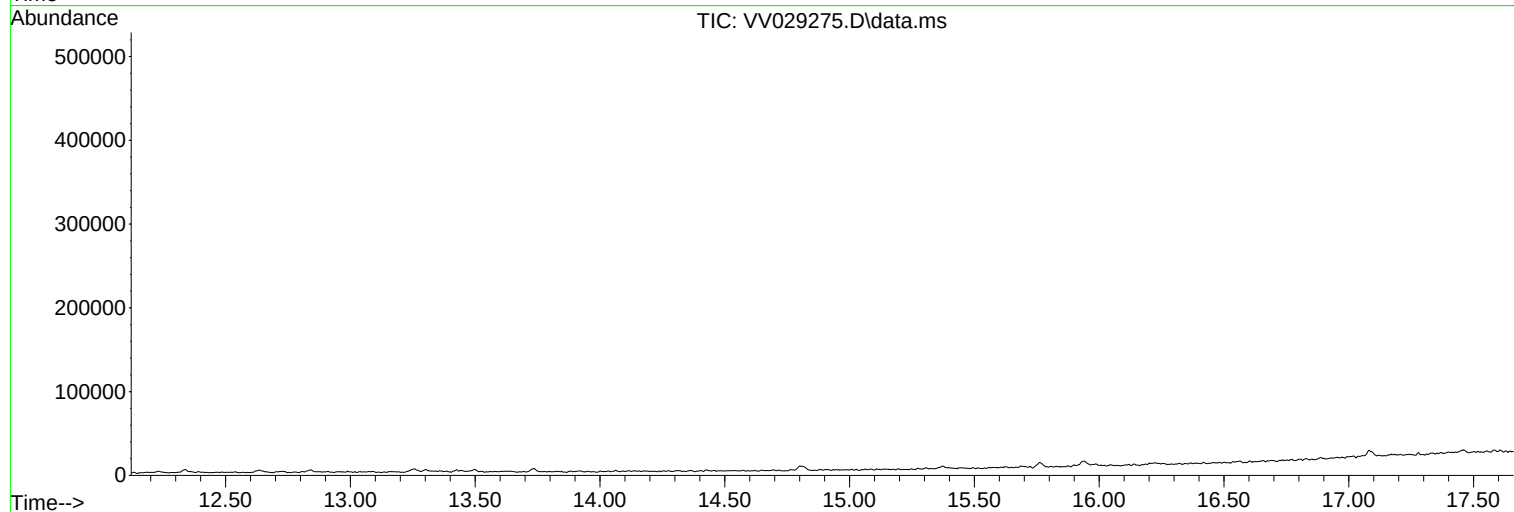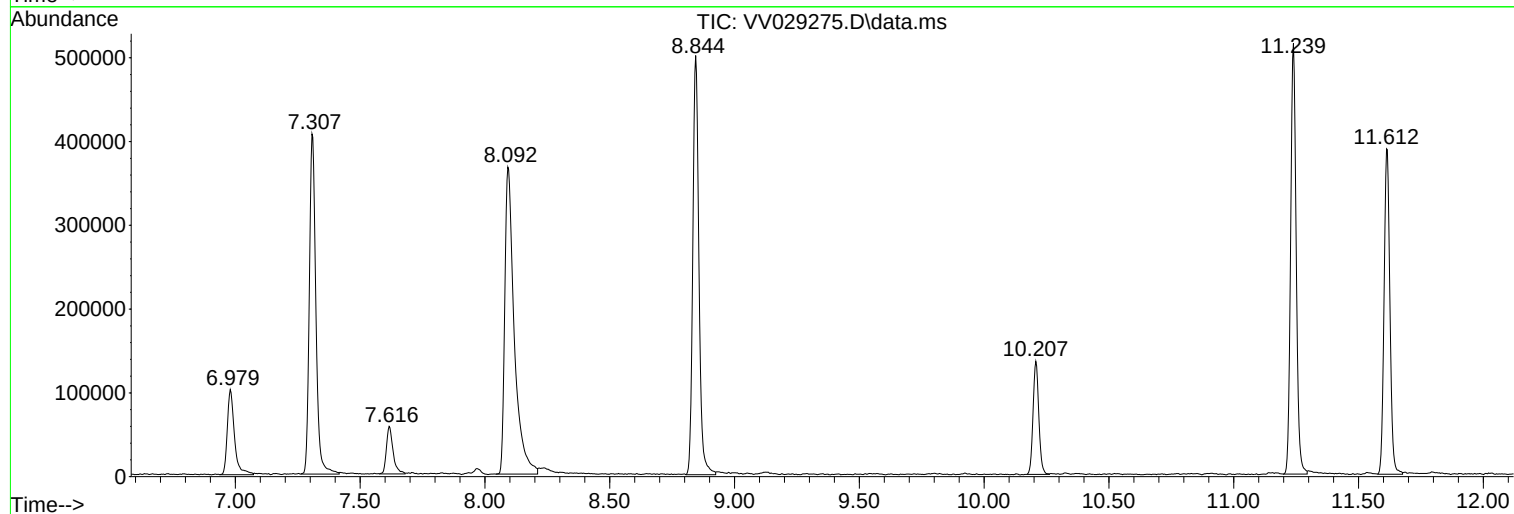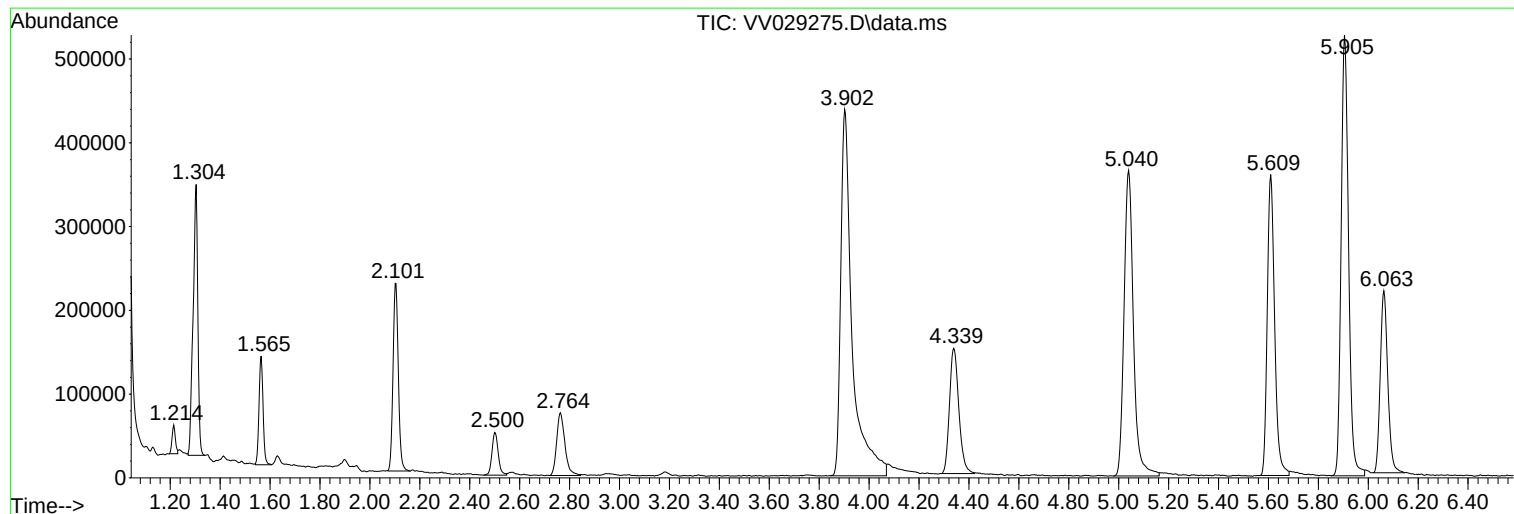

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112222\
Data File : VV029275.D
Acq On : 22 Nov 2022 20:33
Operator : SY/MD
Sample : N5648-02DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46C6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112222\
Data File : VV029275.D
Acq On : 22 Nov 2022 20:33
Operator : SY/MD
Sample : N5648-02DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46C6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc