

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
 Data File : VV038282.D
 Acq On : 22 Nov 2024 21:07
 Operator : SY/MD
 Sample : VV1122WBL02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK261

Quant Time: Nov 23 02:05:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 23 02:01:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	240203	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	257793	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	108726	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	72995	3.965	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.200%
7) Chloroethane-d5	1.529	69	70313	4.721	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.400%
11) 1,1-Dichloroethene-d2	2.053	65	33936	4.283	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	85.600%
20) 2-Butanone-d5	3.793	46	171731	46.627	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.260%
24) Chloroform-d	4.243	84	165295	4.626	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.600%
26) 1,2-Dichloroethane-d4	4.937	65	79047	4.930	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.600%
32) Benzene-d6	4.953	84	291710	4.378	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.600%
36) 1,2-Dichloropropane-d6	5.982	67	95512	4.659	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.200%
41) Toluene-d8	7.240	98	222103	3.603	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.000%
43) trans-1,3-Dichloroprop...	7.558	79	30932	4.058	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.200%
46) 2-Hexanone-d5	8.021	63	126559	42.713	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.420%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	81526	4.684	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.600%
66) 1,2-Dichlorobenzene-d4	11.554	152	91458	4.937	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.800%
Target Compounds					Qvalue	
47) Tetrachloroethene	7.905	164	5240	0.330	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038282.D
Acq On : 22 Nov 2024 21:07
Operator : SY/MD
Sample : VV1122WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK261


Quant Time: Nov 23 02:05:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 23 02:01:29 2024
Response via : Initial Calibration

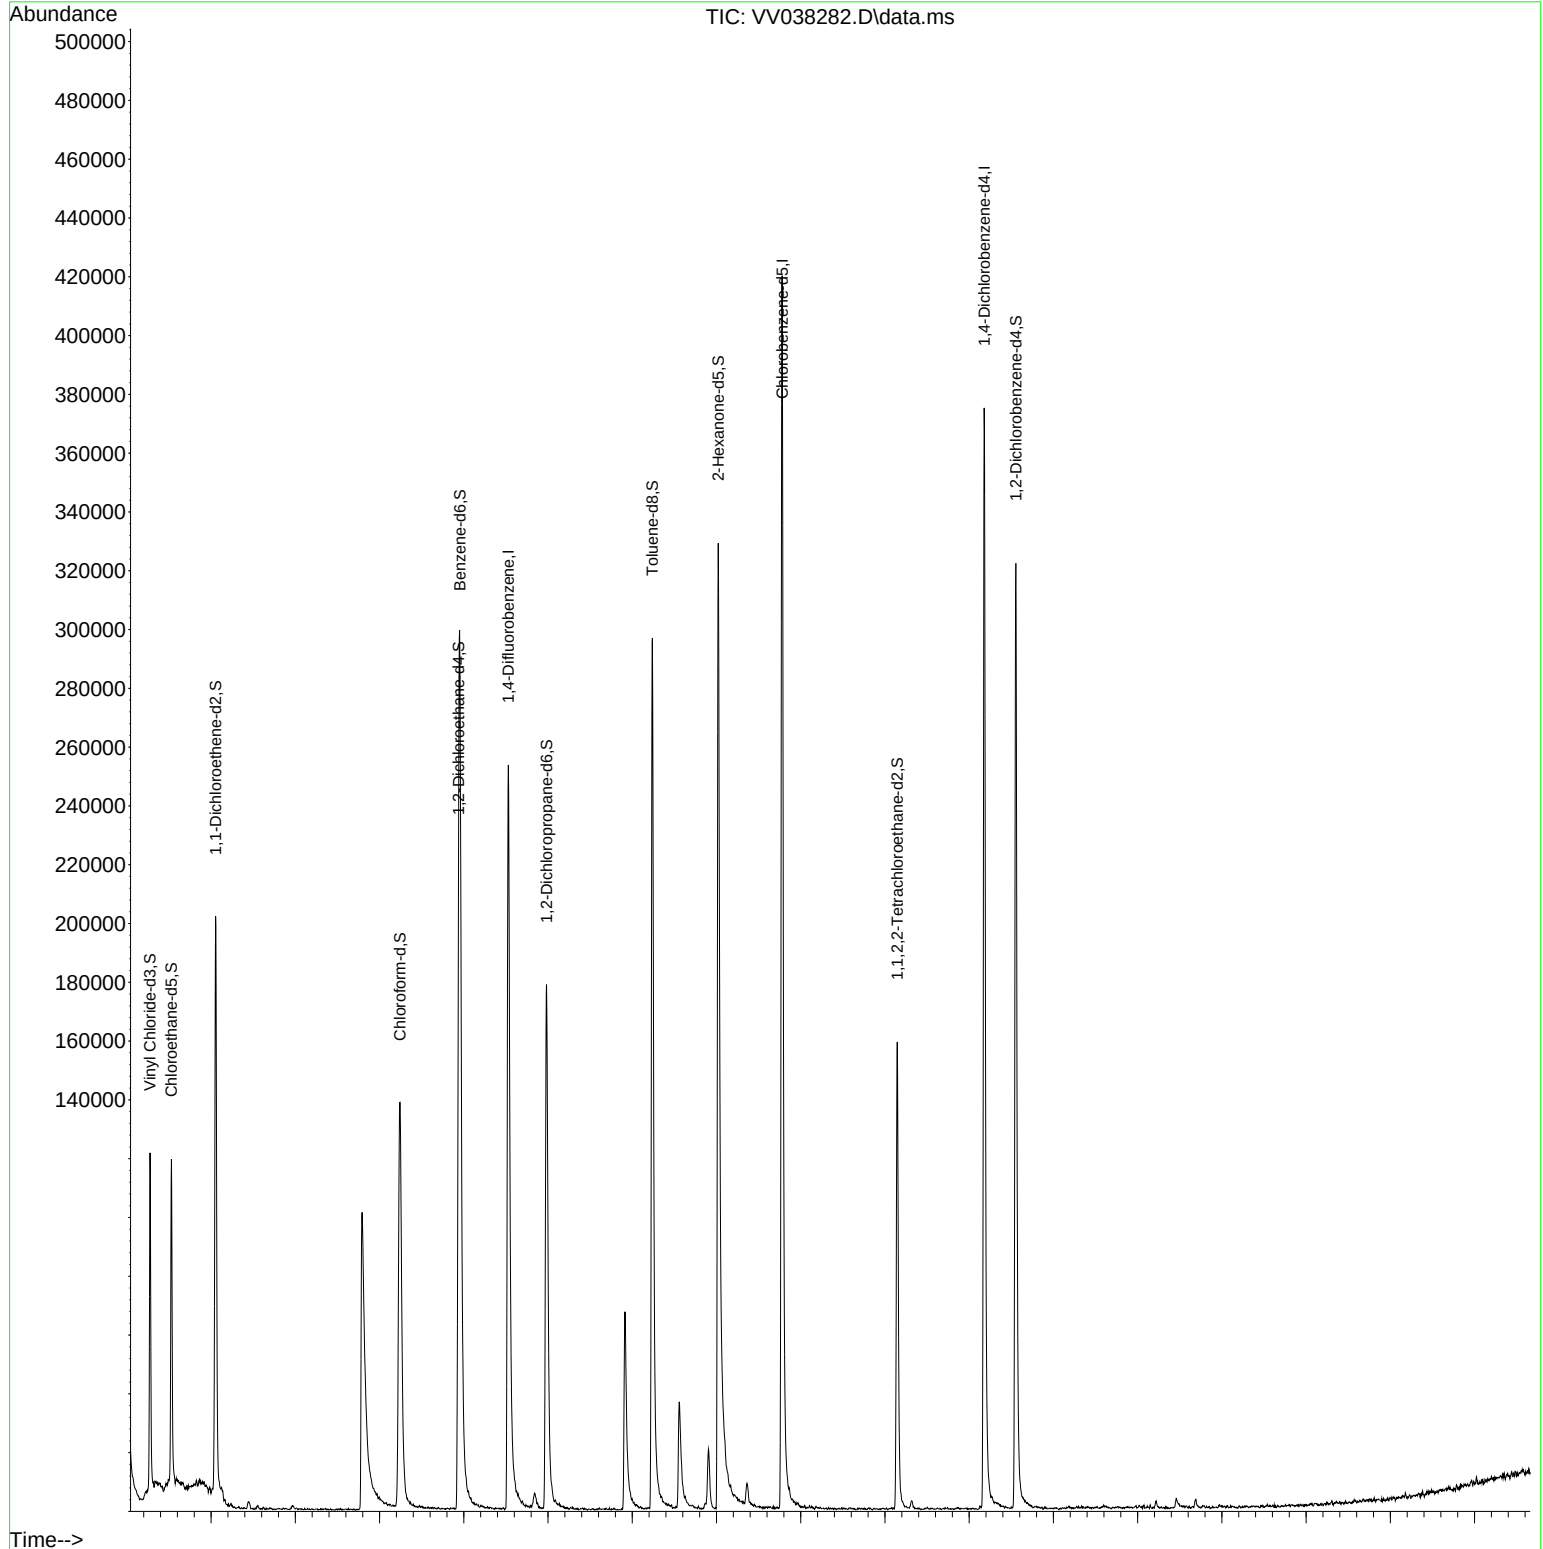

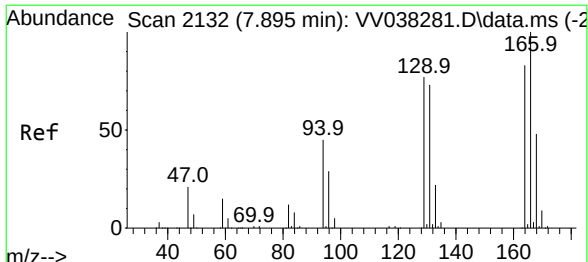

#47
 Tetrachloroethene
 Concen: 0.330 ug/L
 RT: 7.905 min Scan# 21
 Delta R.T. 0.010 min
 Lab File: VV038282.D
 Acq: 22 Nov 2024 21:07

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK261

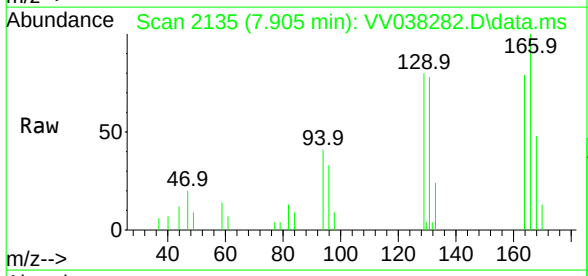

Tgt Ion:164 Resp: 5240

Ion	Ratio	Lower	Upper
164	100		
129	100.3	68.5	127.1
131	98.4	64.8	120.4
166	125.9	88.3	163.9

